

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0102418\
 Data File : P0050501.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2018 23:58
 Operator : SM/SJ
 Sample : J5198-27
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-01-102318-D

Manual Integrations
 APPROVED

Sohil
 10/25/2018 2:00:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:12:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0101818.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 19 02:02:26 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.358	3.354	6802821	5554100	22.798m	28.251
2)	SA Decachlor...	10.020	8.103	4058353	2839972	18.703m	14.858m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO102418\
Data File : PO050501.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2018 23:58
Operator : SM/SJ
Sample : J5198-27
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-01-102318-D


Manual Integrations
APPROVED

Sohil
10/25/2018 2:00:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:12:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO101818.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 19 02:02:26 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

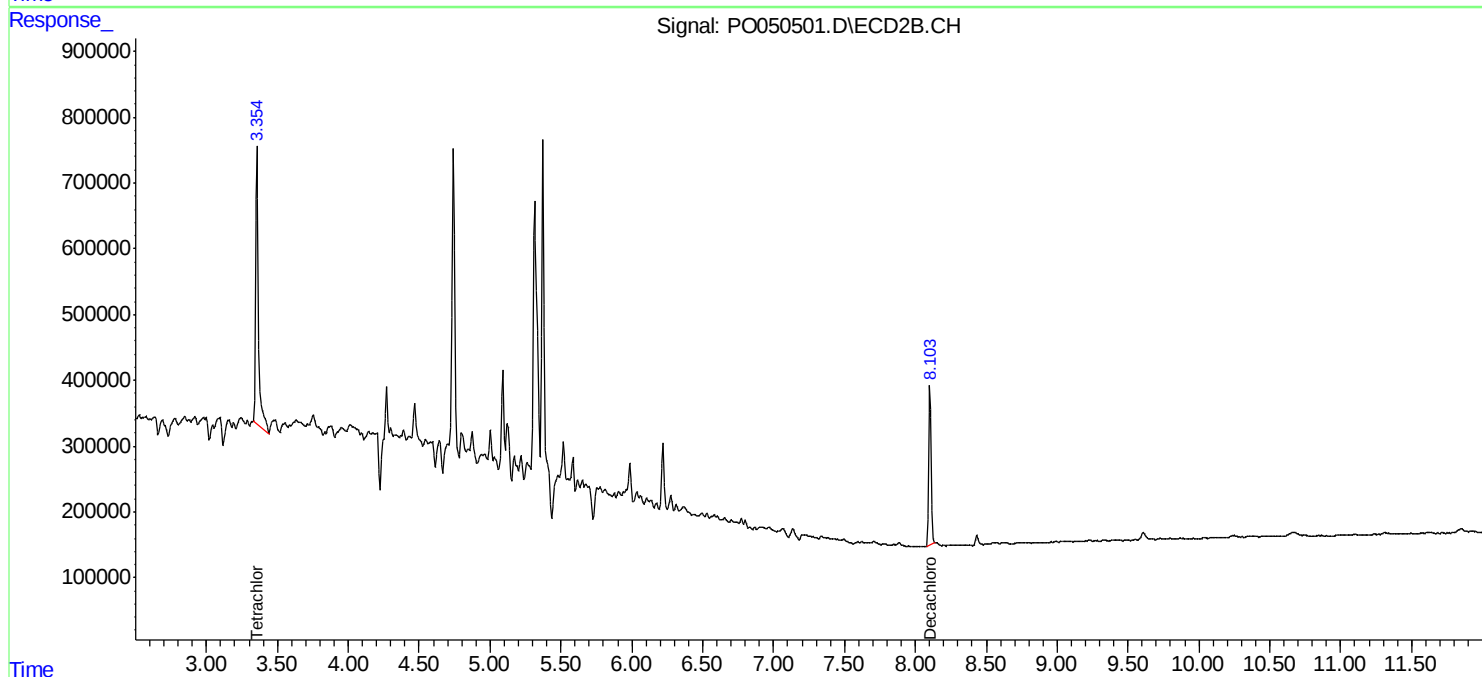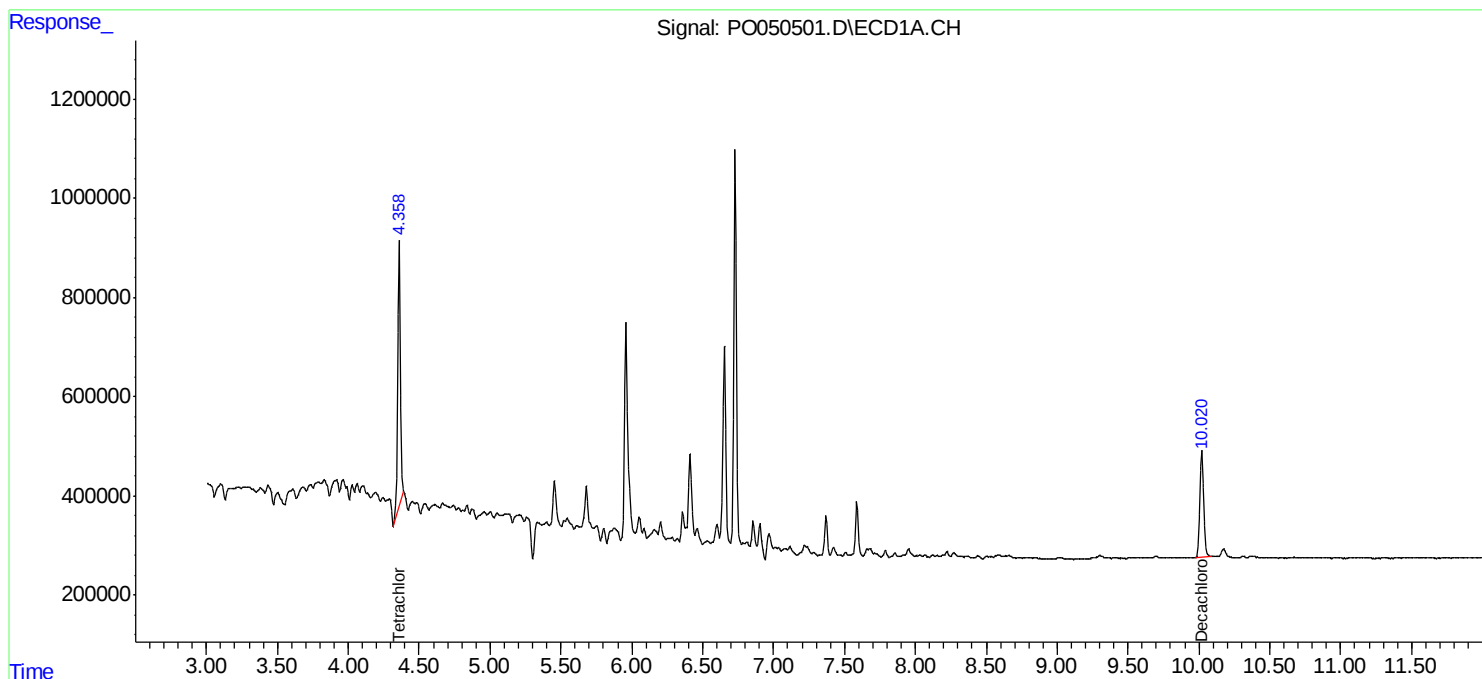

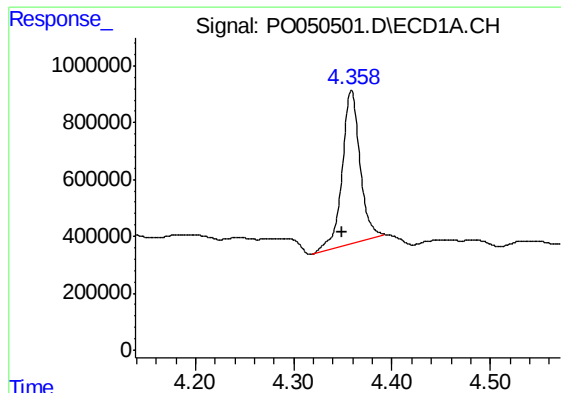


#1 Tetrachloro-m-xylene

R.T.: 4.358 min
Delta R.T.: 0.009 min
Response: 6802821
Conc: 22.80 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-01-102318-D


Manual Integrations
APPROVED

Sohil
10/25/2018 2:00:03 PM

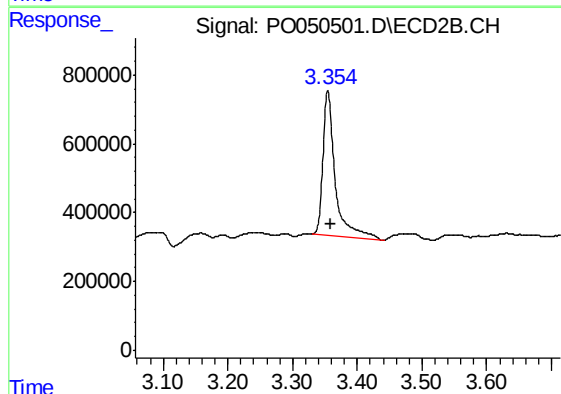


#1 Tetrachloro-m-xylene

R.T.: 3.354 min
Delta R.T.: -0.005 min
Response: 5554100
Conc: 28.25 ng/ml

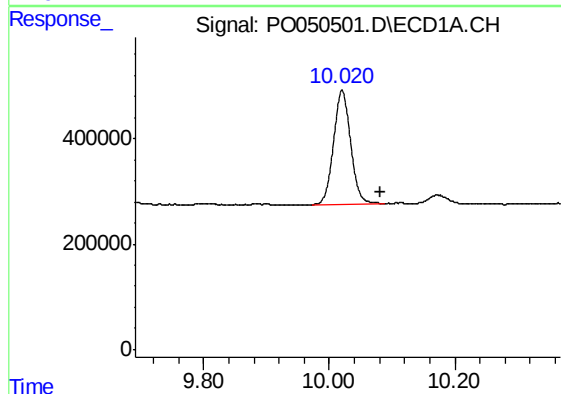

#2 Decachlorobiphenyl

R.T.: 10.020 min
Delta R.T.: -0.061 min
Response: 4058353
Conc: 18.70 ng/ml m

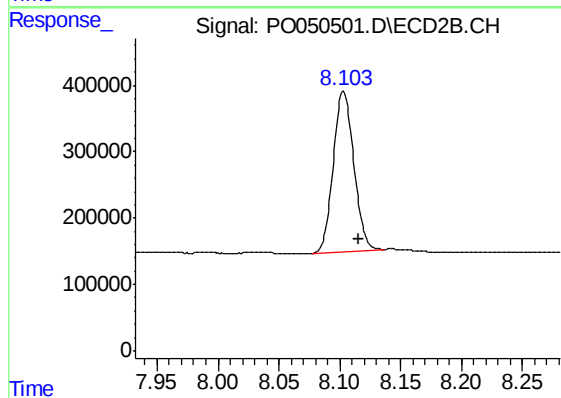

#2 Decachlorobiphenyl

R.T.: 8.103 min
Delta R.T.: -0.014 min
Response: 2839972
Conc: 14.86 ng/ml m