

Data Path : P:\HPCHEM1\ECD 0\Data\P0010218\
Data File : P0041001.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jan 2018 11:15
Operator : SM/UA
Sample : I7064-07
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SAMPLE-4

Manual Integrations
APPROVED

UGO
1/3/2018 10:22:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 11:44:55 2018
Quant Method : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\methods\P0122017.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 20 03:23:29 2017
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.135	3.374	3923686	5357987	18.922	17.383
2)	SA Decachlor...	9.551	8.181	2708190	4128259	13.225m	11.657m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0010218\
Data File : P0041001.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jan 2018 11:15
Operator : SM/UA
Sample : I7064-07
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SAMPLE-4


Manual Integrations
APPROVED

UGO
1/3/2018 10:22:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 02 11:44:55 2018
Quant Method : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\methods\P0122017.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 20 03:23:29 2017
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

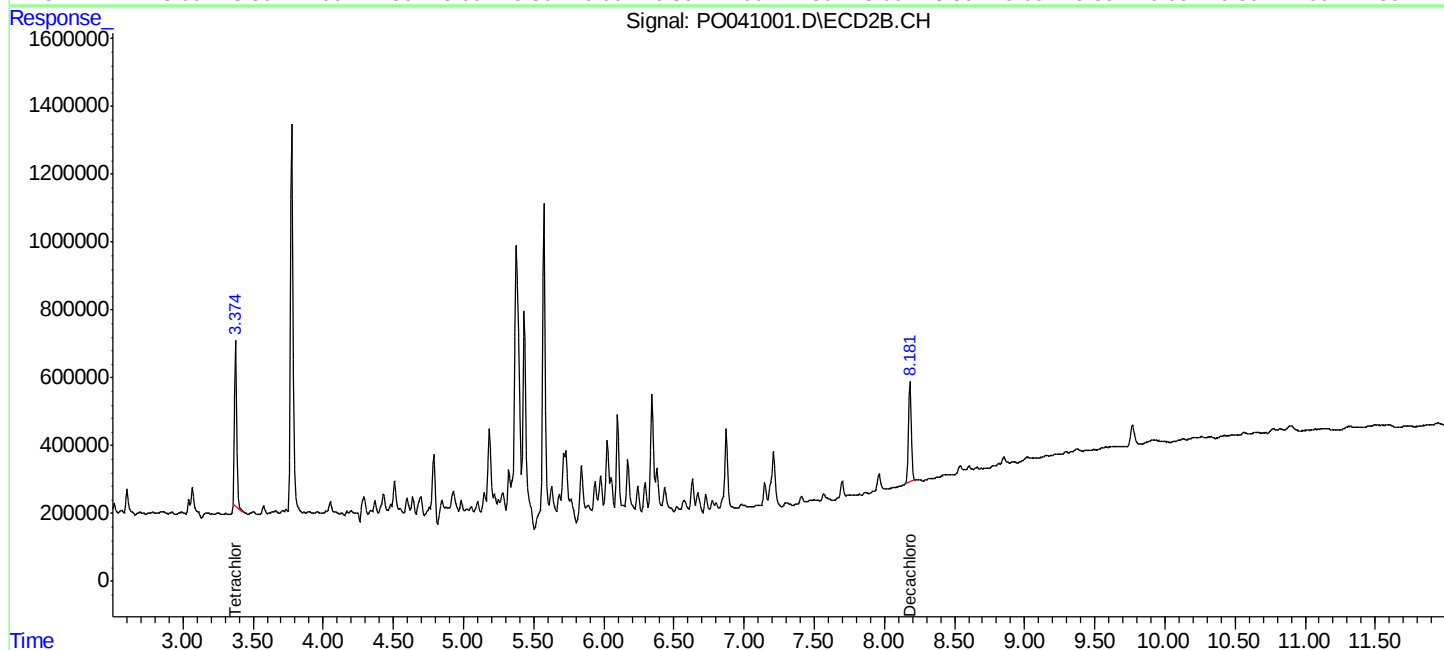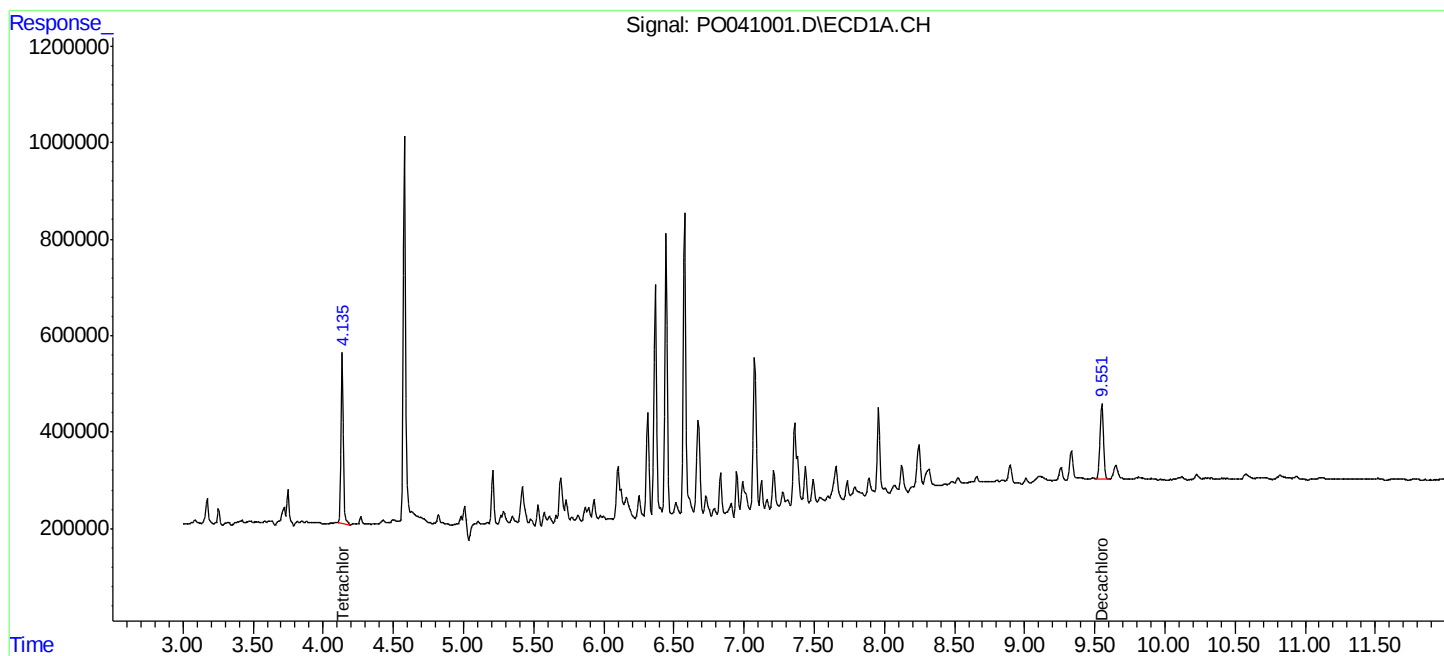

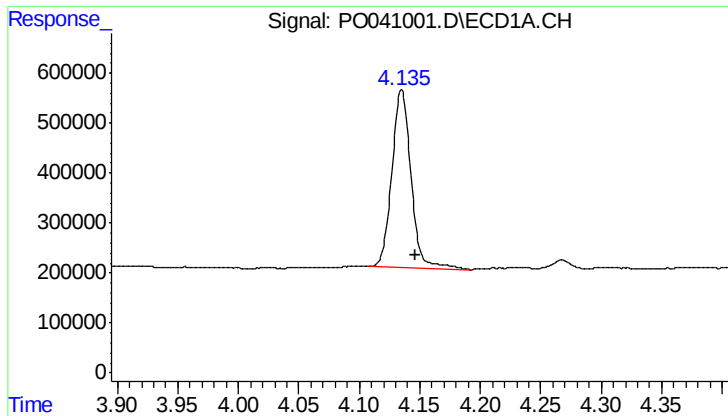


#1 Tetrachloro-m-xylene

R.T.: 4.135 min
Delta R.T.: -0.011 min
Response: 3923686
Conc: 18.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
SAMPLE-4


Manual Integrations
APPROVED

UGO
1/3/2018 10:22:01 AM

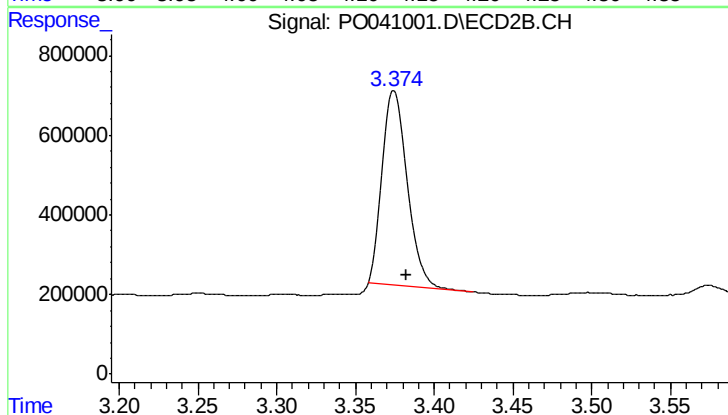


#1 Tetrachloro-m-xylene

R.T.: 3.374 min
Delta R.T.: -0.008 min
Response: 5357987
Conc: 17.38 ng/ml

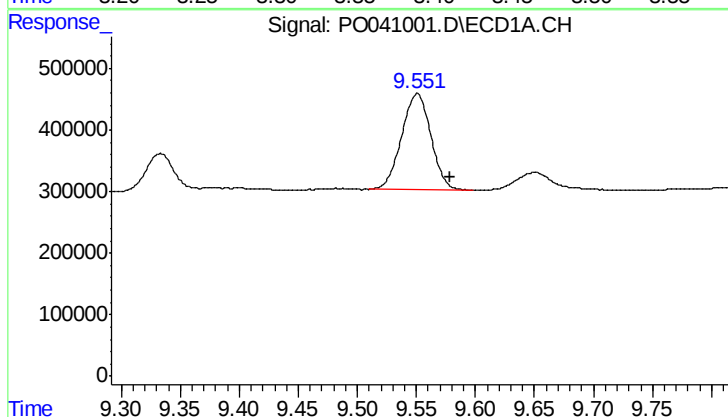

#2 Decachlorobiphenyl

R.T.: 9.551 min
Delta R.T.: -0.028 min
Response: 2708190
Conc: 13.23 ng/ml m

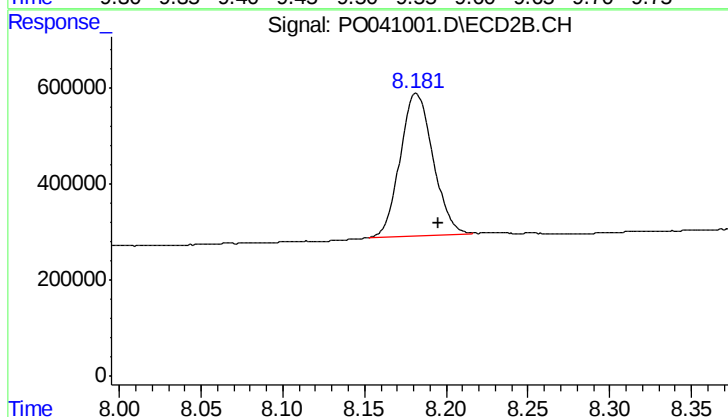

#2 Decachlorobiphenyl

R.T.: 8.181 min
Delta R.T.: -0.014 min
Response: 4128259
Conc: 11.66 ng/ml m