

Data Path : P:\HPCHEM1\ECD 0\Data\P0010218\
 Data File : P0041008.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jan 2018 14:01
 Operator : SM/UA
 Sample : I7095-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DRUMS-1-4

Manual Integrations
 APPROVED

UGO
 1/3/2018 10:22:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 01:02:52 2018
 Quant Method : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\methods\P0122017.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 20 03:23:29 2017
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.137	3.379	2499102	3423960	12.052	11.108
2) SA Decachlor...	9.554	8.182	1876519	2107429	9.164	5.951m#

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0010218\
Data File : P0041008.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jan 2018 14:01
Operator : SM/UA
Sample : I7095-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DRUMS-1-4


Manual Integrations
APPROVED

UGO
1/3/2018 10:22:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 01:02:52 2018
Quant Method : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\methods\P0122017.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 20 03:23:29 2017
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

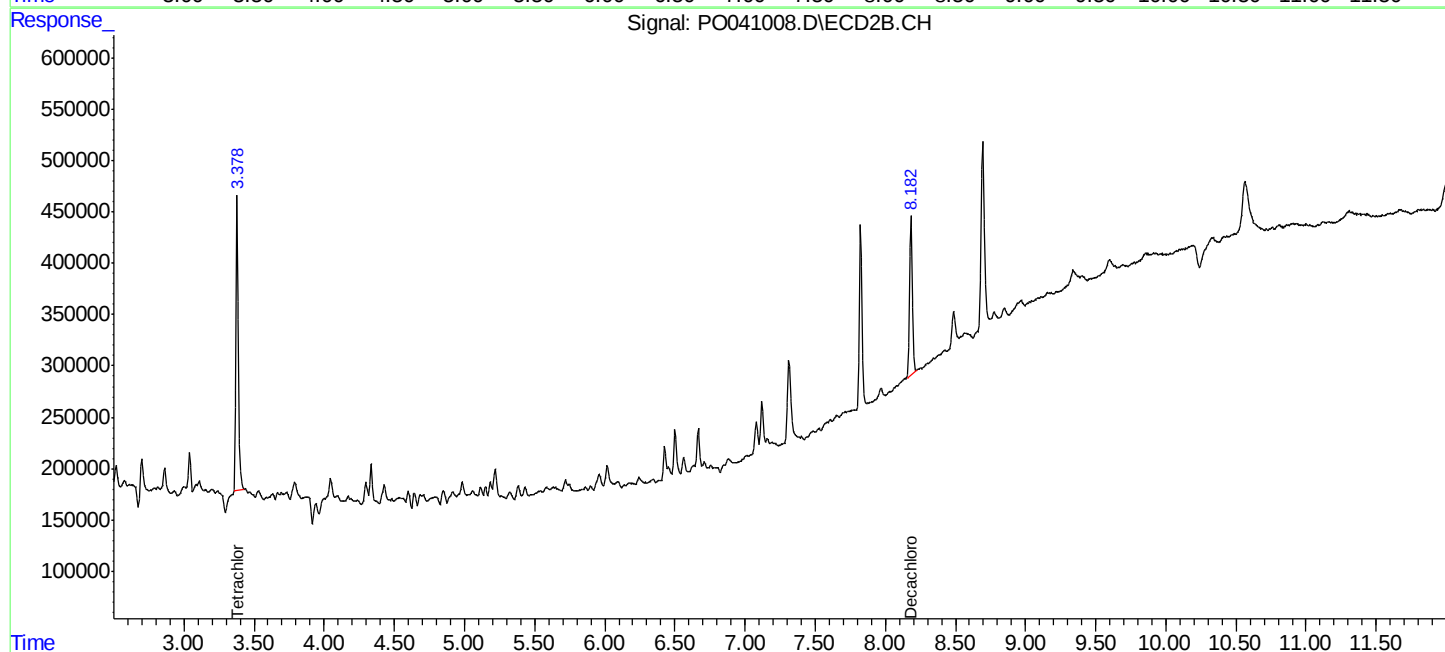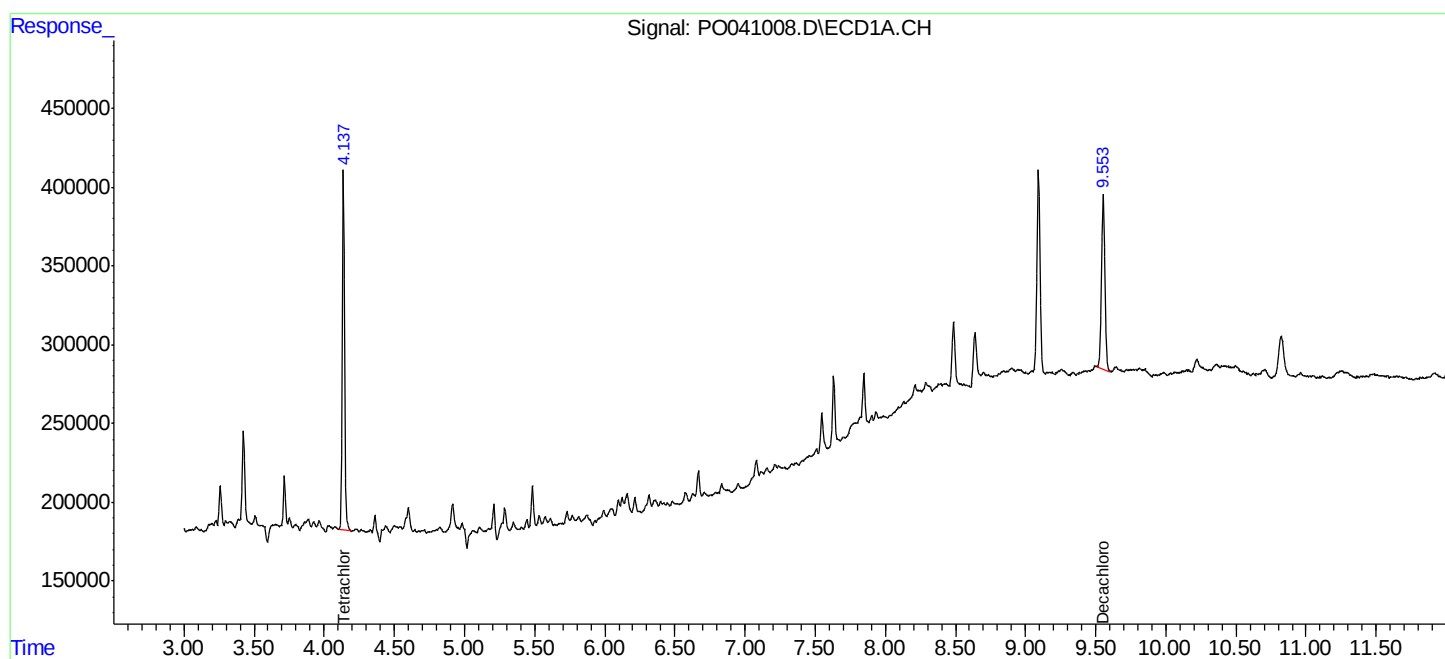

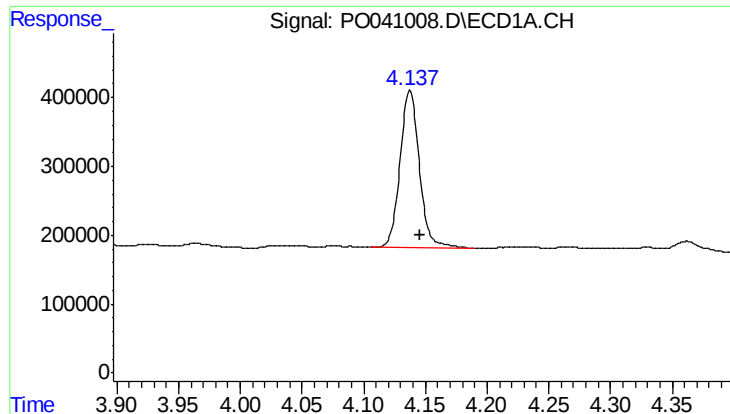


#1 Tetrachloro-m-xylene

R.T.: 4.137 min
Delta R.T.: -0.009 min
Response: 2499102
Conc: 12.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRUMS-1-4


Manual Integrations
APPROVED

UGO
1/3/2018 10:22:35 AM

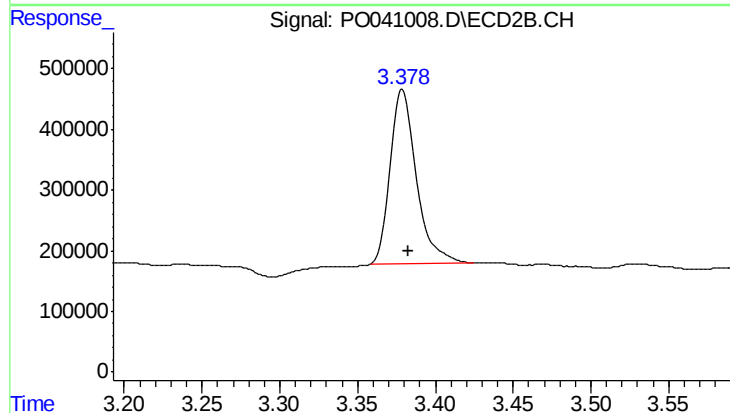


#1 Tetrachloro-m-xylene

R.T.: 3.379 min
Delta R.T.: -0.004 min
Response: 3423960
Conc: 11.11 ng/ml

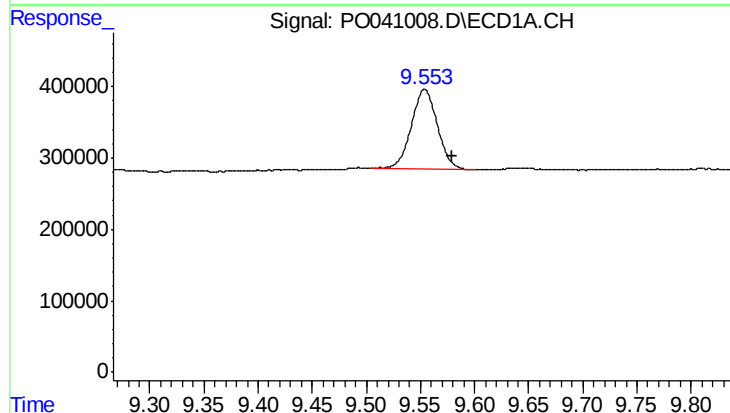

#2 Decachlorobiphenyl

R.T.: 9.554 min
Delta R.T.: -0.025 min
Response: 1876519
Conc: 9.16 ng/ml

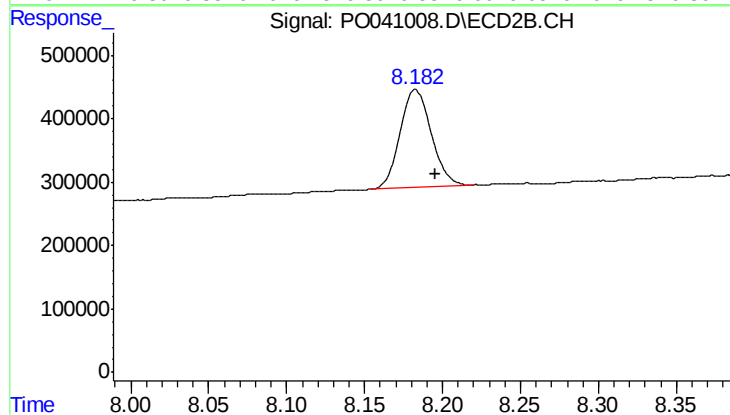

#2 Decachlorobiphenyl

R.T.: 8.182 min
Delta R.T.: -0.013 min
Response: 2107429
Conc: 5.95 ng/ml m