

Data Path : P:\HPCHEM1\ECD 0\Data\P0010218\
 Data File : P0041012.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jan 2018 15:15
 Operator : SM/UA
 Sample : I7091-01RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-CHRT25337RE

Manual Integrations
 APPROVED

UGO
 1/3/2018 10:22:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 03 00:50:59 2018
 Quant Method : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\methods\P0122017.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 20 03:23:29 2017
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.141	3.384	1459482	1983632	7.039	6.436m
2) SA Decachlor...	9.562	8.189	1652740	1404679	8.071m	3.966 #

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0010218\
Data File : P0041012.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jan 2018 15:15
Operator : SM/UA
Sample : I7091-01RE
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RO-CHRT25337RE


Manual Integrations
APPROVED

UGO
1/3/2018 10:22:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 03 00:50:59 2018
Quant Method : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\methods\P0122017.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 20 03:23:29 2017
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

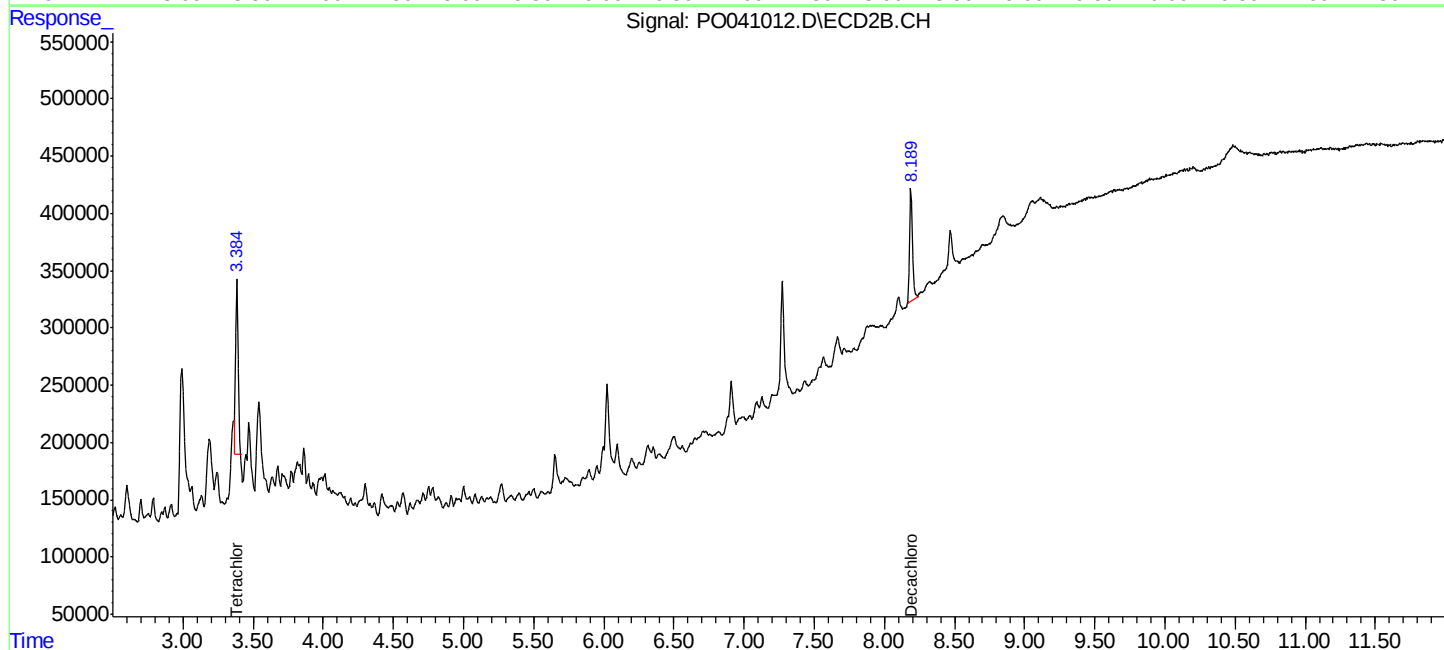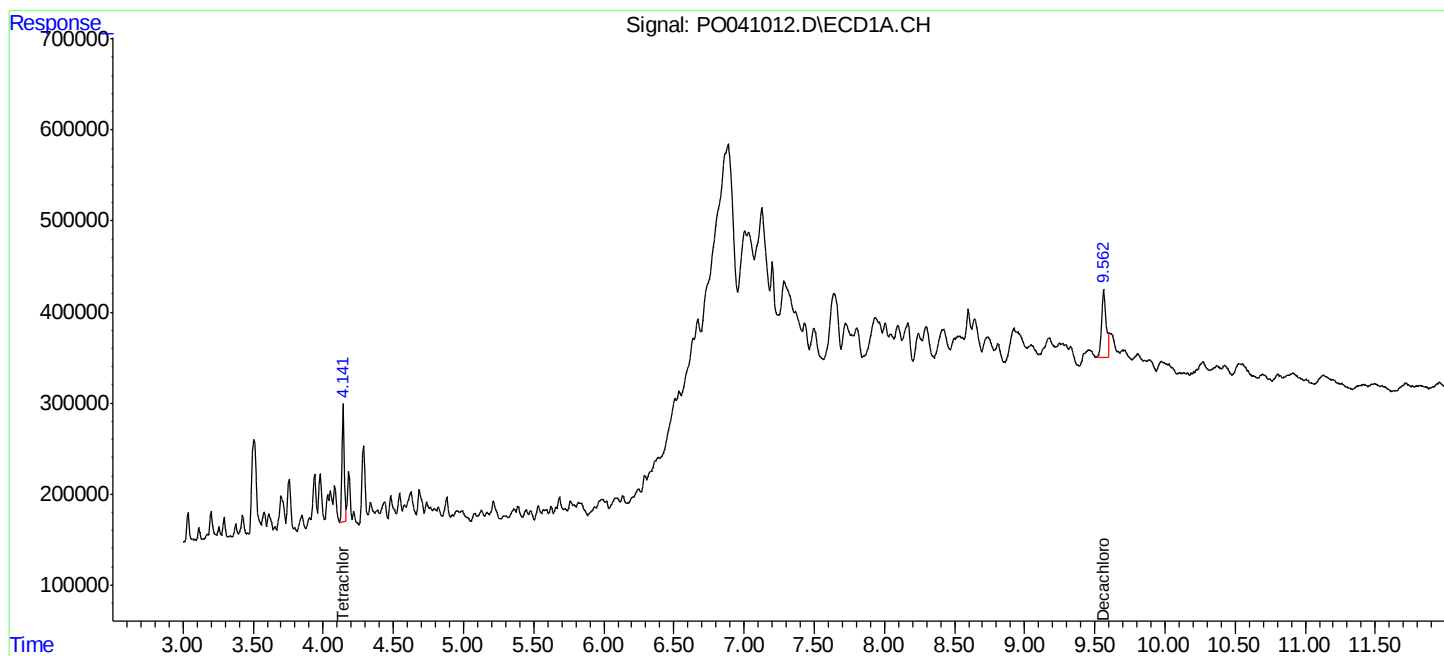

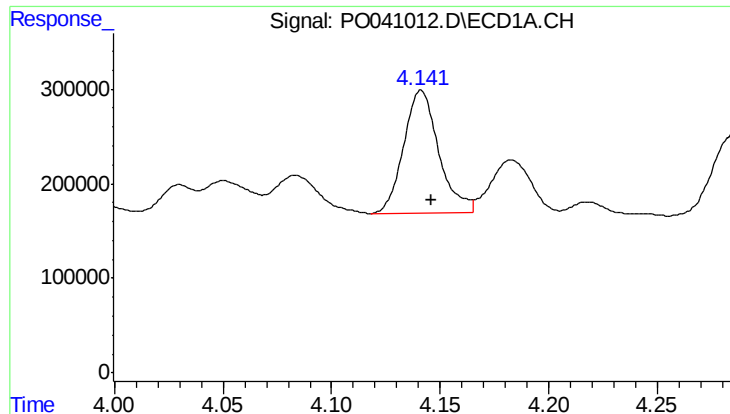


#1 Tetrachloro-m-xylene

R.T.: 4.141 min
Delta R.T.: -0.005 min
Response: 1459482
Conc: 7.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-CHRT25337RE


Manual Integrations
APPROVED

UGO
1/3/2018 10:22:55 AM

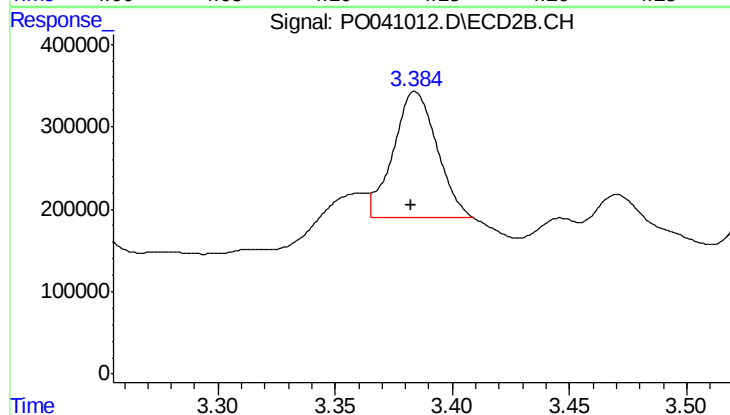


#1 Tetrachloro-m-xylene

R.T.: 3.384 min
Delta R.T.: 0.001 min
Response: 1983632
Conc: 6.44 ng/ml m

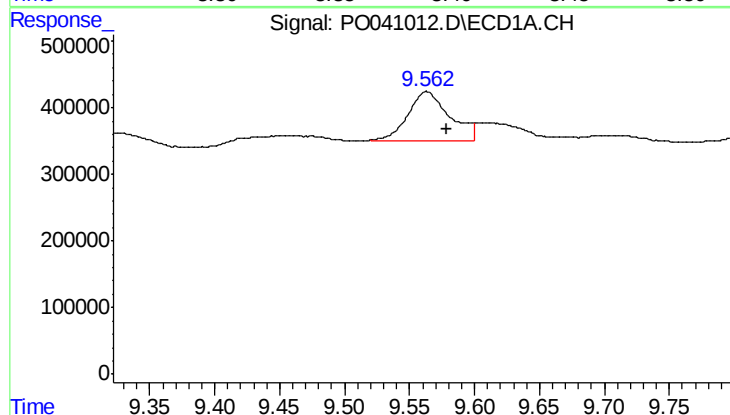

#2 Decachlorobiphenyl

R.T.: 9.562 min
Delta R.T.: -0.016 min
Response: 1652740
Conc: 8.07 ng/ml m

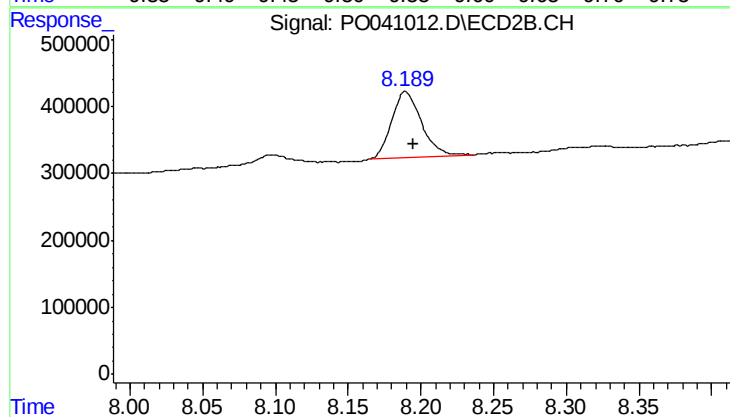

#2 Decachlorobiphenyl

R.T.: 8.189 min
Delta R.T.: -0.006 min
Response: 1404679
Conc: 3.97 ng/ml