

Data Path : P:\HPCHEM1\ECD\_0\Data\P0010318\  
Data File : P0041037.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 03 Jan 2018 16:58  
Operator : SM/UA  
Sample : I6680-21  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
CL-01-122917-A

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 03 23:38:17 2018  
Quant Method : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0122017.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Dec 20 03:23:29 2017  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1  | Resp#2  | ng/ml  | ng/ml   |
|-----------------------------|-------|-------|---------|---------|--------|---------|
| -----                       |       |       |         |         |        |         |
| System Monitoring Compounds |       |       |         |         |        |         |
| 1) SA Tetrachlo...          | 4.136 | 3.376 | 4467881 | 6412521 | 21.547 | 20.804m |
| 2) SA Decachlor...          | 9.547 | 8.179 | 2919213 | 3086807 | 14.256 | 8.716m# |

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD\_0\Data\P0010318\  
Data File : P0041037.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 03 Jan 2018 16:58  
Operator : SM/UA  
Sample : I6680-21  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
CL-01-122917-A

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 03 23:38:17 2018  
Quant Method : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0122017.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Dec 20 03:23:29 2017  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

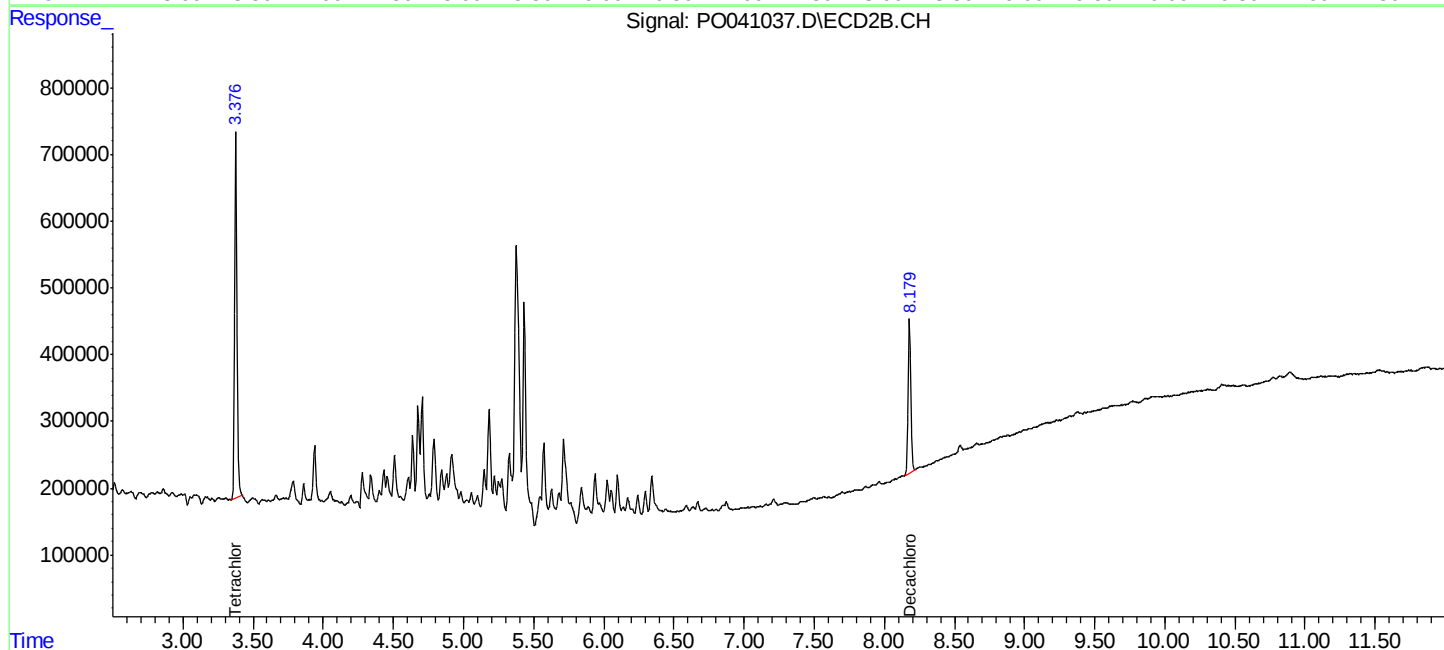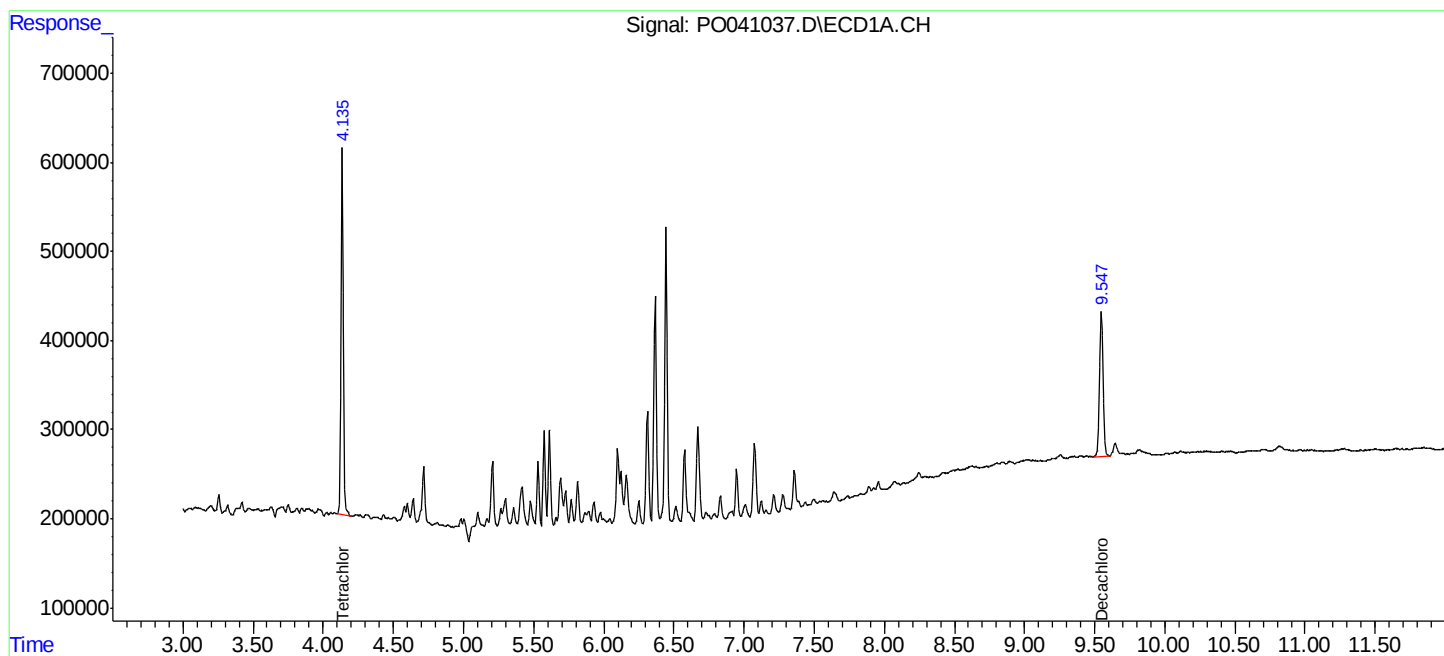


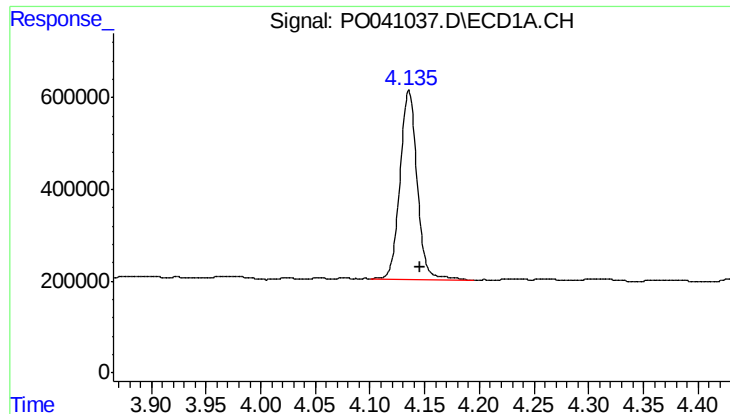

#1 Tetrachloro-m-xylene


R.T.: 4.136 min  
Delta R.T.: -0.010 min  
Response: 4467881  
Conc: 21.55 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
CL-01-122917-A

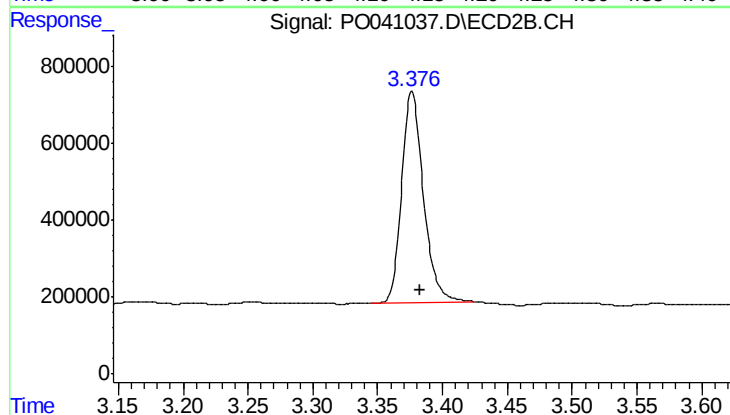


#1 Tetrachloro-m-xylene

R.T.: 3.376 min  
Delta R.T.: -0.006 min  
Response: 6412521  
Conc: 20.80 ng/ml m

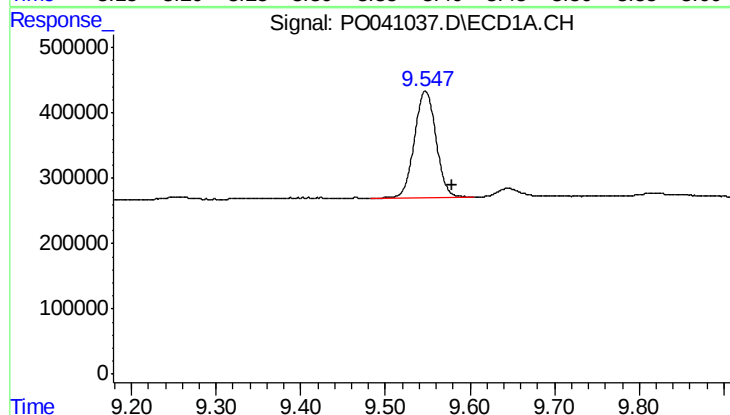

#2 Decachlorobiphenyl

R.T.: 9.547 min  
Delta R.T.: -0.032 min  
Response: 2919213  
Conc: 14.26 ng/ml

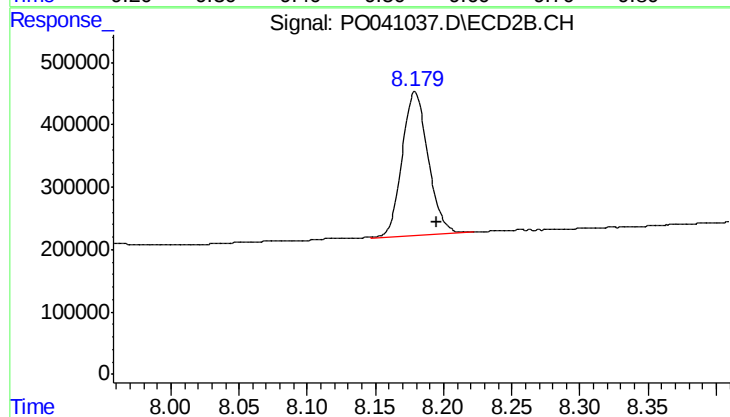

#2 Decachlorobiphenyl

R.T.: 8.179 min  
Delta R.T.: -0.016 min  
Response: 3086807  
Conc: 8.72 ng/ml m