

Data Path : P:\HPCHEM1\ECD_0\Data\P0010618\
 Data File : P0041158.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jan 2018 3:21
 Operator : SM/UA
 Sample : AR1254 MDL6
 Misc : 25PPB WATERECD_0
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1254 MDL6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 04:14:12 2018
 Quant Method : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\methods\AR1254P0010618CLP.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 06 00:32:32 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
 Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.132	3.373	3423882	5295653	21.245	20.092
2) SA Decachlor...	9.540	8.175	8778814	13704268	41.310	40.455
Target Compounds						
26) L6 AR-1254-1	6.308	5.322	425394	475426	31.512	26.958
27) L6 AR-1254-2	6.581	5.625	256330	381476	31.015	26.228
28) L6 AR-1254-3	6.665	5.936	455068	759885	30.539	34.717
29) L6 AR-1254-4	6.945	6.240	475419	386826	36.501	27.412
30) L6 AR-1254-5	7.211	6.341	254835	754367	28.347	25.433


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_0\Data\PO010618\
Data File : PO041158.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jan 2018 3:21
Operator : SM/UA
Sample : AR1254 MDL6
Misc : 25PPB WATER ECD_0
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254 MDL6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 04:14:12 2018
Quant Method : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\methods\AR1254PO010618CLP.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 06 00:32:32 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB MR1 Signal #2 Phase: ZB MR2
Signal #1 Info : 30Mx0.32mmx 0.5µm Signal #2 Info : 30M x 0.32mm x 0.25µm

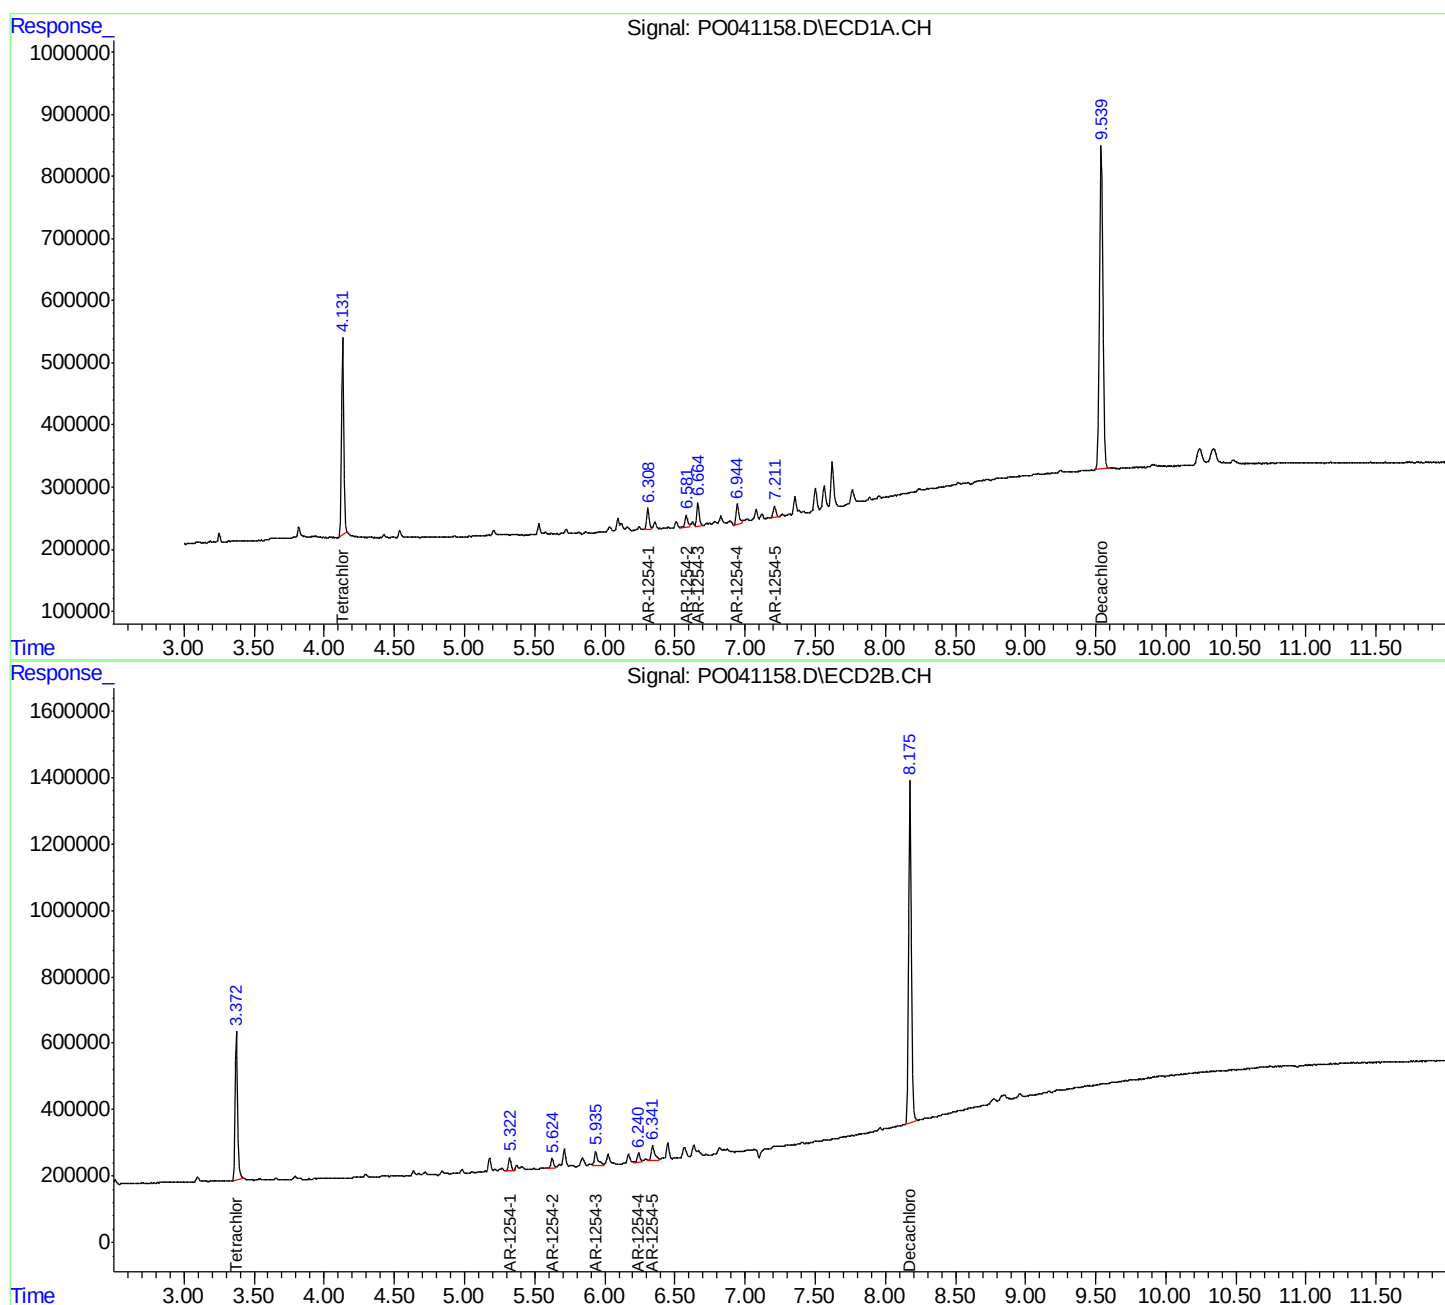


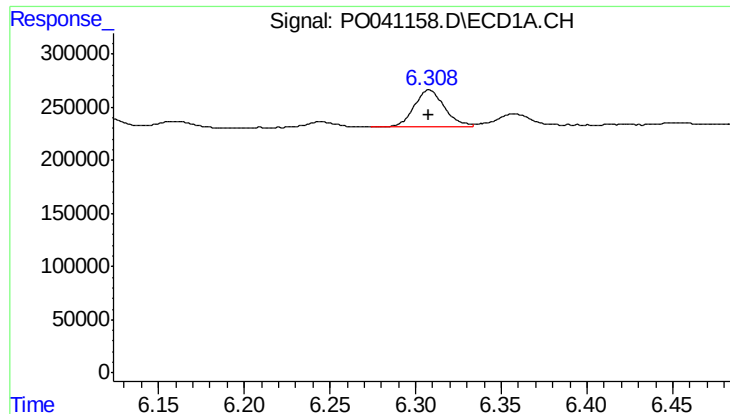

#26 AR-1254-1


R.T.: 6.308 min
Delta R.T.: 0.000 min
Response: 425394
Conc: 31.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254 MDL6

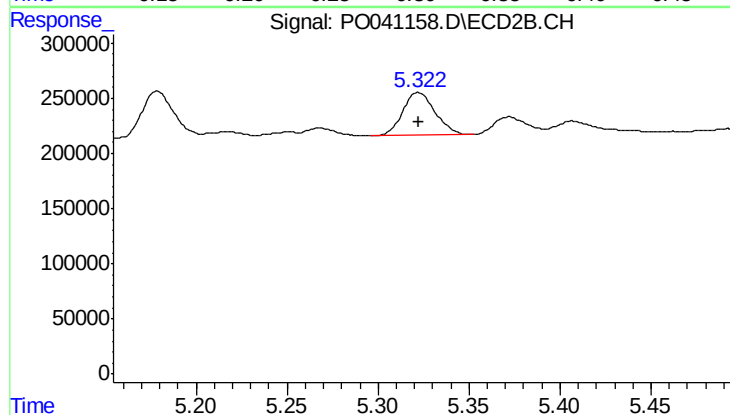


#26 AR-1254-1

R.T.: 5.322 min
Delta R.T.: 0.000 min
Response: 475426
Conc: 26.96 ng/ml

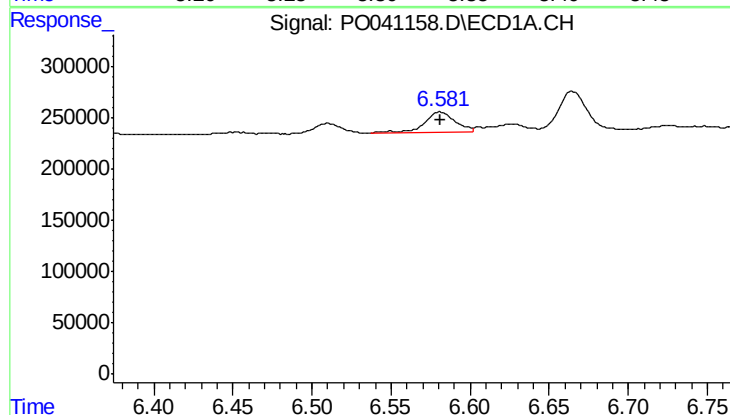


#27 AR-1254-2

R.T.: 6.581 min
Delta R.T.: 0.000 min
Response: 256330
Conc: 31.02 ng/ml

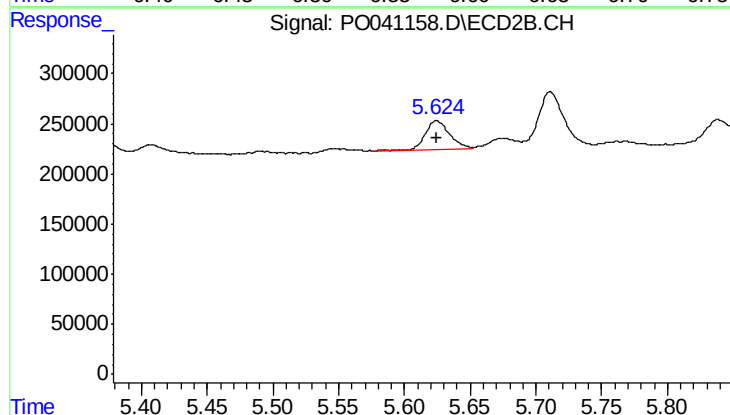

#27 AR-1254-2


R.T.: 5.625 min
Delta R.T.: 0.000 min
Response: 381476
Conc: 26.23 ng/ml

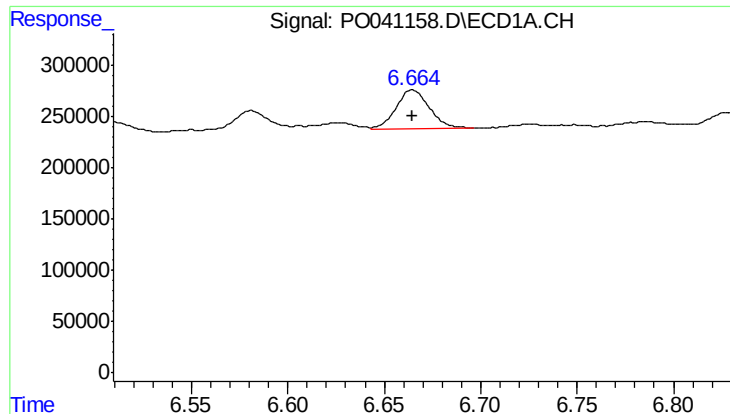

#28 AR-1254-3


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 455068
Conc: 30.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254 MDL6

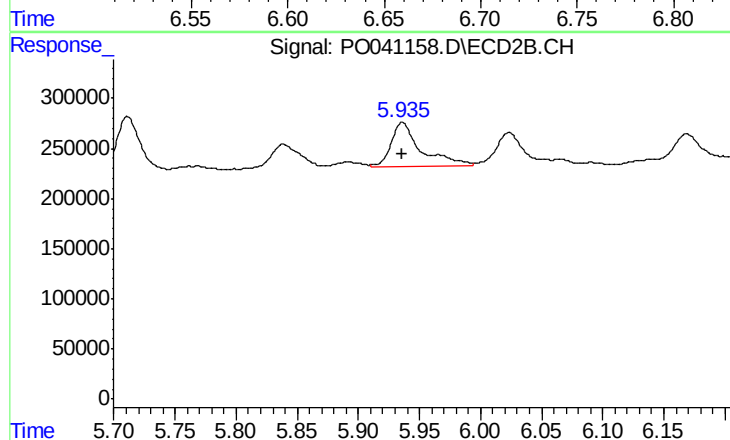


#28 AR-1254-3

R.T.: 5.936 min
Delta R.T.: 0.000 min
Response: 759885
Conc: 34.72 ng/ml

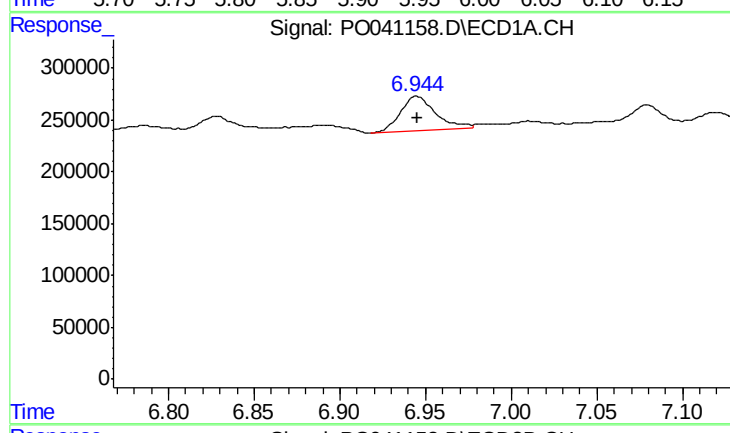


#29 AR-1254-4

R.T.: 6.945 min
Delta R.T.: 0.000 min
Response: 475419
Conc: 36.50 ng/ml

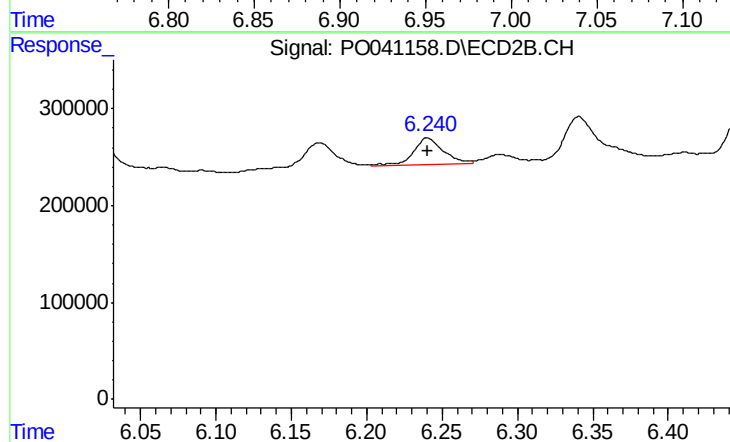

#29 AR-1254-4


R.T.: 6.240 min
Delta R.T.: 0.000 min
Response: 386826
Conc: 27.41 ng/ml

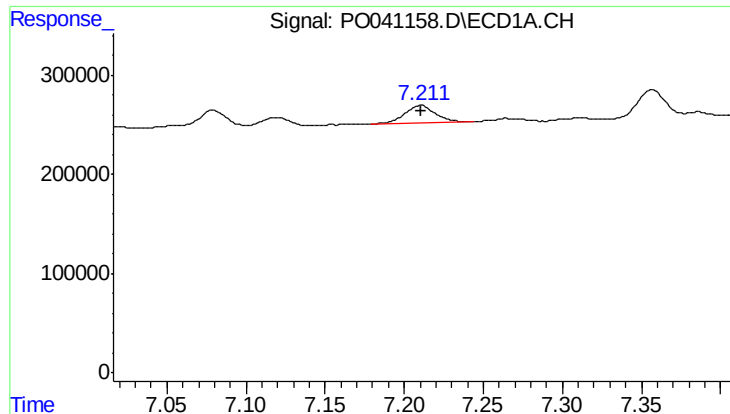

#30 AR-1254-5

R.T.: 7.211 min
Delta R.T.: 0.000 min
Response: 254835
Conc: 28.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254 MDL6

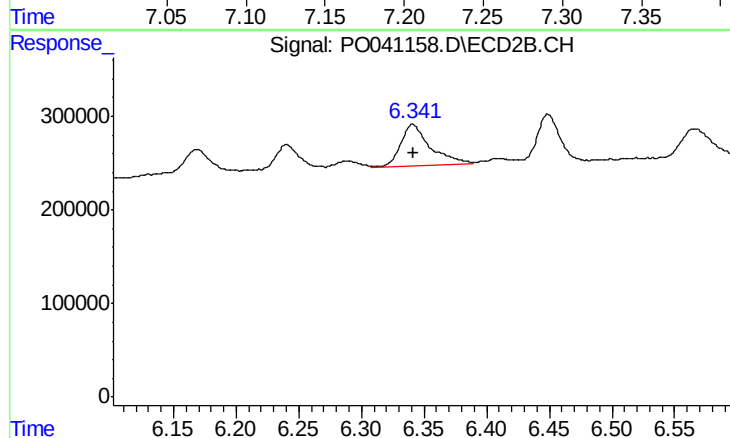

#30 AR-1254-5

R.T.: 6.341 min
Delta R.T.: -0.001 min
Response: 754367
Conc: 25.43 ng/ml