

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010623\
 Data File : P0091892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2023 20:38
 Operator : YP/AJ
 Sample : 01048-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-01-010523

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/09/2023
 Supervised By :Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 05:12:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 05 01:51:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.290	3.466	79143820	35287616	24.628	25.561
2) SA Decachlor...	10.029	8.461	54373844	27688604	22.906	22.000

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010623\
Data File : PO091892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2023 20:38
Operator : YP/AJ
Sample : 01048-01
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-01-010523


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/09/2023
Supervised By :Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 05:12:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010423.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 05 01:51:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

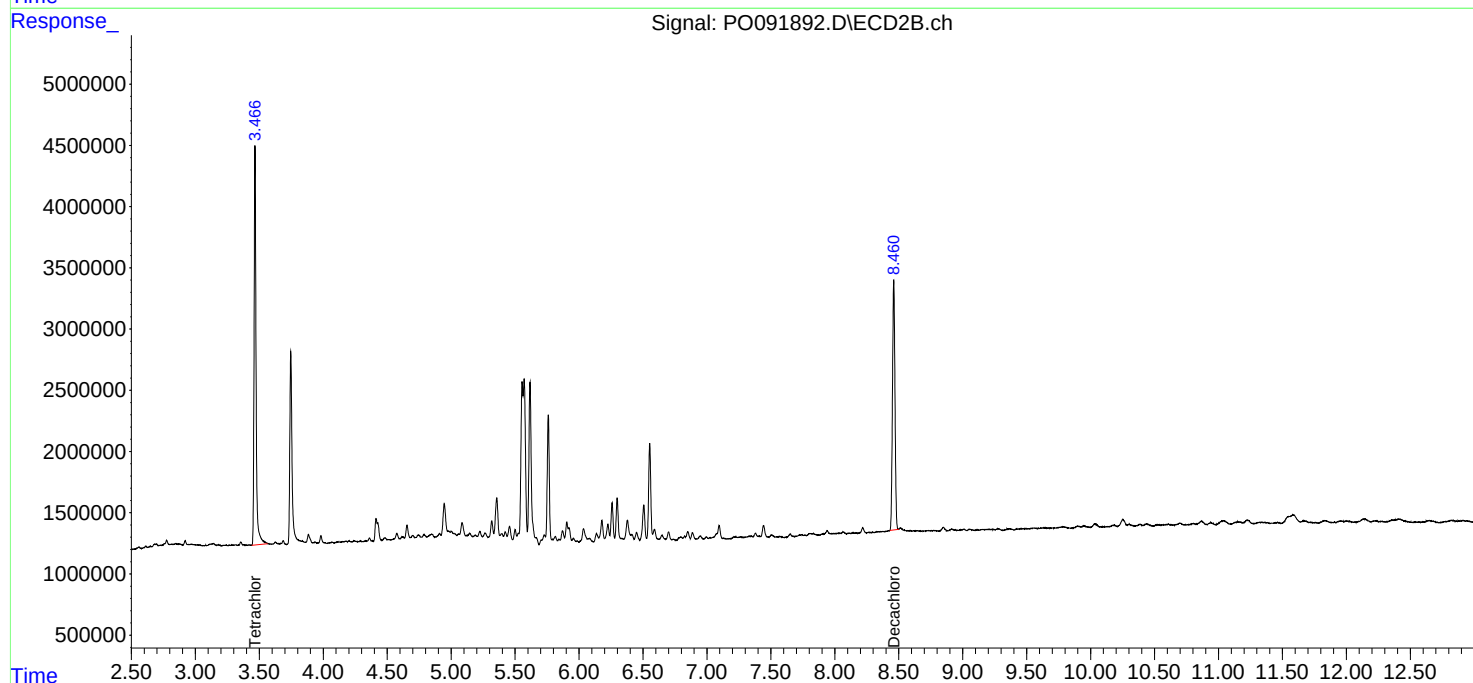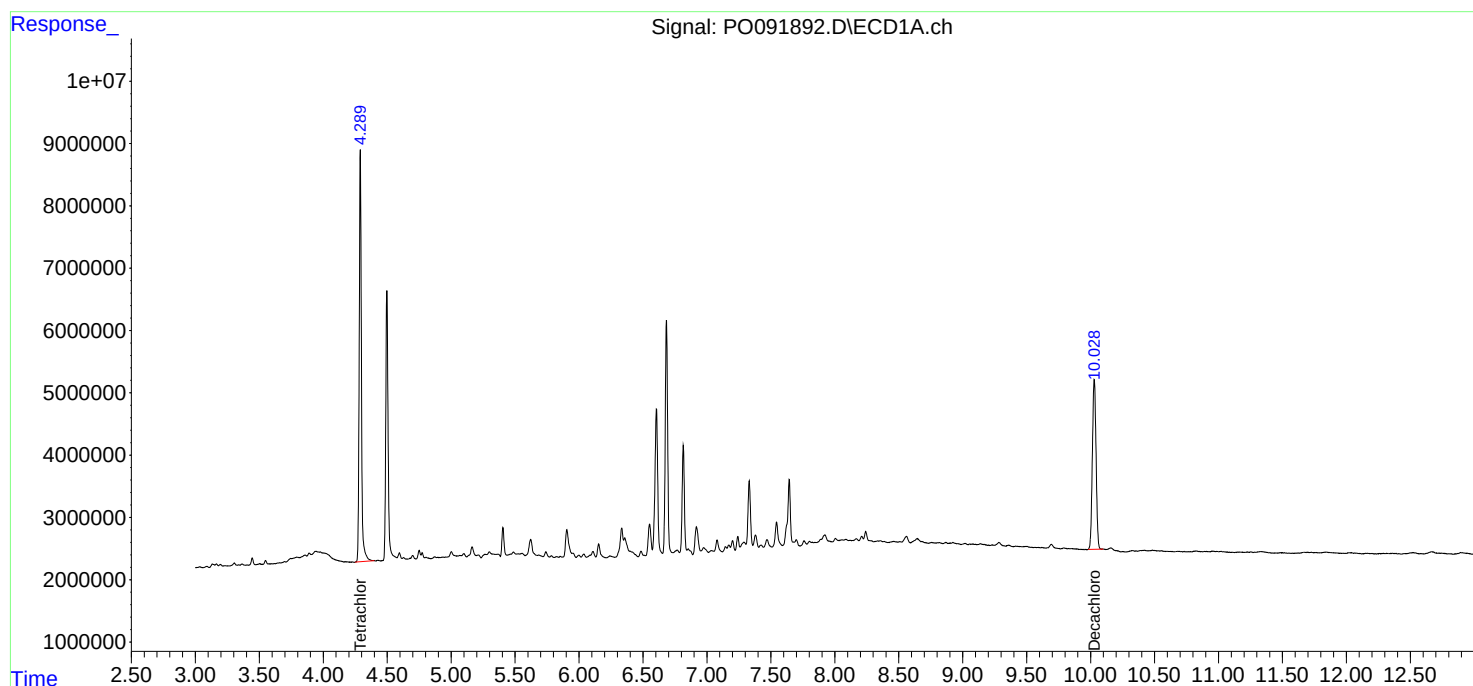

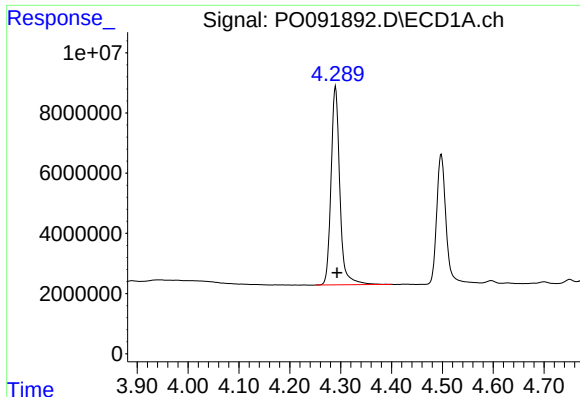


#1 Tetrachloro-m-xylene

R.T.: 4.290 min
Delta R.T.: -0.003 min
Response: 79143820
Conc: 24.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-01-010523


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/09/2023
Supervised By :Ankita Jodhani 01/09/2023

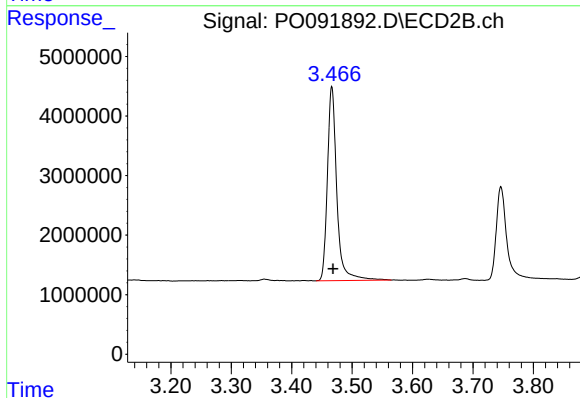


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: -0.002 min
Response: 35287616
Conc: 25.56 ng/ml

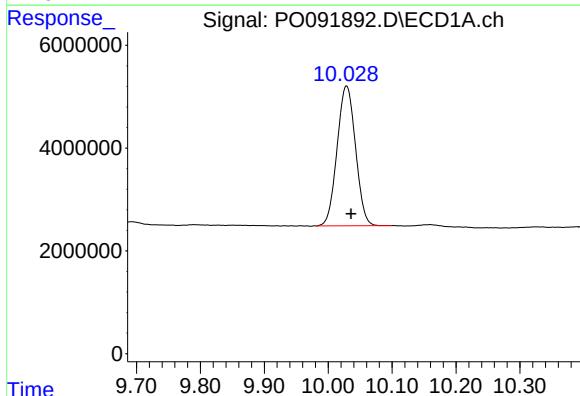

#2 Decachlorobiphenyl

R.T.: 10.029 min
Delta R.T.: -0.007 min
Response: 54373844
Conc: 22.91 ng/ml

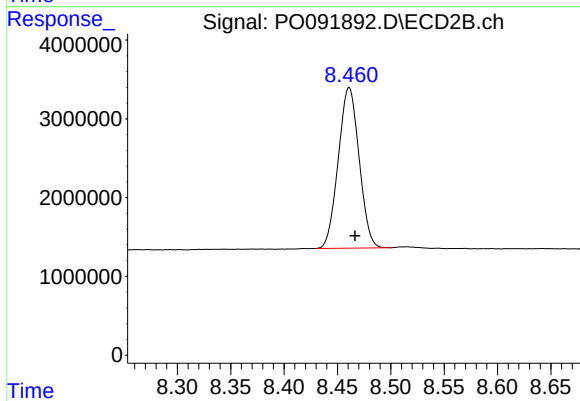

#2 Decachlorobiphenyl

R.T.: 8.461 min
Delta R.T.: -0.005 min
Response: 27688604
Conc: 22.00 ng/ml