

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010623\
 Data File : P0091899.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2023 22:55
 Operator : YP/AJ
 Sample : 01045-01
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-SAMPLE-TANK-11-12-31-32-33

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/09/2023
 Supervised By :Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 05:17:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 05 01:51:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.289	3.466	68343155	31420304	21.267m	22.760
2) SA Decachlor...	10.027	8.460	51900799	27647127	21.864	21.967

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010623\
Data File : PO091899.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2023 22:55
Operator : YP/AJ
Sample : 01045-01
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-SAMPLE-TANK-11-12-31-32-33


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/09/2023
Supervised By :Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 05:17:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010423.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 05 01:51:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

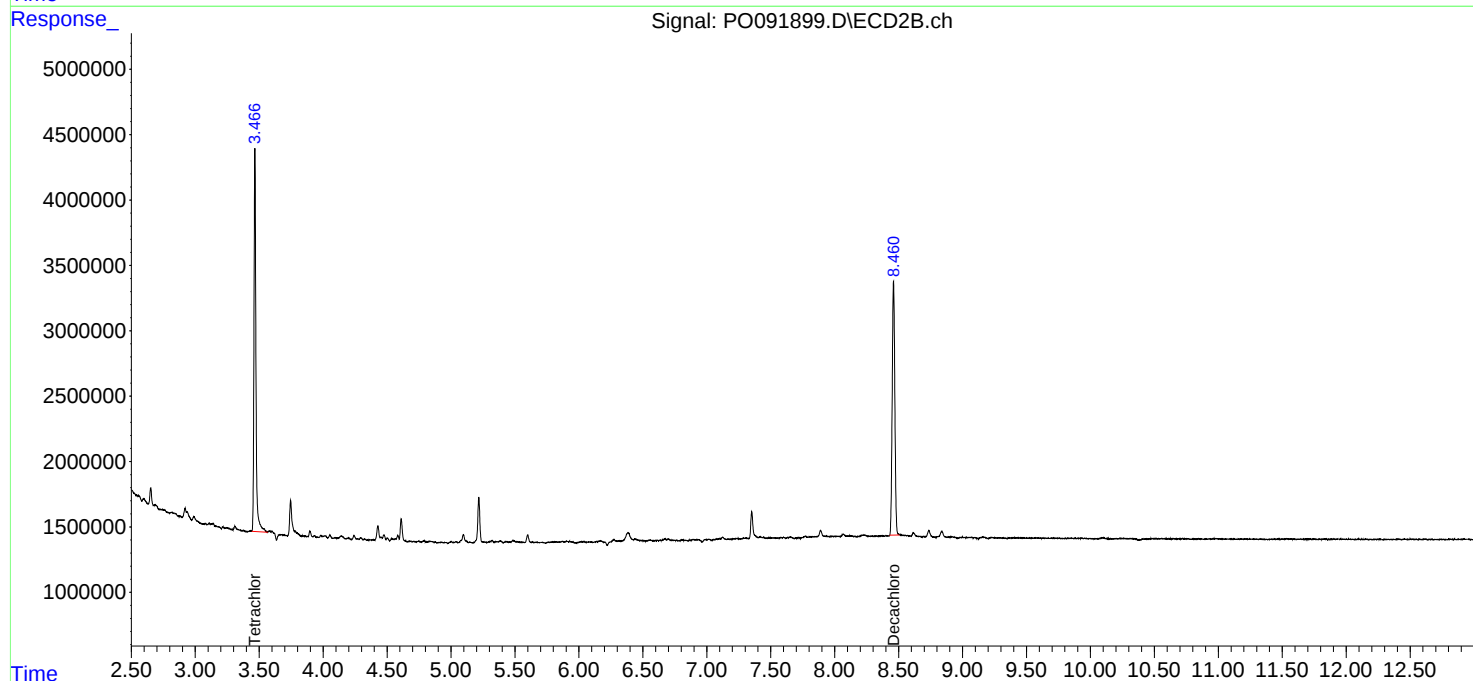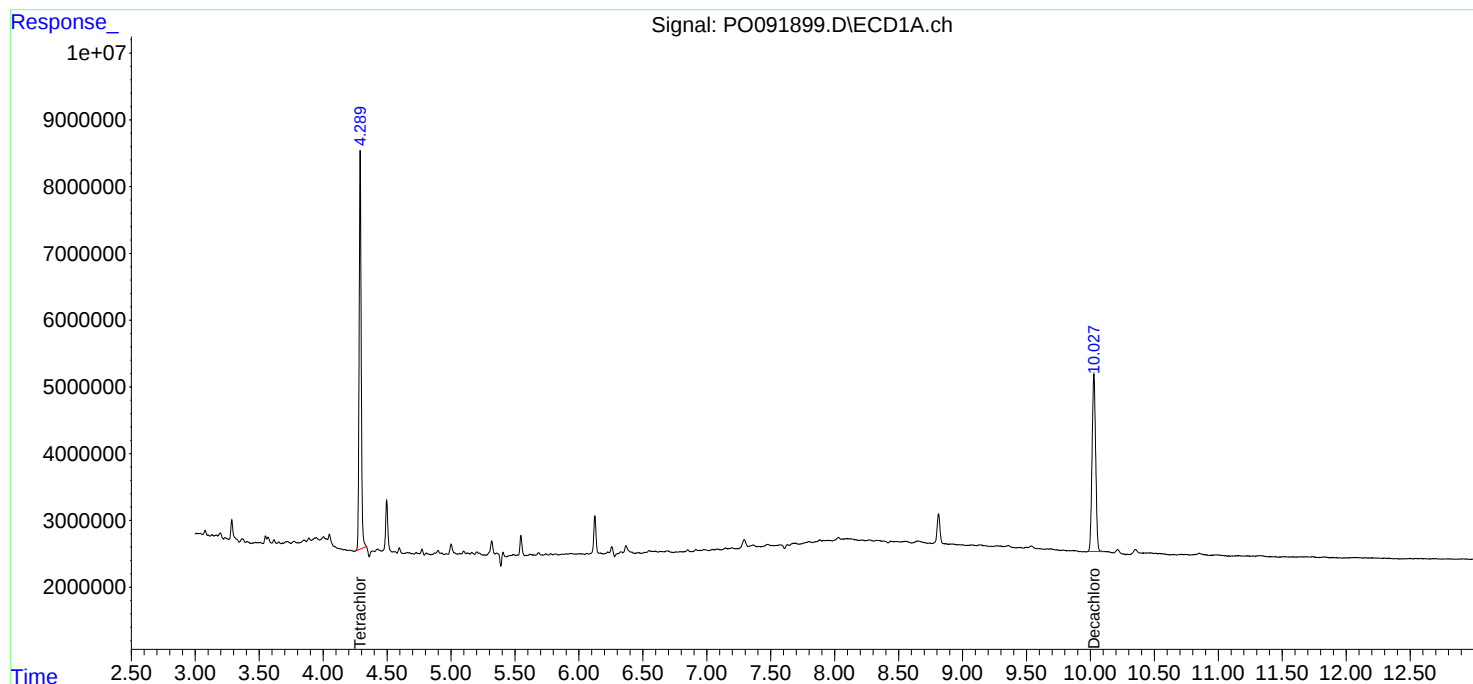

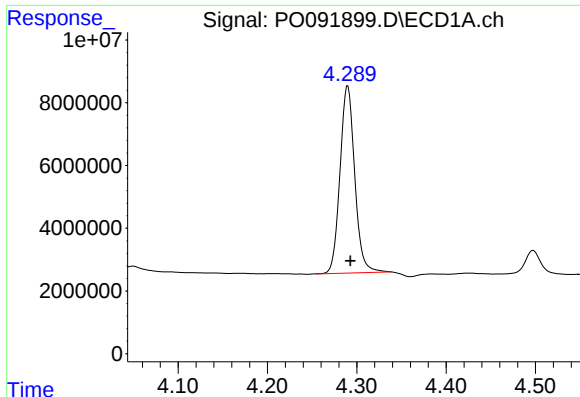


#1 Tetrachloro-m-xylene

R.T.: 4.289 min
Delta R.T.: -0.004 min
Response: 68343155
Conc: 21.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-SAMPLE-TANK-11-12-31-32-33


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/09/2023
Supervised By :Ankita Jodhani 01/09/2023

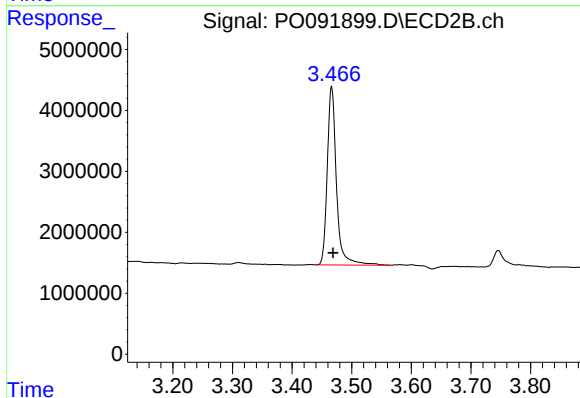


#1 Tetrachloro-m-xylene

R.T.: 3.466 min
Delta R.T.: -0.002 min
Response: 31420304
Conc: 22.76 ng/ml

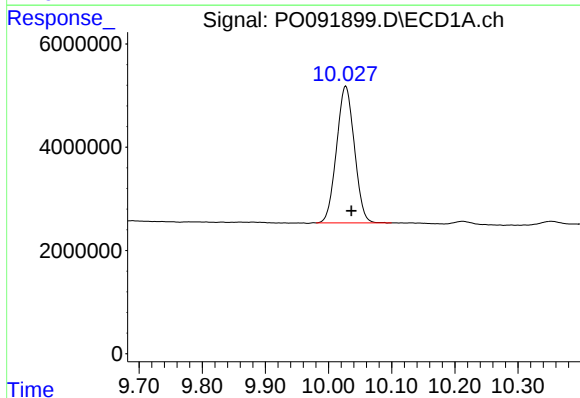

#2 Decachlorobiphenyl

R.T.: 10.027 min
Delta R.T.: -0.009 min
Response: 51900799
Conc: 21.86 ng/ml

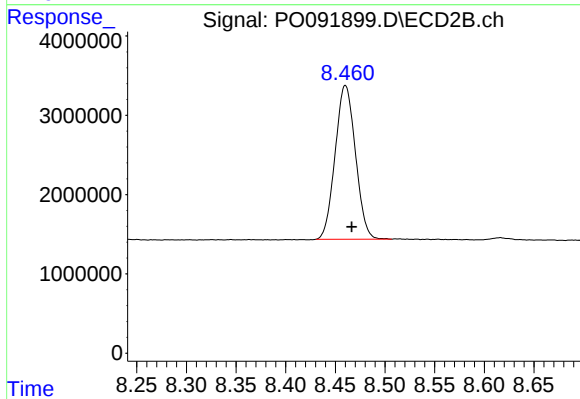

#2 Decachlorobiphenyl

R.T.: 8.460 min
Delta R.T.: -0.006 min
Response: 27647127
Conc: 21.97 ng/ml