

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010819\
Data File : P0053292.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2019 8:54
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 03:38:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 09 03:34:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.171	3.207	24952840	5034555	18.674	20.135
2) SA Decachlor...	9.630	7.851	15848264	4526361	20.065	19.765

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010819\
Data File : PO053292.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2019 8:54
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 03:38:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 09 03:34:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

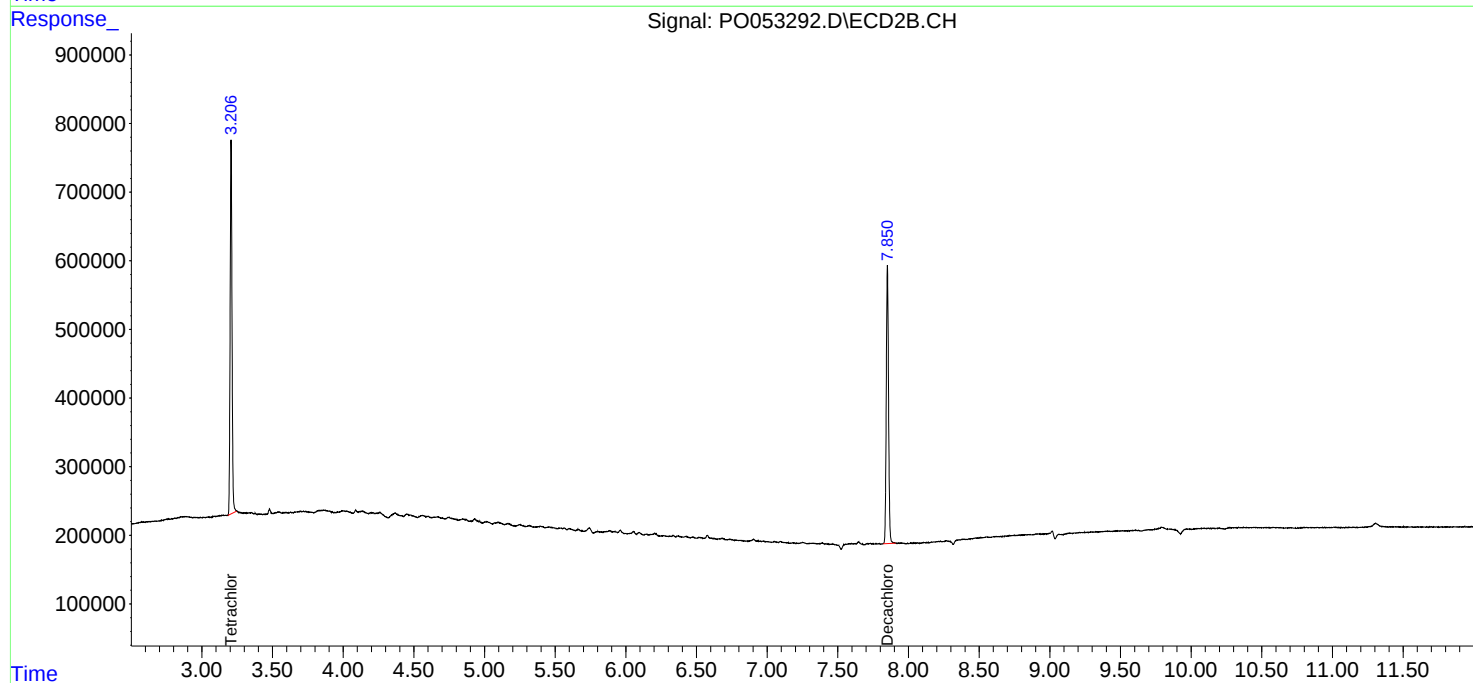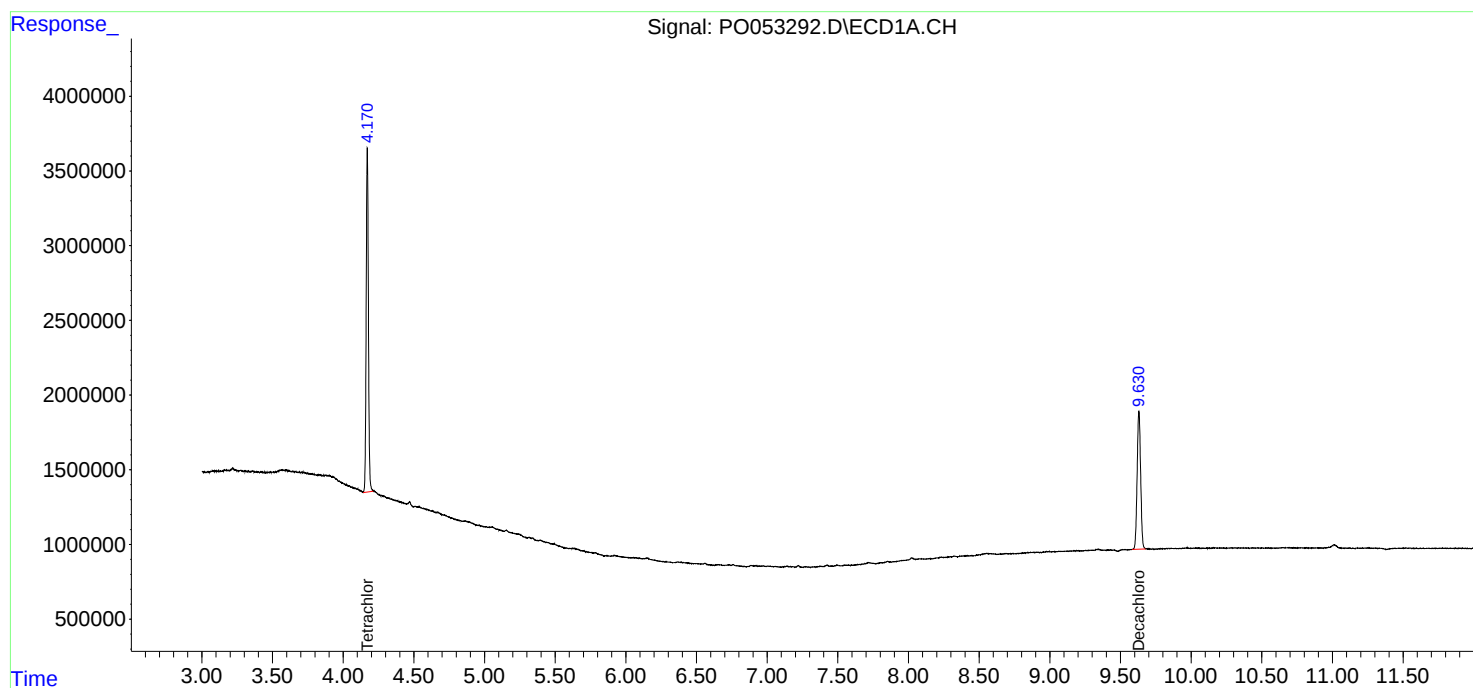


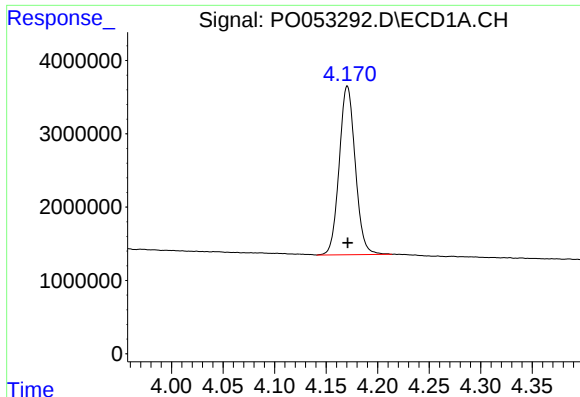

#1 Tetrachloro-m-xylene


R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 24952840
Conc: 18.67 ng/ml

Instrument :
ECD_O
ClientSampleId :

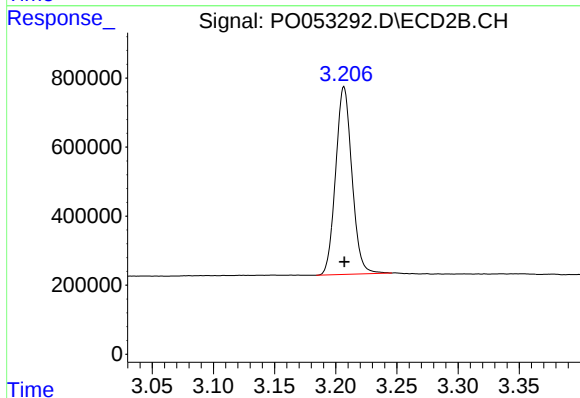


#1 Tetrachloro-m-xylene

R.T.: 3.207 min
Delta R.T.: 0.000 min
Response: 5034555
Conc: 20.13 ng/ml

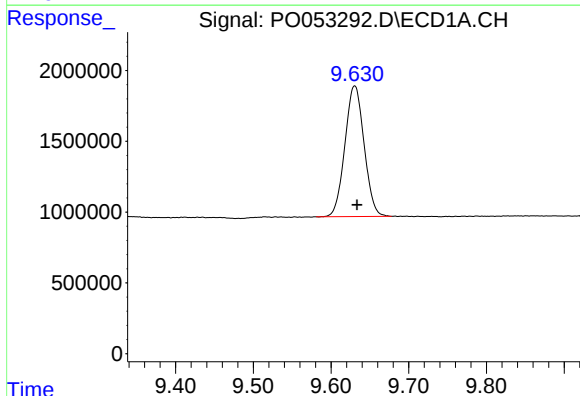

#2 Decachlorobiphenyl

R.T.: 9.630 min
Delta R.T.: -0.003 min
Response: 15848264
Conc: 20.06 ng/ml

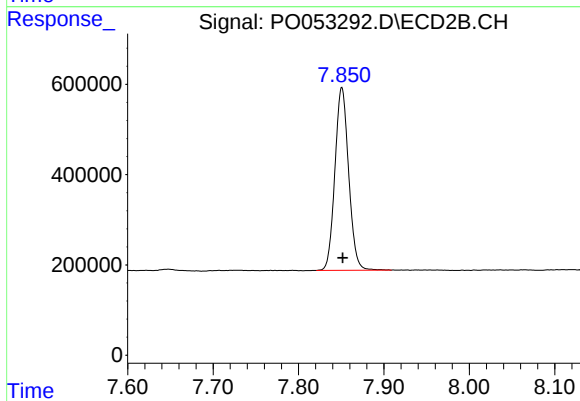

#2 Decachlorobiphenyl

R.T.: 7.851 min
Delta R.T.: -0.001 min
Response: 4526361
Conc: 19.77 ng/ml