

Data Path : P:\HPCHEM1\ECD_0\Data\P0011118\
 Data File : P0041297.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2018 10:55
 Operator : SM/UA
 Sample : J1044-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-COMP-A

Manual Integrations
 APPROVED

ugo
 1/12/2018 11:26:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 22:20:15 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0122017.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 20 03:23:29 2017
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.136	3.369	2976434	4024691	14.354	13.057m
2) SA Decachlor...	9.549	8.175	1875337	2674463	9.158	7.552m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0011118\
Data File : P0041297.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2018 10:55
Operator : SM/UA
Sample : J1044-04
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SP-COMP-A


Manual Integrations
APPROVED

ugo
1/12/2018 11:26:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 22:20:15 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0122017.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 20 03:23:29 2017
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

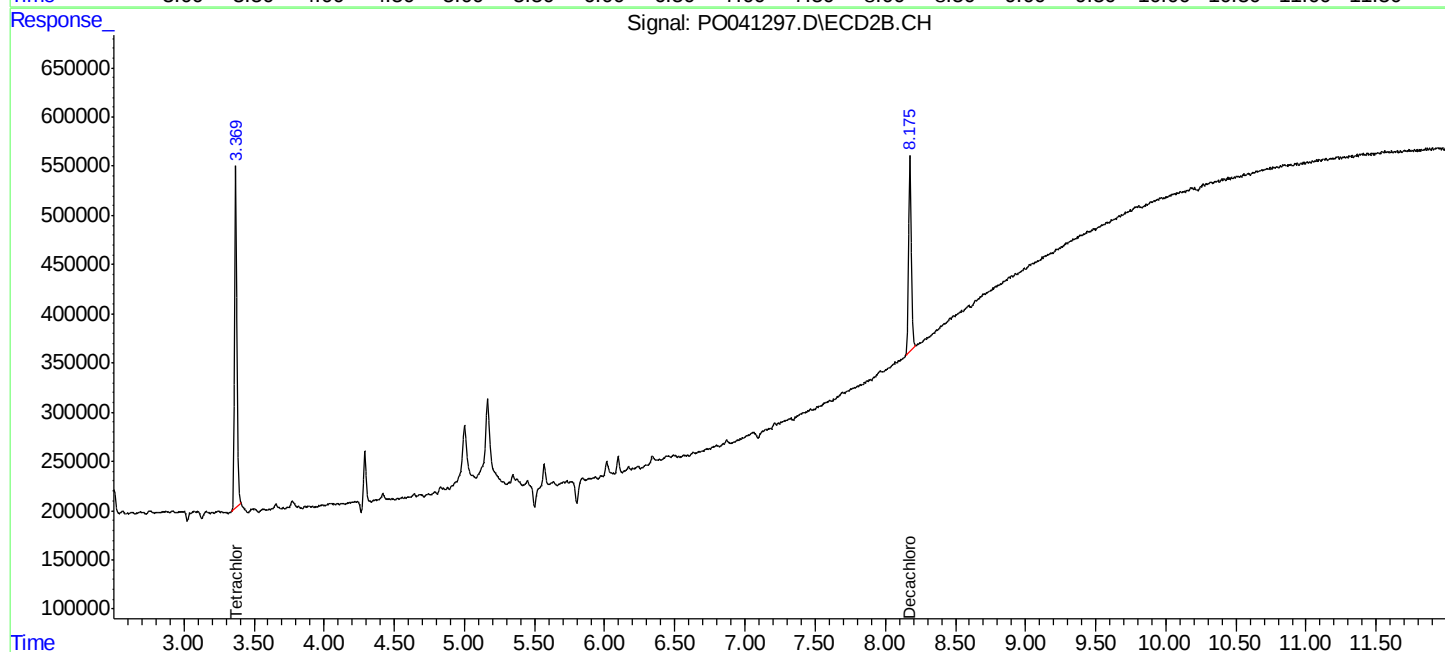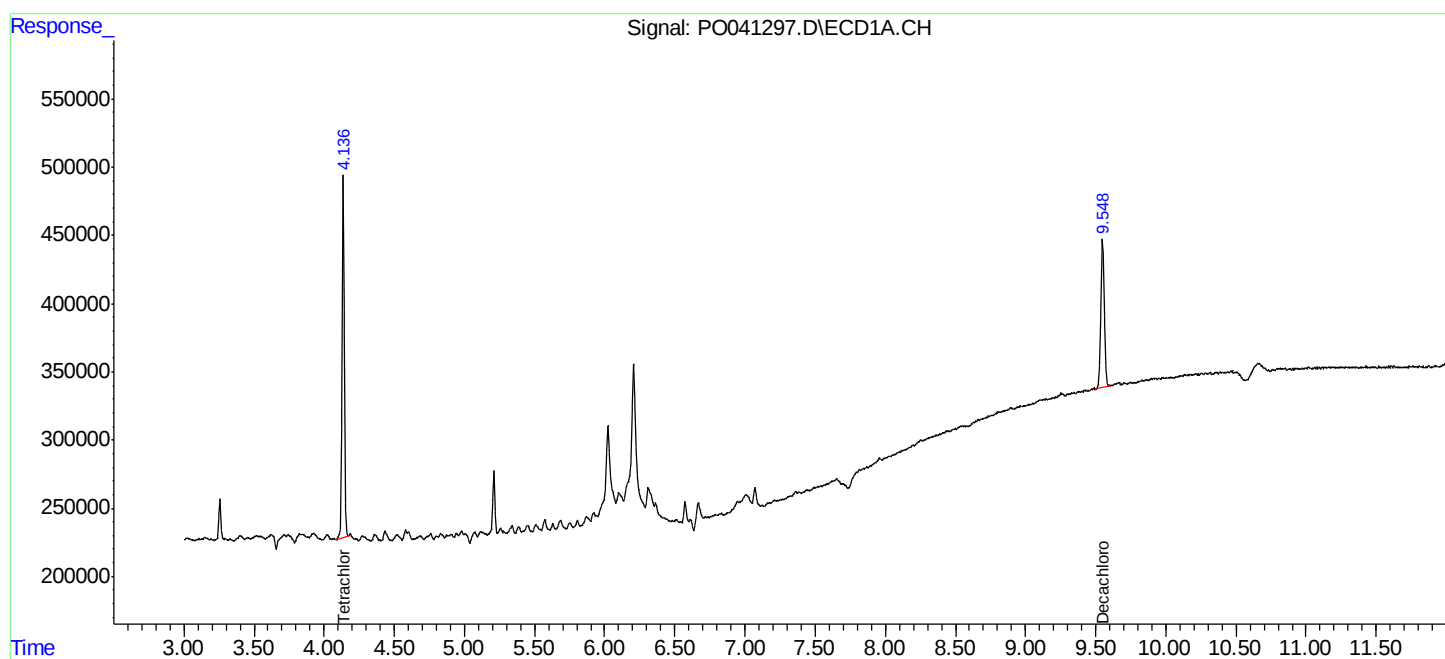

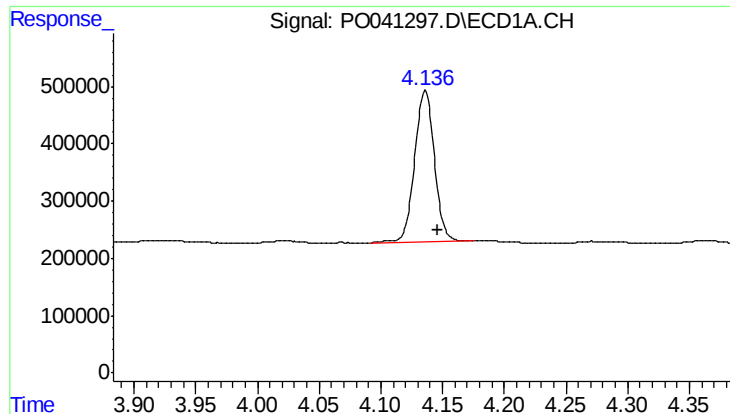


#1 Tetrachloro-m-xylene

R.T.: 4.136 min
Delta R.T.: -0.010 min
Response: 2976434
Conc: 14.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
SP-COMP-A


Manual Integrations
APPROVED

ugo
1/12/2018 11:26:29 AM

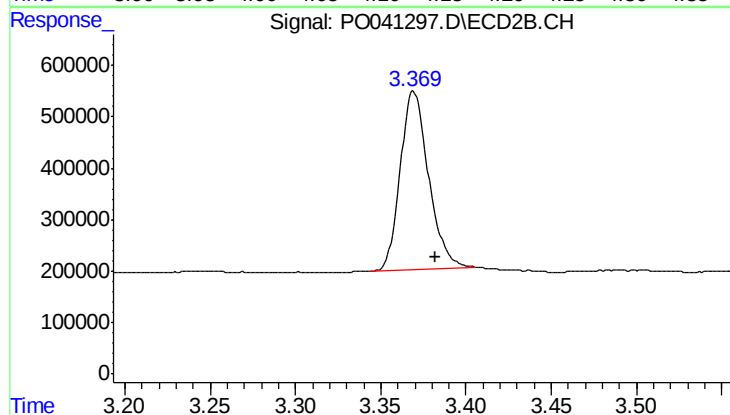


#1 Tetrachloro-m-xylene

R.T.: 3.369 min
Delta R.T.: -0.014 min
Response: 4024691
Conc: 13.06 ng/ml m

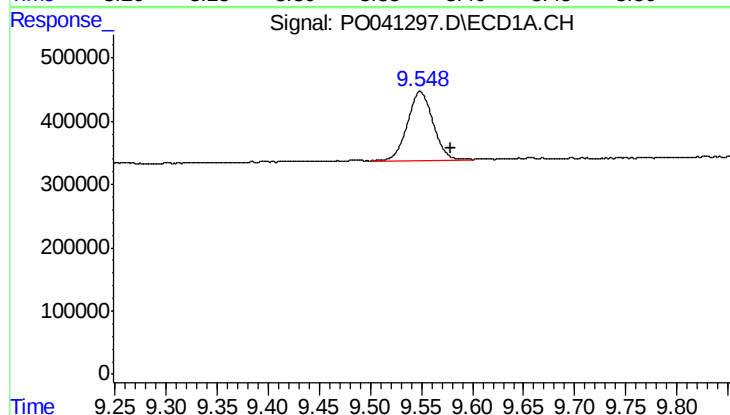

#2 Decachlorobiphenyl

R.T.: 9.549 min
Delta R.T.: -0.030 min
Response: 1875337
Conc: 9.16 ng/ml

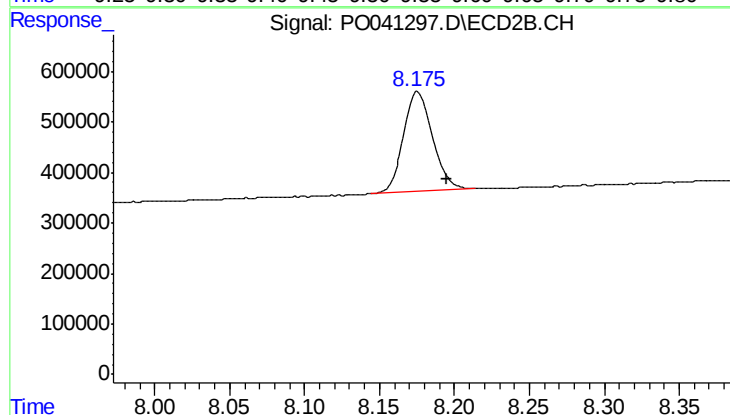

#2 Decachlorobiphenyl

R.T.: 8.175 min
Delta R.T.: -0.020 min
Response: 2674463
Conc: 7.55 ng/ml m