

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011119\
 Data File : P0053389.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jan 2019 13:58
 Operator : SM/SJ
 Sample : K1100-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WATER-DRUMS-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 22:08:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 09 03:34:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.164	3.203	15366097	1996267	11.499	7.984 #
2)	SA Decachlor...	9.616	7.842	6559467	2107080	8.305	9.201
Target Compounds							
32)	L7 AR-1260-2	7.120	0.000	38144	0	0.796	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011119\
Data File : P0053389.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jan 2019 13:58
Operator : SM/SJ
Sample : K1100-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
WATER-DRUMS-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 22:08:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 09 03:34:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

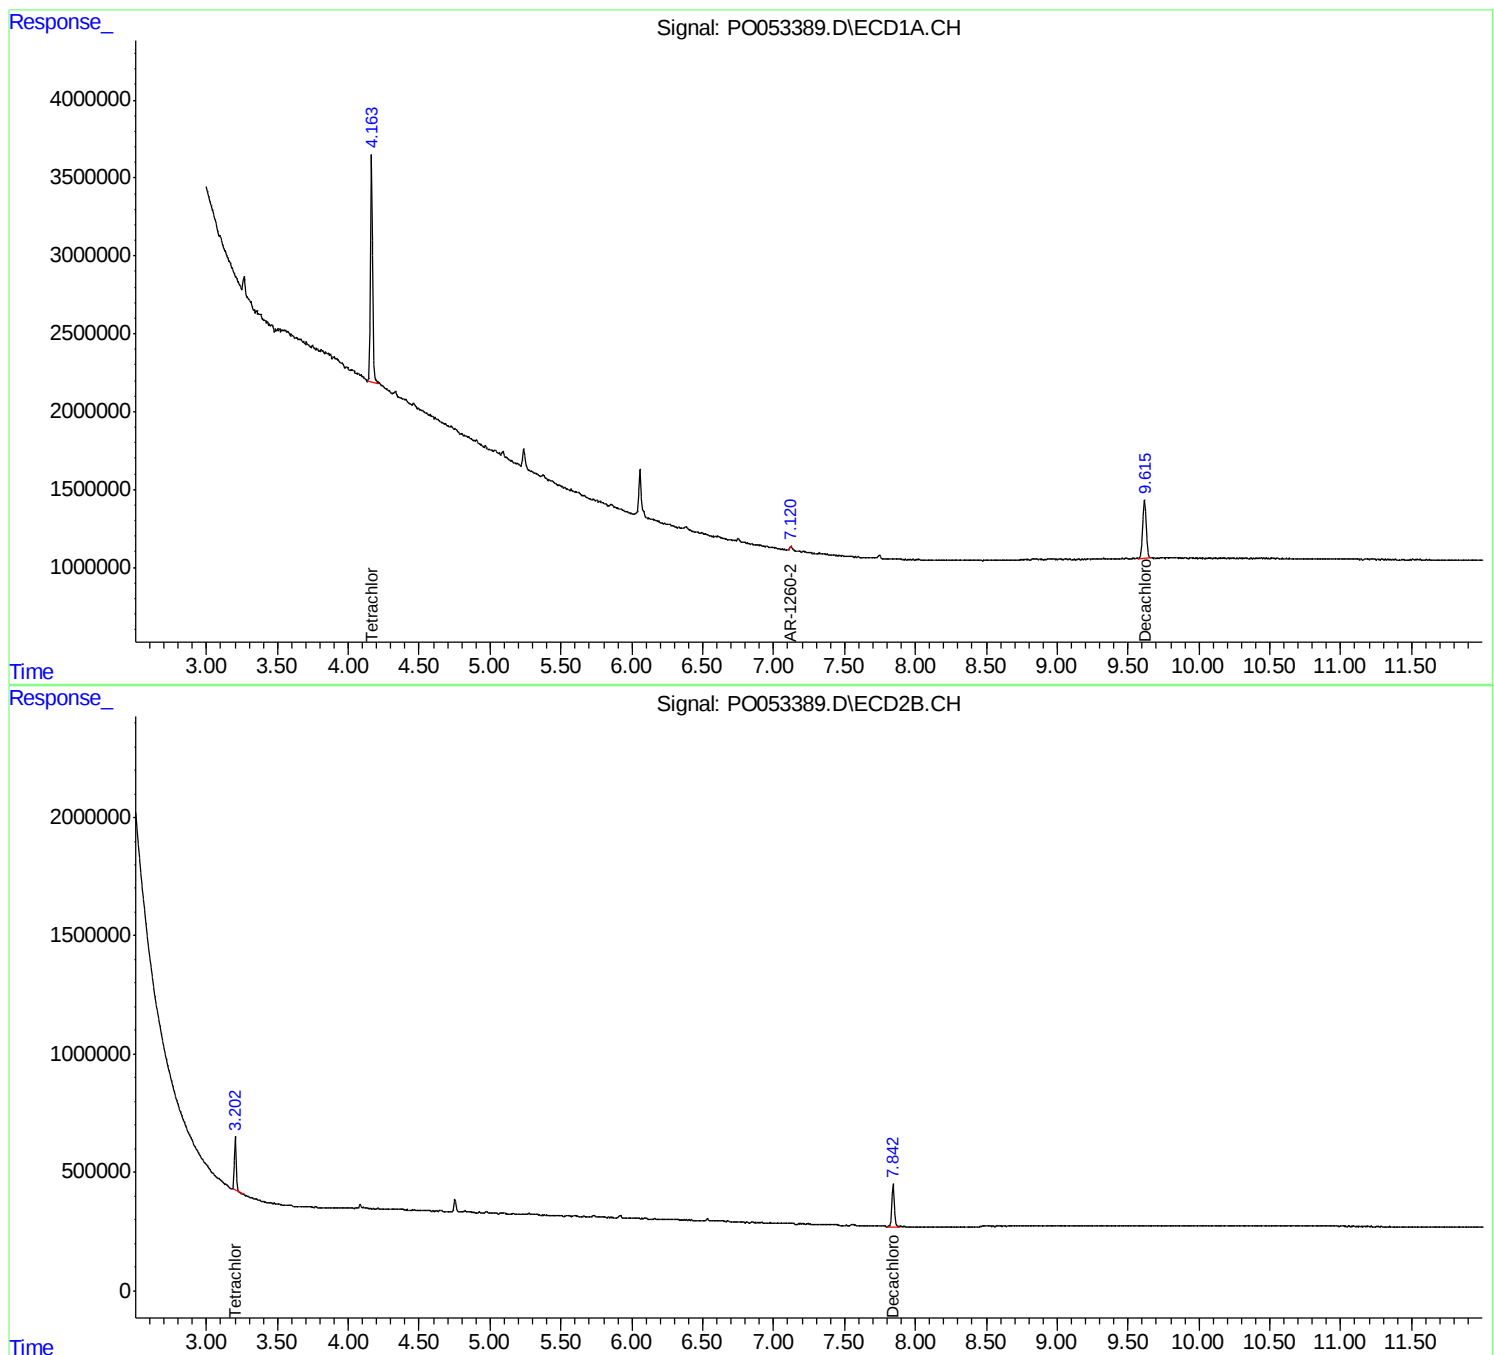


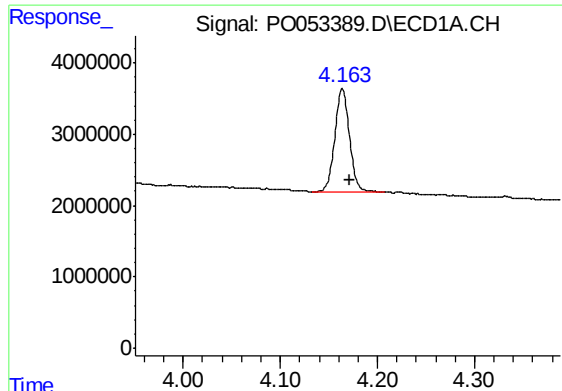

#1 Tetrachloro-m-xylene


R.T.: 4.164 min
Delta R.T.: -0.007 min
Response: 15366097
Conc: 11.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
WATER-DRUMS-A

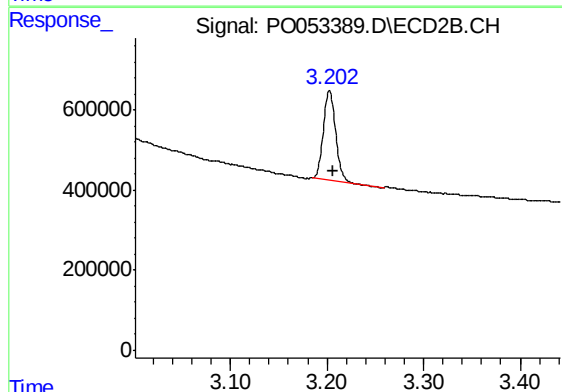


#1 Tetrachloro-m-xylene

R.T.: 3.203 min
Delta R.T.: -0.004 min
Response: 1996267
Conc: 7.98 ng/ml

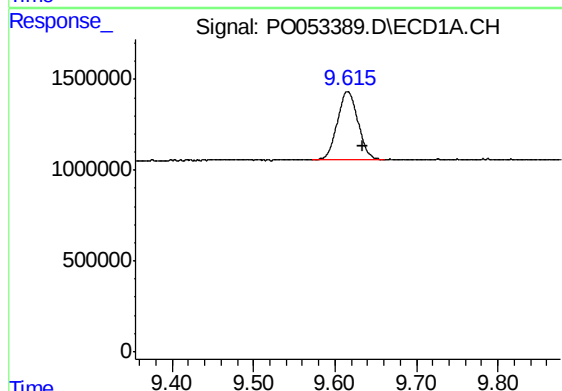


#2 Decachlorobiphenyl

R.T.: 9.616 min
Delta R.T.: -0.018 min
Response: 6559467
Conc: 8.30 ng/ml

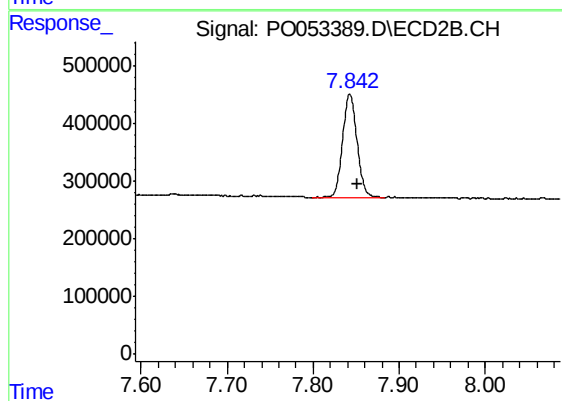

#2 Decachlorobiphenyl


R.T.: 7.842 min
Delta R.T.: -0.009 min
Response: 2107080
Conc: 9.20 ng/ml

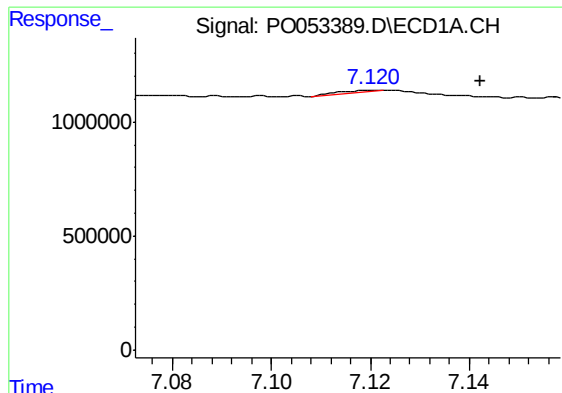

#32 AR-1260-2

R.T.: 7.120 min
Delta R.T.: -0.022 min
Response: 38144
Conc: 0.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
WATER-DRUMS-A

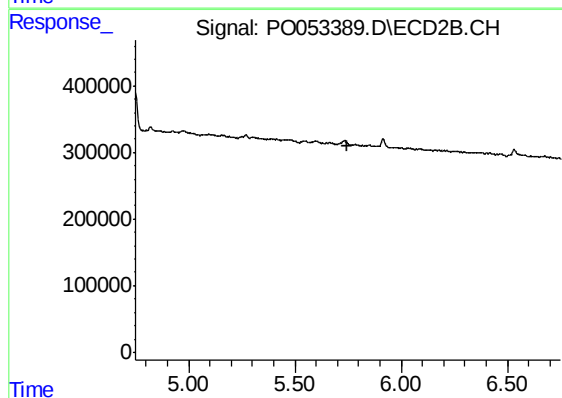

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 5.750 min
Response: 0
Conc: N.D.