

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011119\
 Data File : P0053419.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jan 2019 22:52
 Operator : SM/SJ
 Sample : K1119-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DS-B

Manual Integrations
 APPROVED

Sohil
 1/14/2019 3:58:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 23:54:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 09 03:34:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.162	3.203	19408245	3494804	14.524m	13.977
2) SA Decachlor...	9.612	7.841	13745345	3970762	17.402	17.339

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011119\
Data File : P0053419.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jan 2019 22:52
Operator : SM/SJ
Sample : K1119-03
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DS-B


Manual Integrations
APPROVED

Sohil
1/14/2019 3:58:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 23:54:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 09 03:34:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

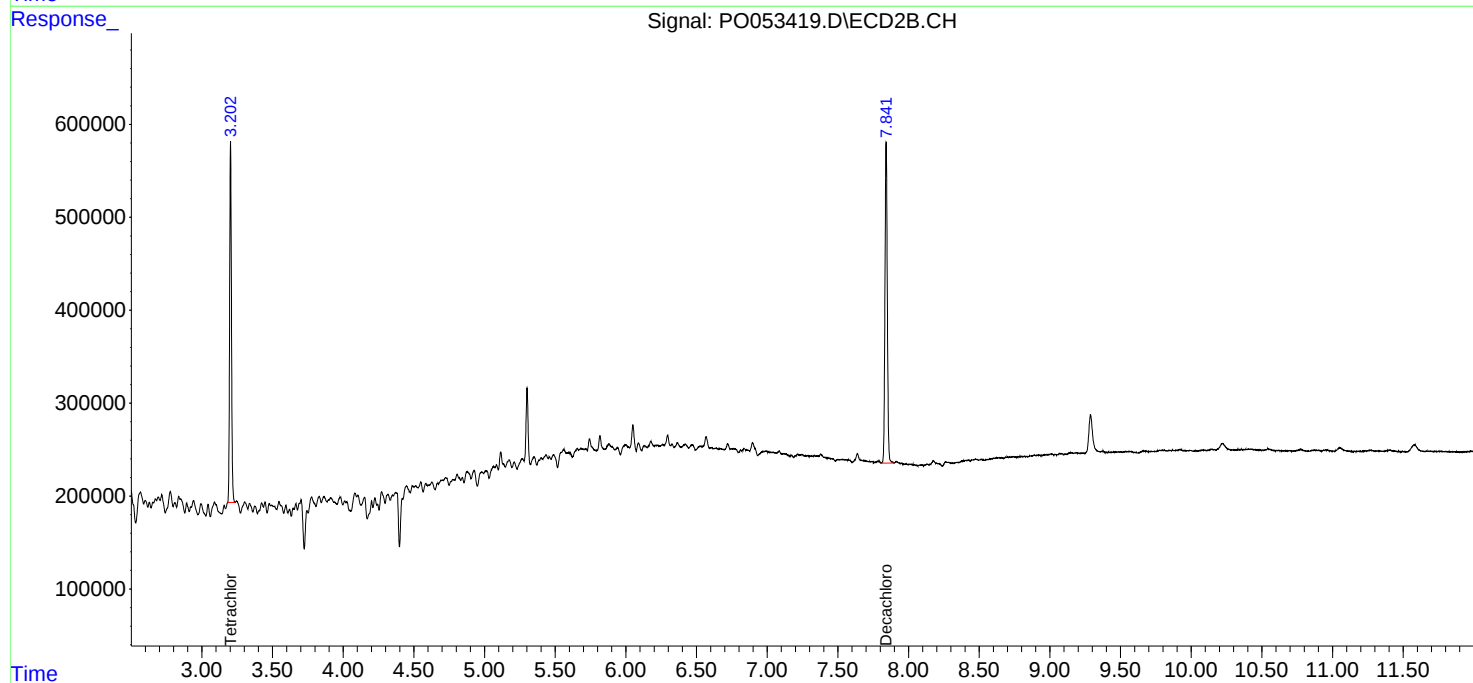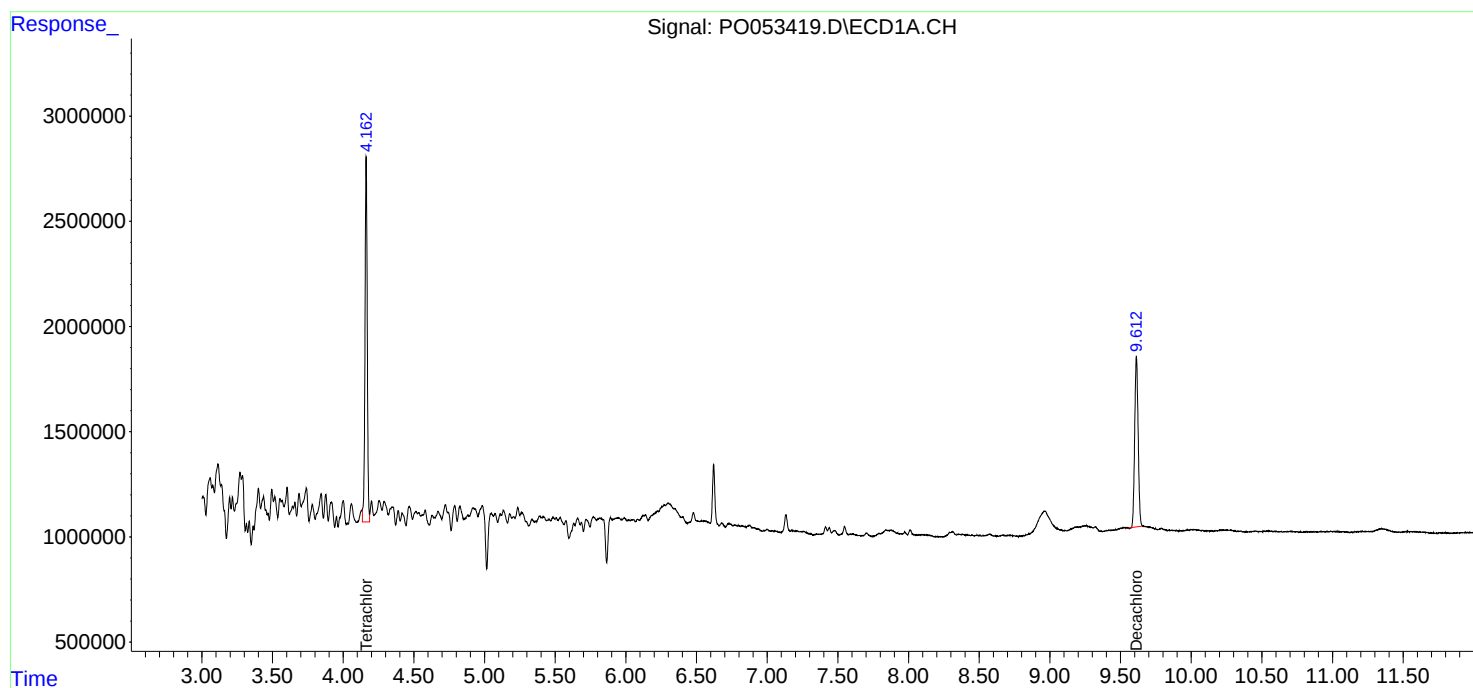

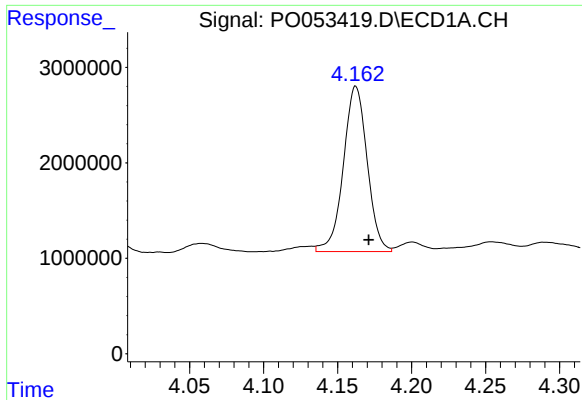


#1 Tetrachloro-m-xylene

R.T.: 4.162 min
Delta R.T.: -0.009 min
Response: 19408245
Conc: 14.52 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DS-B


Manual Integrations
APPROVED

Sohil
1/14/2019 3:58:06 PM

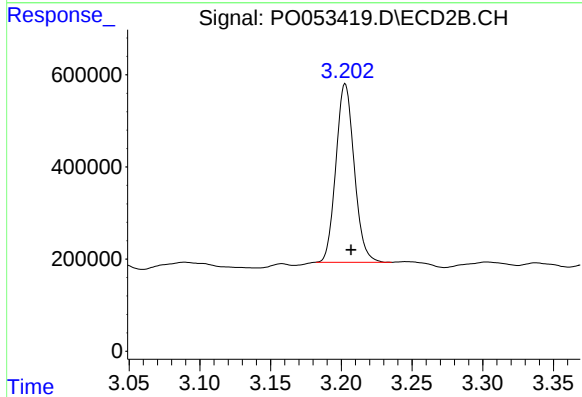


#1 Tetrachloro-m-xylene

R.T.: 3.203 min
Delta R.T.: -0.004 min
Response: 3494804
Conc: 13.98 ng/ml

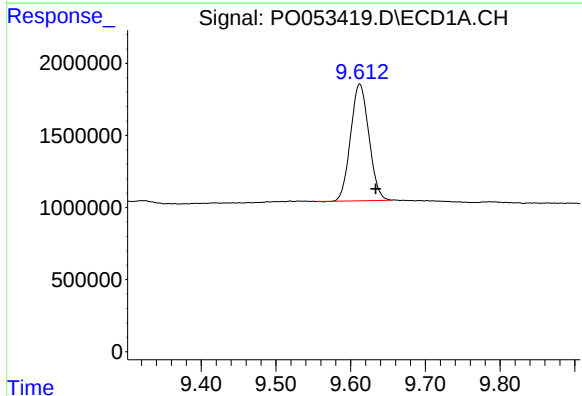

#2 Decachlorobiphenyl

R.T.: 9.612 min
Delta R.T.: -0.021 min
Response: 13745345
Conc: 17.40 ng/ml

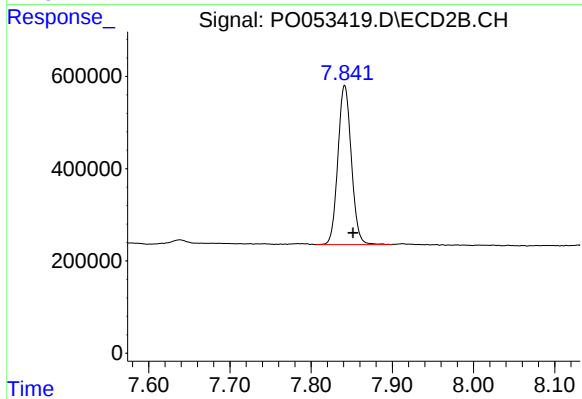

#2 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: -0.011 min
Response: 3970762
Conc: 17.34 ng/ml