

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011419\
 Data File : P0053439.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 Jan 2019 16:08
 Operator : SM/SJ
 Sample : K1087-14
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MH-444-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 14 16:27:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 09 03:34:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.171	3.206	38662953	5973554	28.934	23.890
2) SA Decachlor...	9.623	7.845	12870335	3515261	16.295	15.350

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011419\
Data File : P0053439.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 Jan 2019 16:08
Operator : SM/SJ
Sample : K1087-14
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MH-444-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 14 16:27:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 09 03:34:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

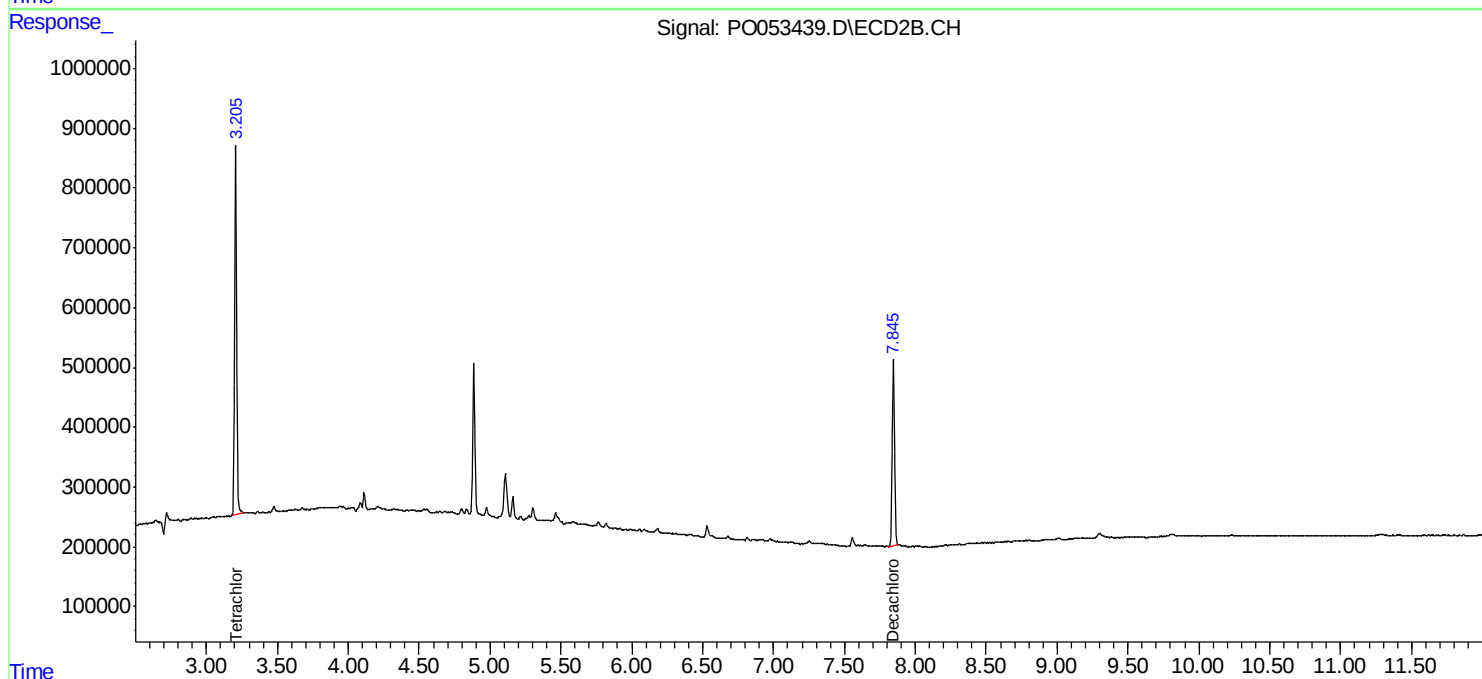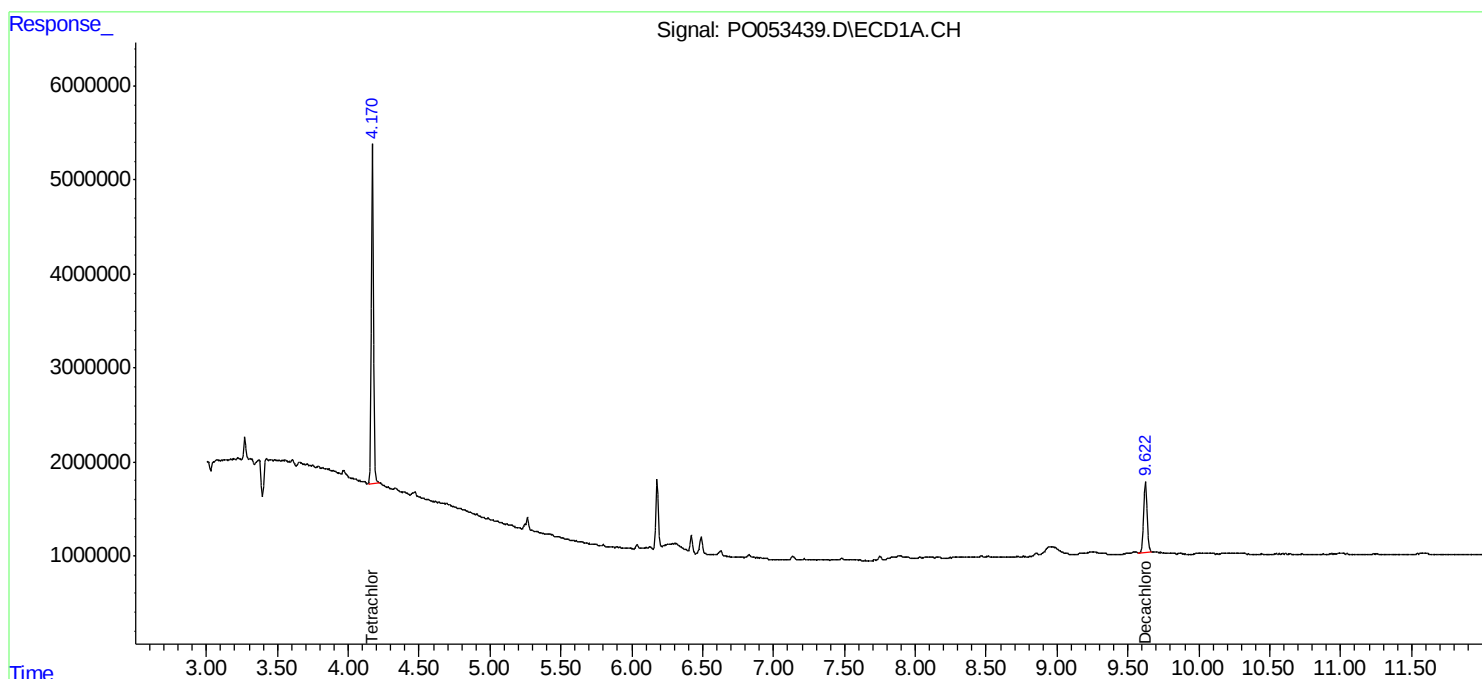


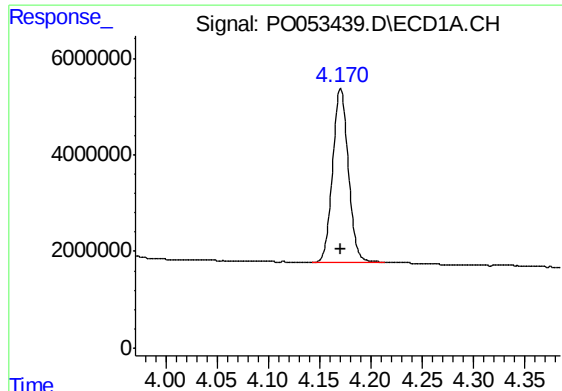

#1 Tetrachloro-m-xylene


R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 38662953
Conc: 28.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-444-C

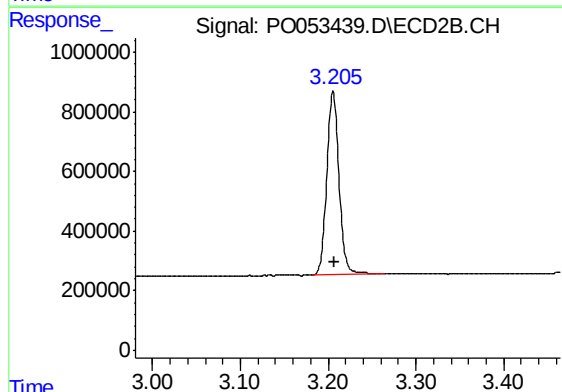


#1 Tetrachloro-m-xylene

R.T.: 3.206 min
Delta R.T.: -0.001 min
Response: 5973554
Conc: 23.89 ng/ml

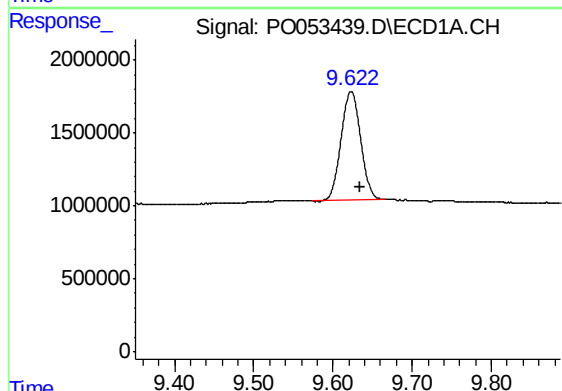

#2 Decachlorobiphenyl

R.T.: 9.623 min
Delta R.T.: -0.011 min
Response: 12870335
Conc: 16.29 ng/ml

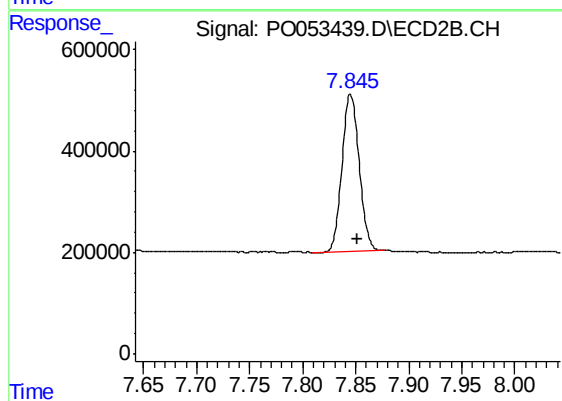

#2 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: -0.007 min
Response: 3515261
Conc: 15.35 ng/ml