

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011519\
 Data File : P0053447.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2019 15:35
 Operator : SM/SJ
 Sample : K1127-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 23832

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 04:04:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 09 03:34:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.165	3.202	16131518	2340189	12.072	9.359
2) SA Decachlor...	9.616	7.842	3498784	1029148	4.430	4.494

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011519\
Data File : P0053447.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2019 15:35
Operator : SM/SJ
Sample : K1127-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
23832

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 04:04:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 09 03:34:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

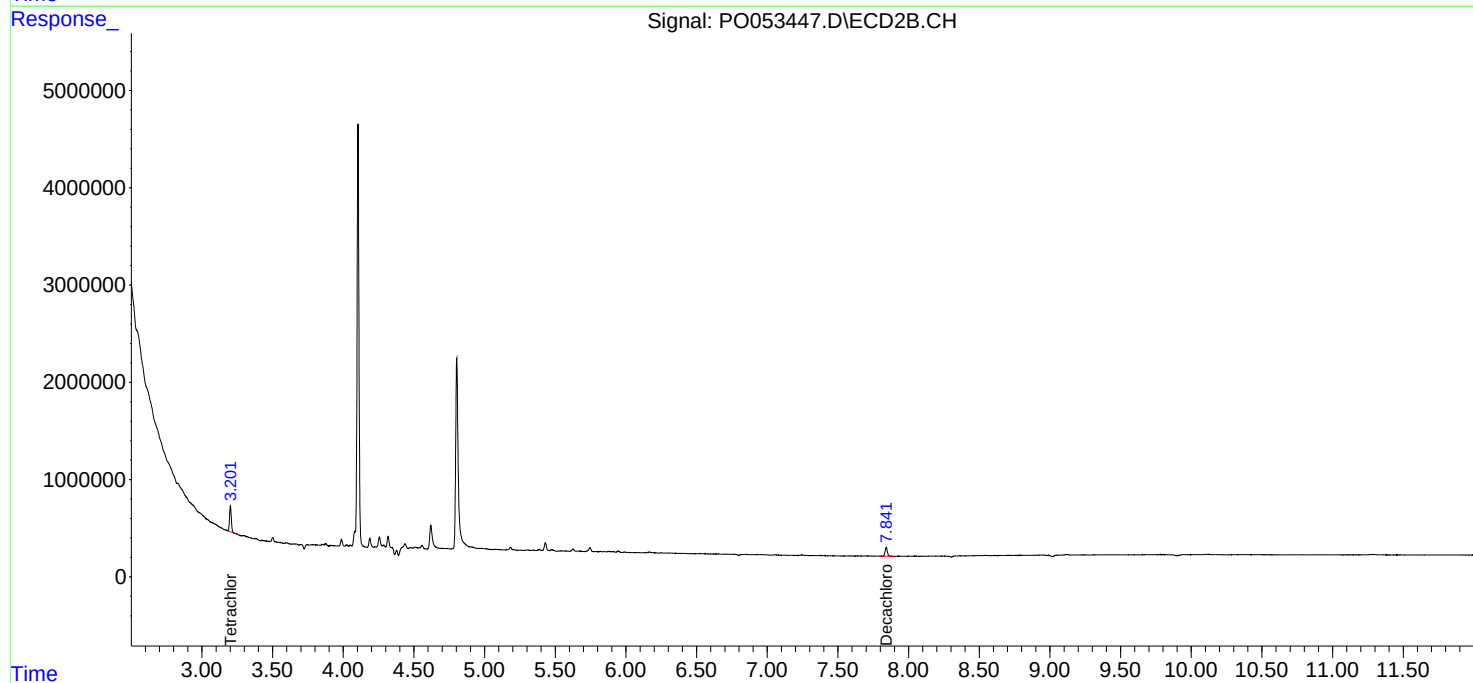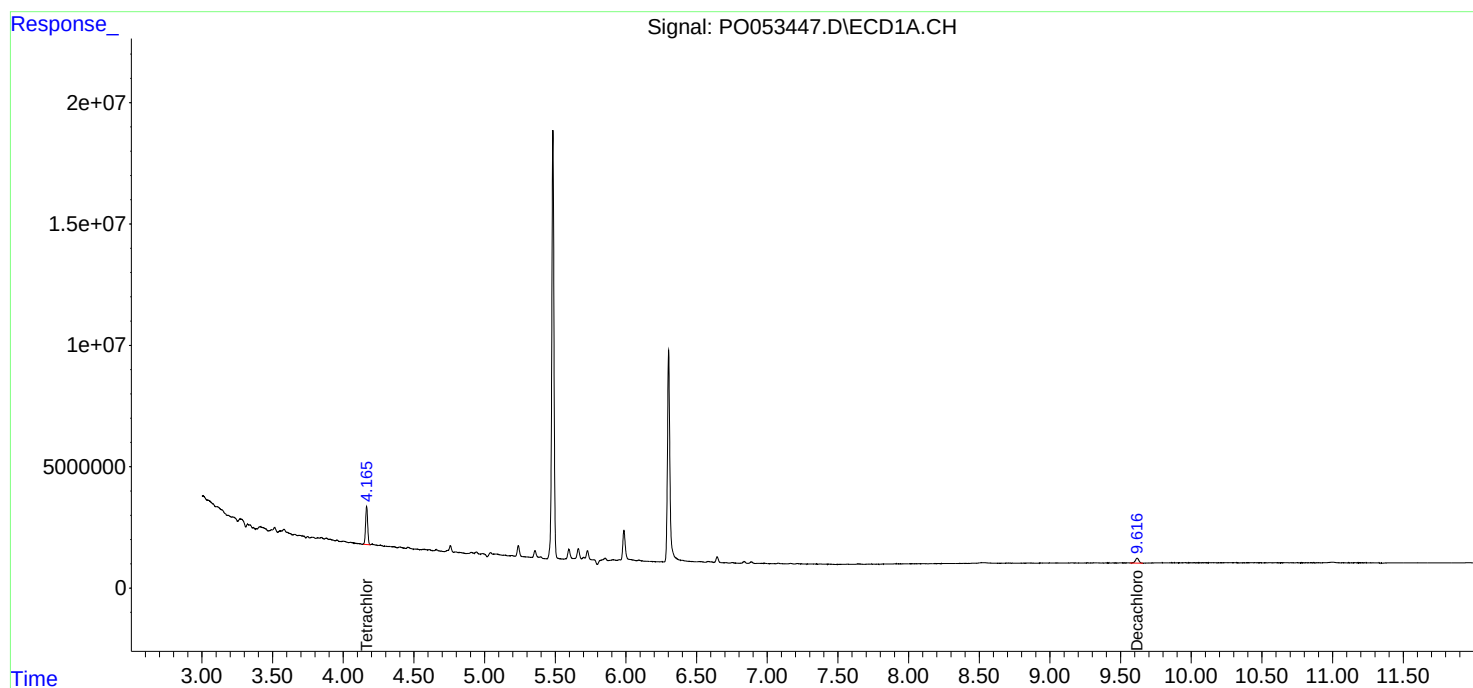


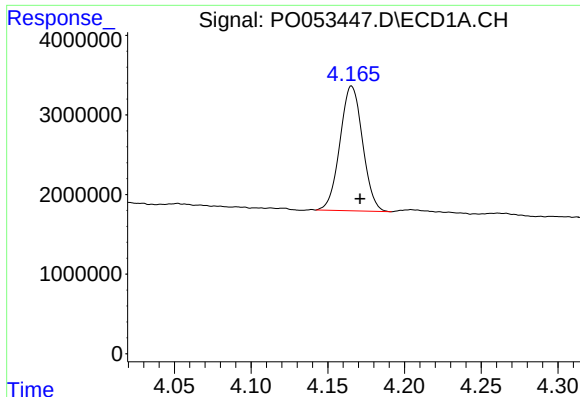

#1 Tetrachloro-m-xylene


R.T.: 4.165 min
Delta R.T.: -0.006 min
Response: 16131518
Conc: 12.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
23832

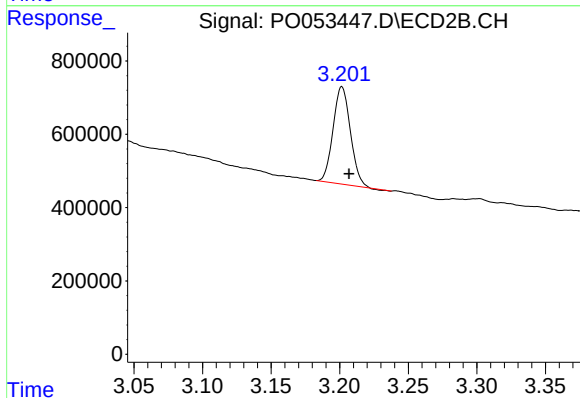


#1 Tetrachloro-m-xylene

R.T.: 3.202 min
Delta R.T.: -0.005 min
Response: 2340189
Conc: 9.36 ng/ml

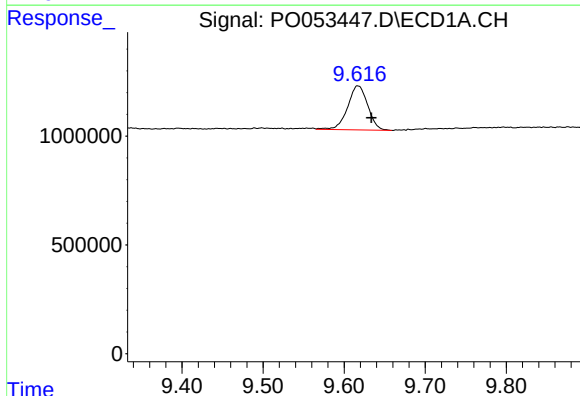

#2 Decachlorobiphenyl

R.T.: 9.616 min
Delta R.T.: -0.017 min
Response: 3498784
Conc: 4.43 ng/ml

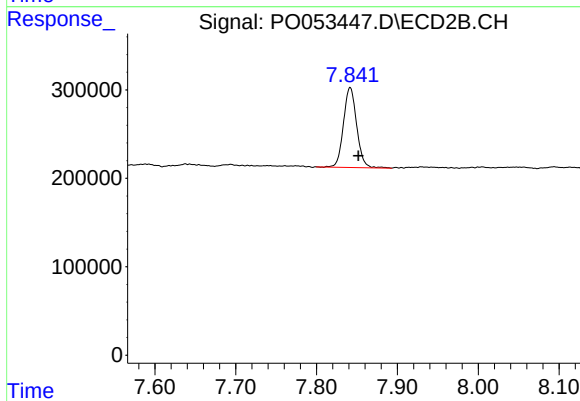

#2 Decachlorobiphenyl

R.T.: 7.842 min
Delta R.T.: -0.010 min
Response: 1029148
Conc: 4.49 ng/ml