

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011519\
 Data File : P0053448.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 Jan 2019 15:52
 Operator : SM/SJ
 Sample : K1127-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 16 04:04:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 09 03:34:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.160	3.201	5302409	766941	3.968	3.067
2) SA Decachlor...	9.607	7.839	2017782	701744	2.555	3.064

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011519\
Data File : P0053448.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 Jan 2019 15:52
Operator : SM/SJ
Sample : K1127-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 16 04:04:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 09 03:34:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

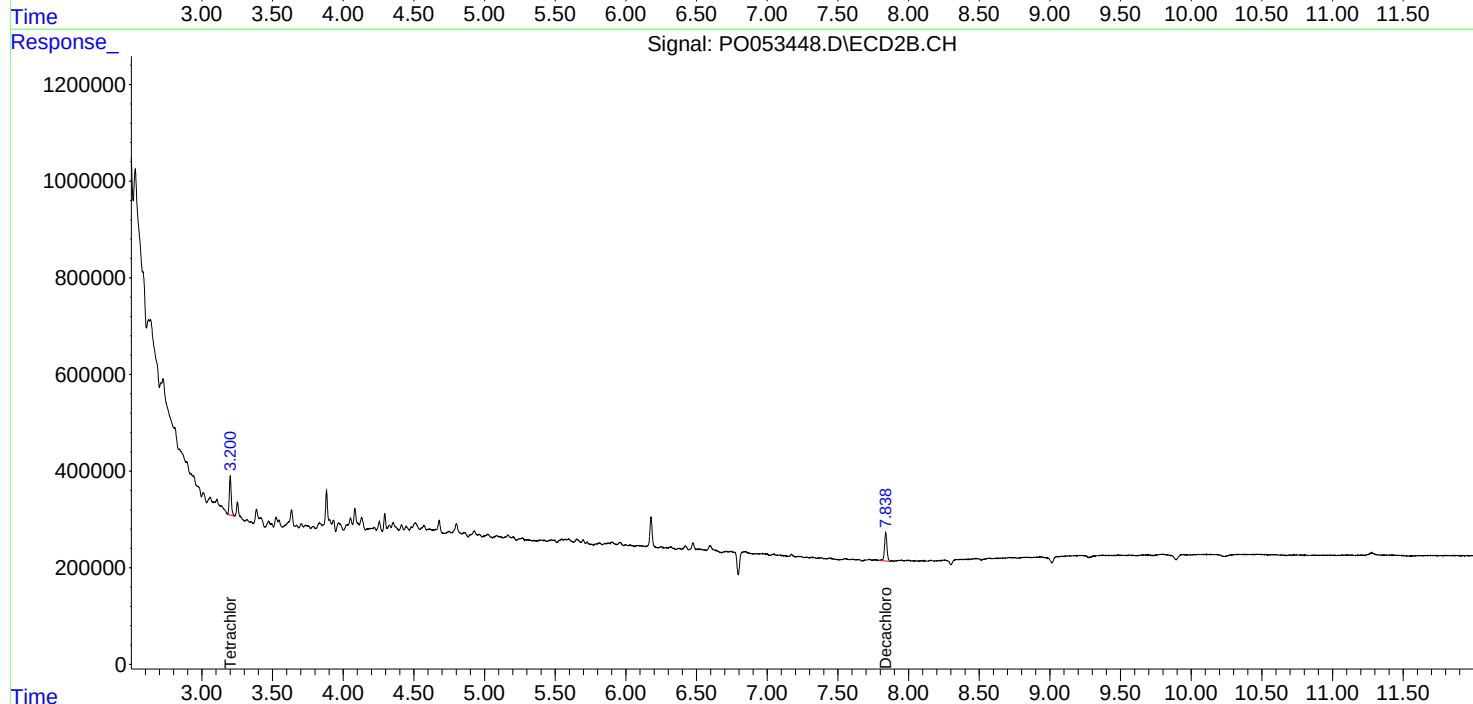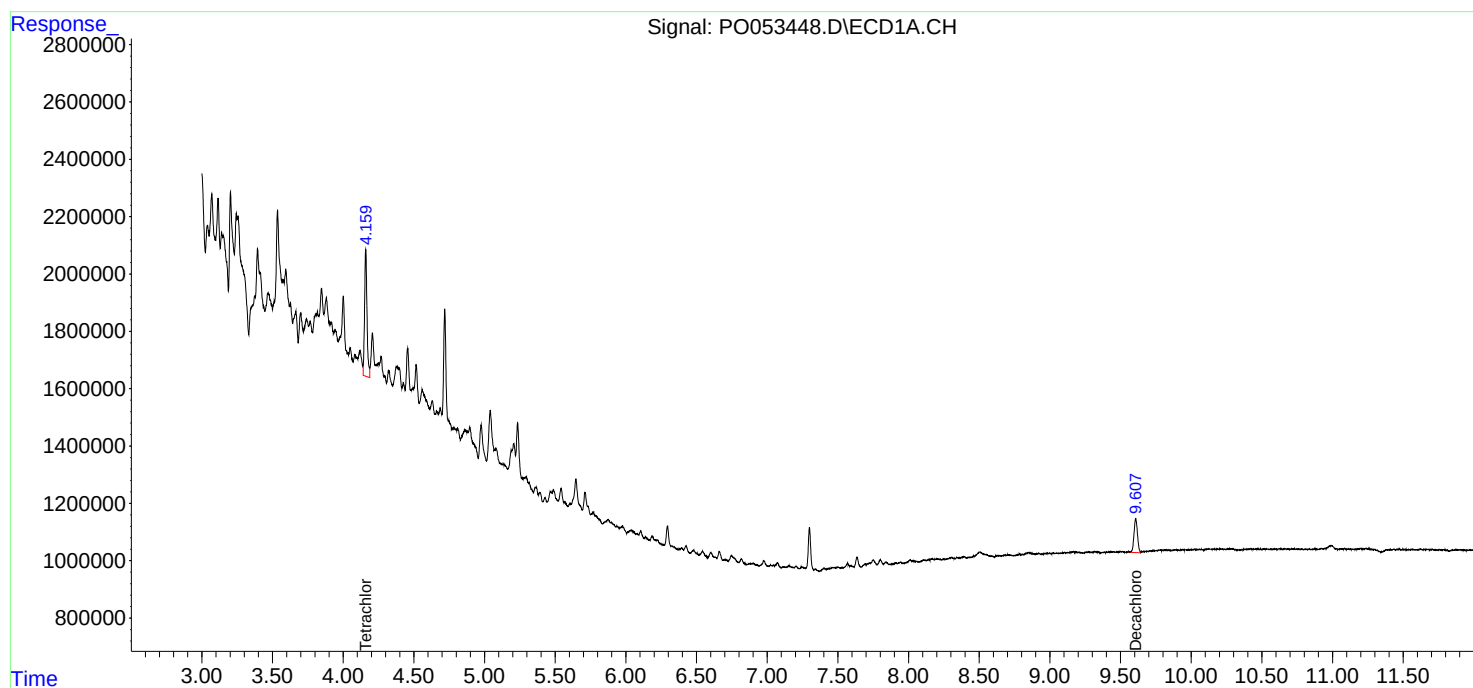


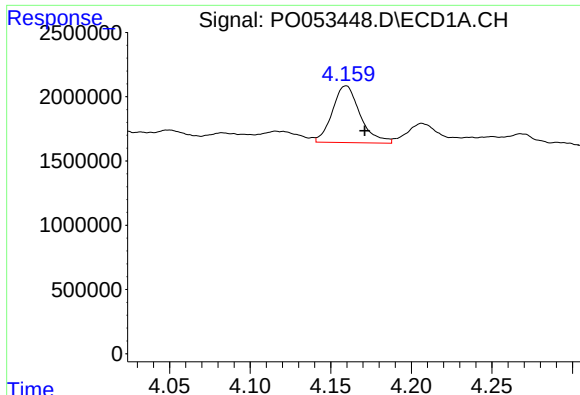

#1 Tetrachloro-m-xylene


R.T.: 4.160 min
Delta R.T.: -0.011 min
Response: 5302409
Conc: 3.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1

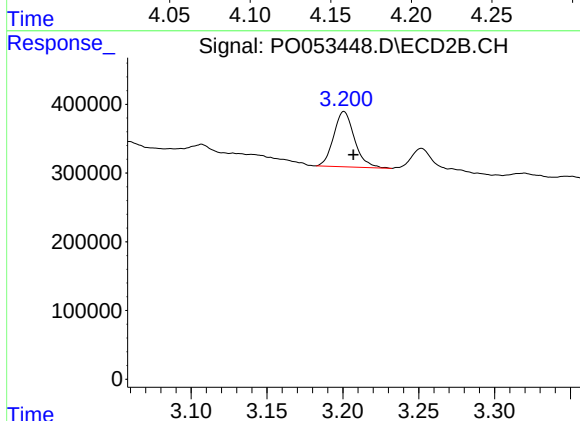


#1 Tetrachloro-m-xylene

R.T.: 3.201 min
Delta R.T.: -0.006 min
Response: 766941
Conc: 3.07 ng/ml

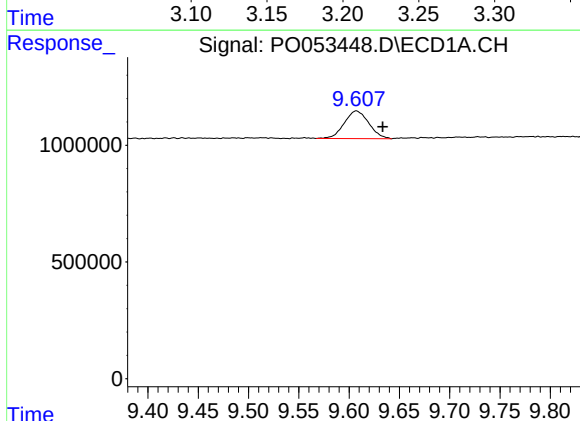

#2 Decachlorobiphenyl

R.T.: 9.607 min
Delta R.T.: -0.026 min
Response: 2017782
Conc: 2.55 ng/ml

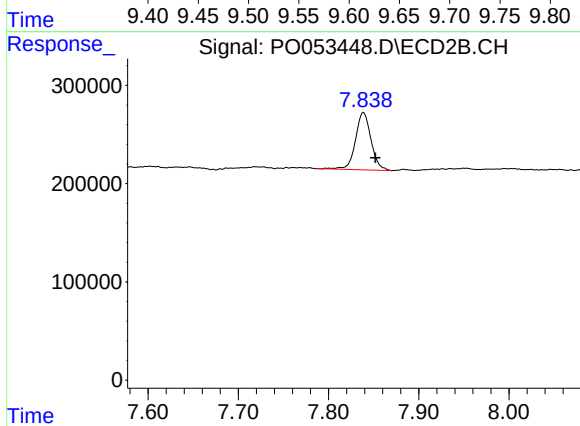

#2 Decachlorobiphenyl

R.T.: 7.839 min
Delta R.T.: -0.013 min
Response: 701744
Conc: 3.06 ng/ml