

Data Path : P:\HPCHEM1\ECD 0\Data\P0012018\
 Data File : P0041572.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jan 2018 11:25
 Operator : SM/UA
 Sample : J1088-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-COMP

Manual Integrations
 APPROVED

ugo
 1/19/2018 9:47:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 19 00:34:16 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0122017.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 20 03:23:29 2017
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.124	3.365	3547473	5606760	17.108	18.190m
2) SA Decachlor...	9.533	8.165	3227597	3930286	15.762	11.098m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\PO012018\
Data File : PO041572.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jan 2018 11:25
Operator : SM/UA
Sample : J1088-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-COMP


Manual Integrations
APPROVED

ugo
1/19/2018 9:47:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 19 00:34:16 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\PO122017.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 20 03:23:29 2017
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

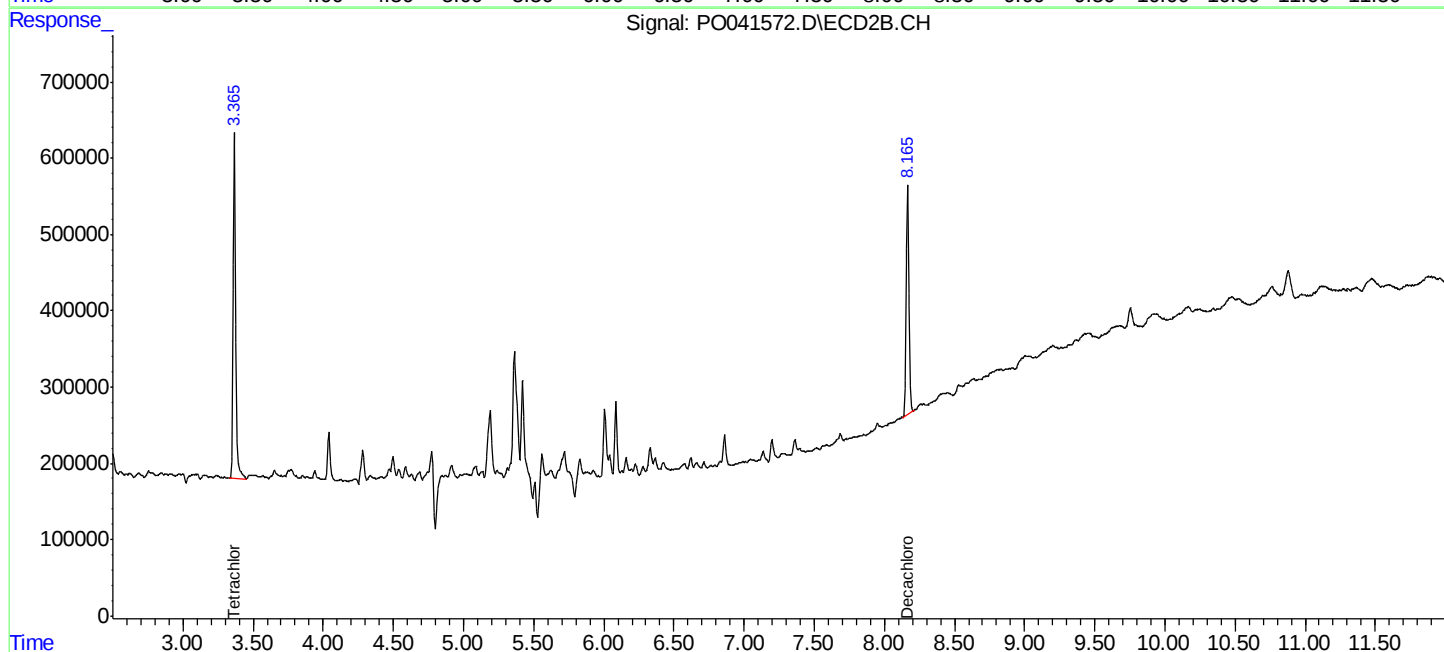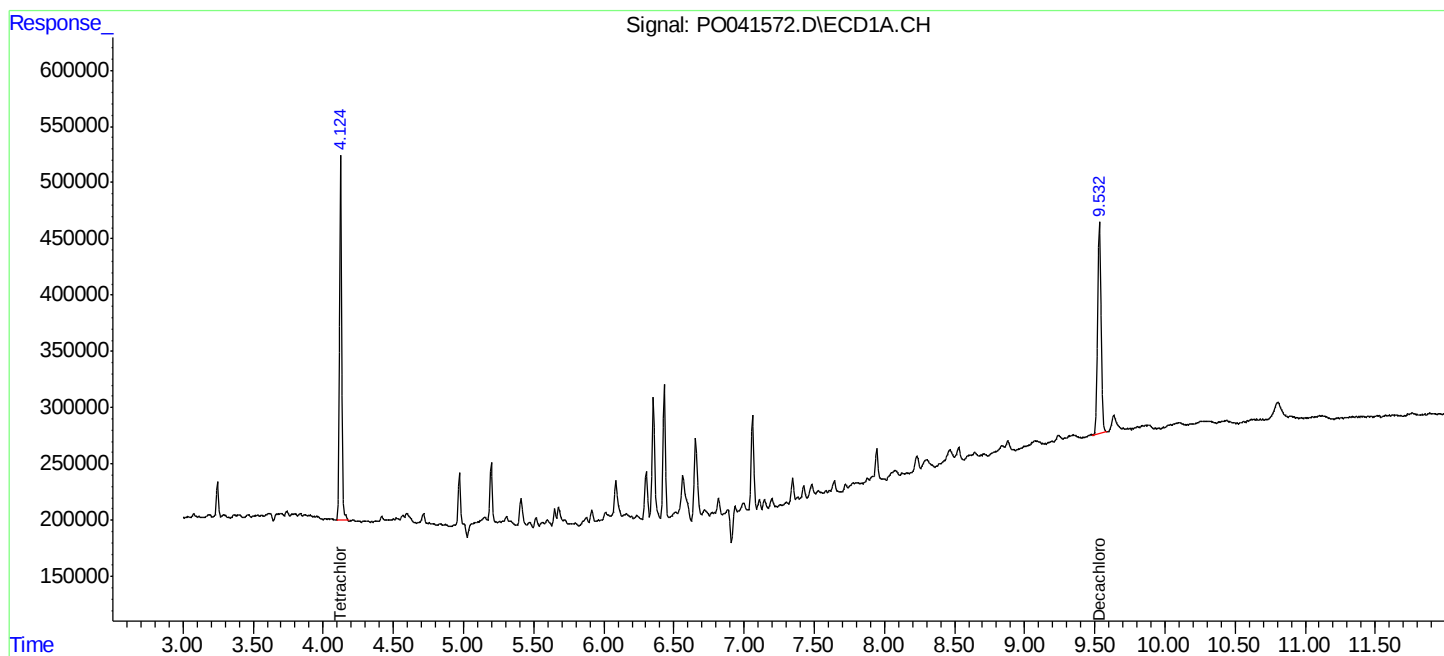

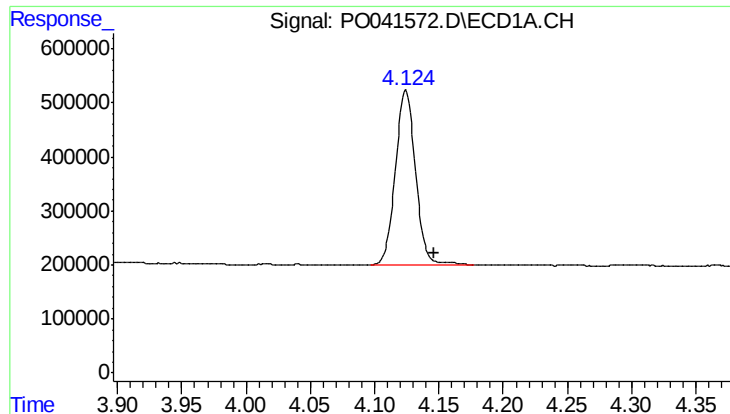


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: -0.022 min
Response: 3547473
Conc: 17.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-COMP


Manual Integrations
APPROVED

ugo
1/19/2018 9:47:38 AM

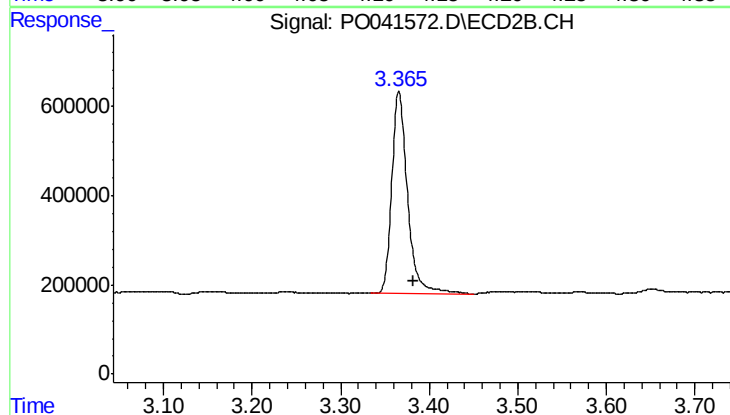


#1 Tetrachloro-m-xylene

R.T.: 3.365 min
Delta R.T.: -0.017 min
Response: 5606760
Conc: 18.19 ng/ml m

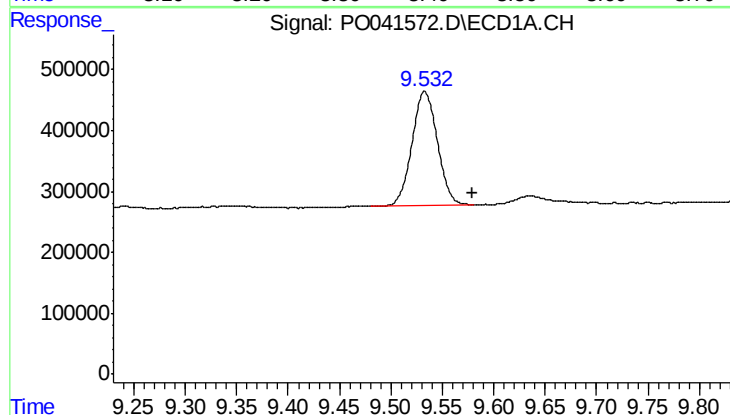

#2 Decachlorobiphenyl

R.T.: 9.533 min
Delta R.T.: -0.046 min
Response: 3227597
Conc: 15.76 ng/ml

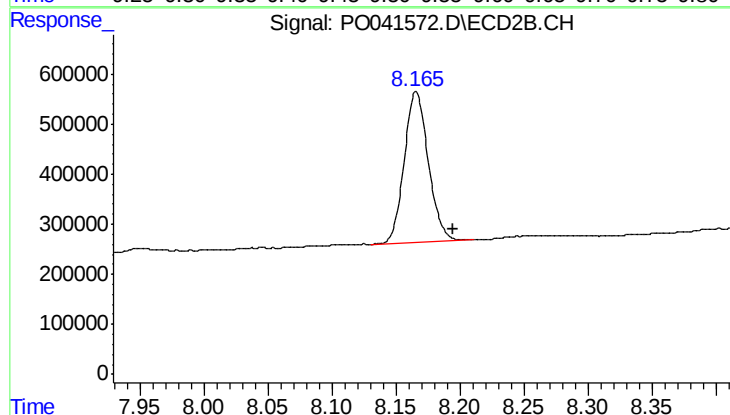

#2 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.030 min
Response: 3930286
Conc: 11.10 ng/ml m