

Data Path : P:\HPCHEM1\ECD_0\Data\P0012218\
 Data File : P0041659.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jan 2018 20:12
 Operator : SM/UA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 01:04:37 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0122017.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Dec 20 03:23:29 2017
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	ugo
System Monitoring Compounds							
1) SA Tetrachlo...	4.124	3.366	3897677	6090373	18.797	19.759m	
2) SA Decachlor...	9.532	8.165	4907793	7004007	23.967	19.777m	1/22/2018 9:28:06 AM

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : P:\HPCHEM1\ECD_0\Data\P0012218\
Data File : P0041659.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jan 2018 20:12
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 01:04:37 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0122017.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Dec 20 03:23:29 2017
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

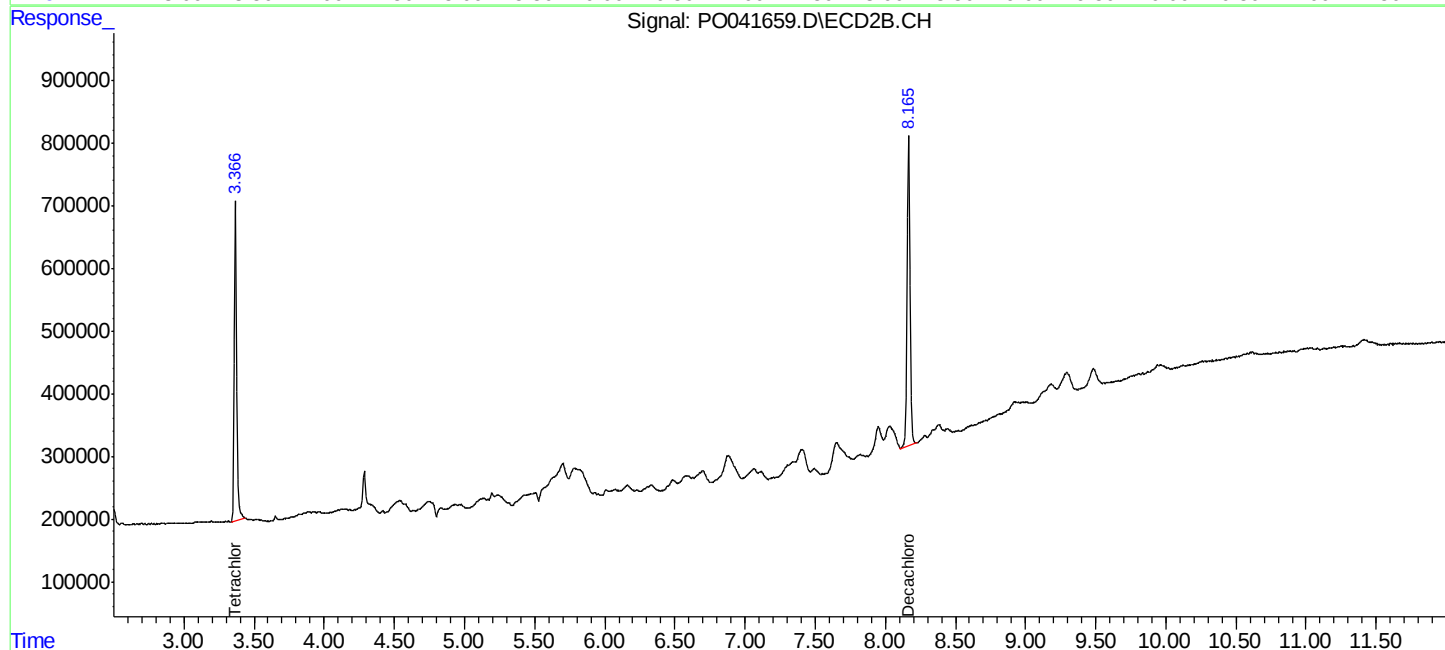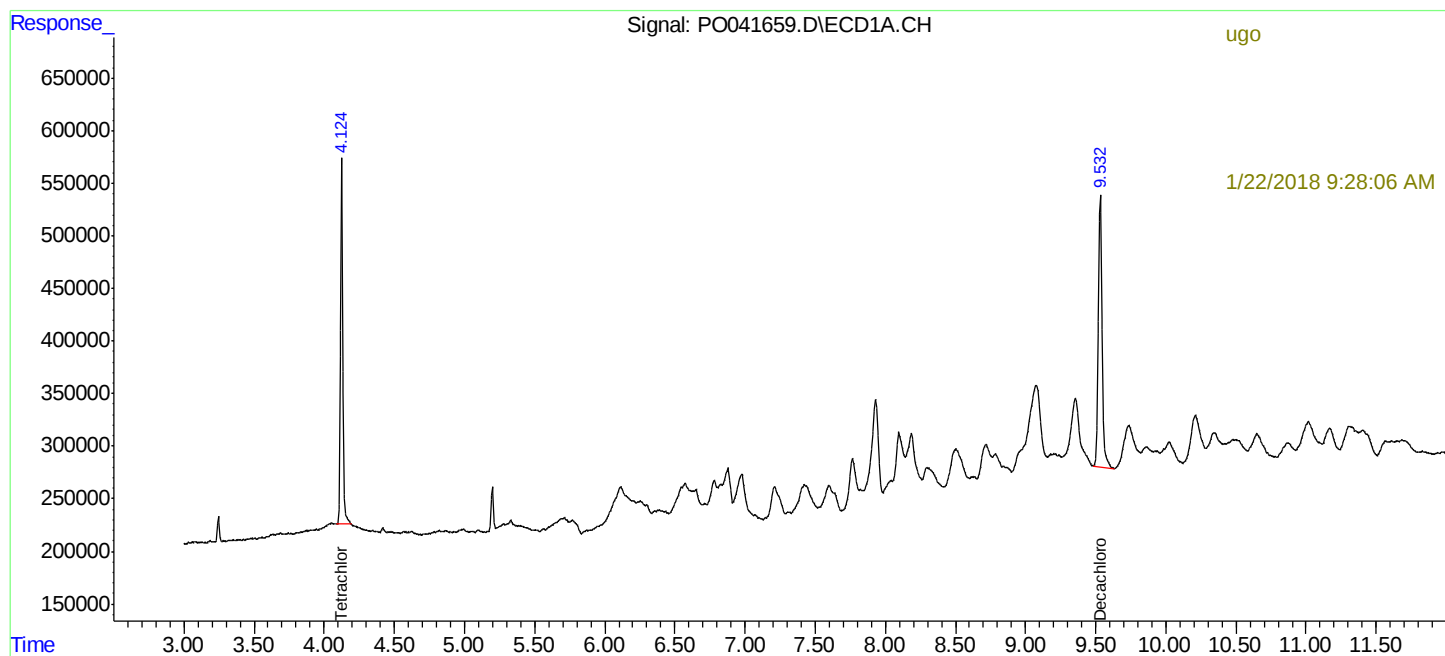

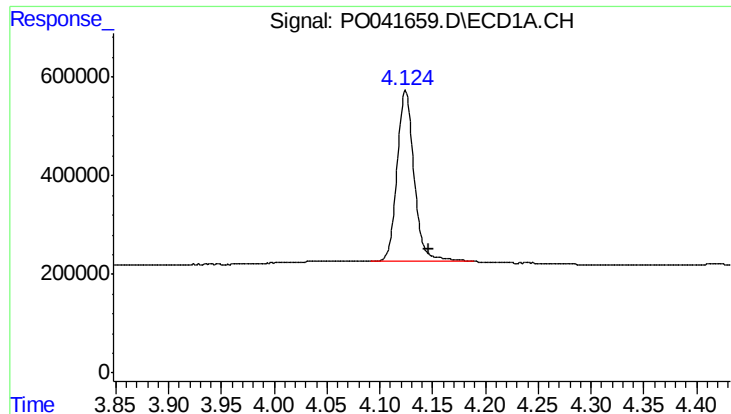


#1 Tetrachloro-m-xylene

R.T.: 4.124 min
Delta R.T.: -0.022 min
Response: 3897677
Conc: 18.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

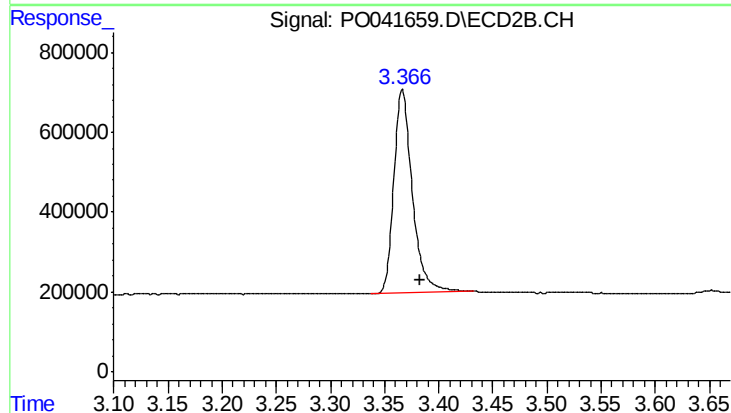

#1 Tetrachloro-m-xylene

R.T.: 3.366 min
Delta R.T.: -0.016 min
Response: 6090373
Conc: 19.76 ng/ml m


ugo

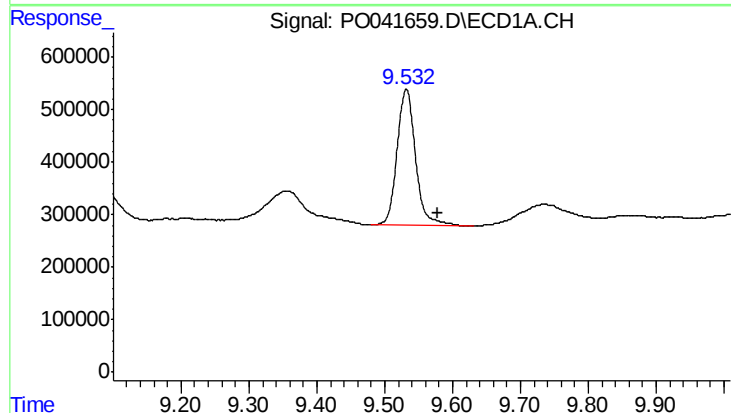

#2 Decachlorobiphenyl

1/22/2018 9:28:06 AM

R.T.: 9.532 min
Delta R.T.: -0.047 min
Response: 4907793
Conc: 23.97 ng/ml

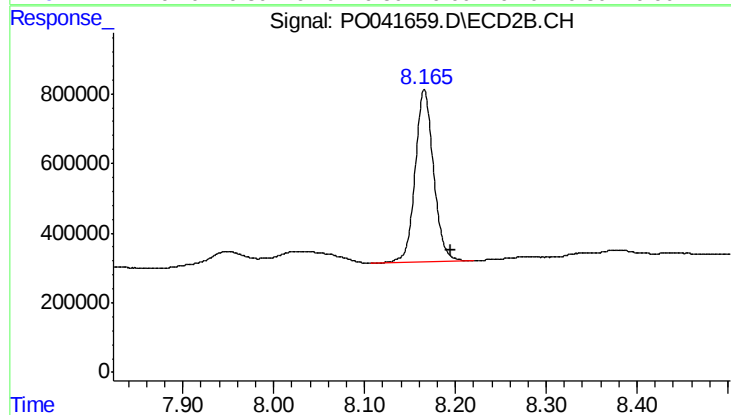

#2 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.030 min
Response: 7004007
Conc: 19.78 ng/ml m