

Data Path : P:\HPCHEM1\ECD 0\Data\P0012318\
Data File : P0041682.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2018 16:28
Operator : SM/UA
Sample : J1202-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ROLLOFF-1-5

Manual Integrations
APPROVED

UGO
1/24/2018 9:26:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 04:52:48 2018
Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.122	3.365	1641206	3195711	8.503m	11.009m#
2) SA Decachlor...	9.525	8.161	1445814	1731910	6.154	4.843m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0012318\
Data File : P0041682.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2018 16:28
Operator : SM/UA
Sample : J1202-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ROLLOFF-1-5


Manual Integrations
APPROVED

UGO
1/24/2018 9:26:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 04:52:48 2018
Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

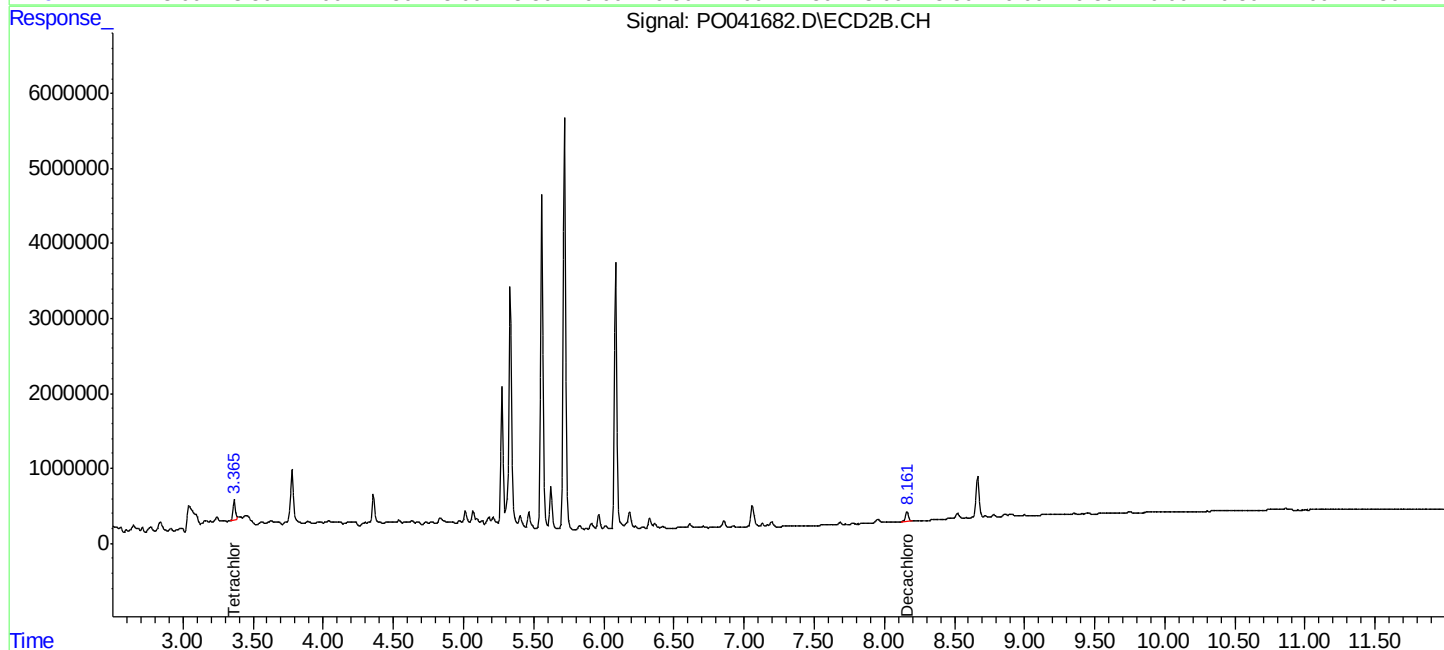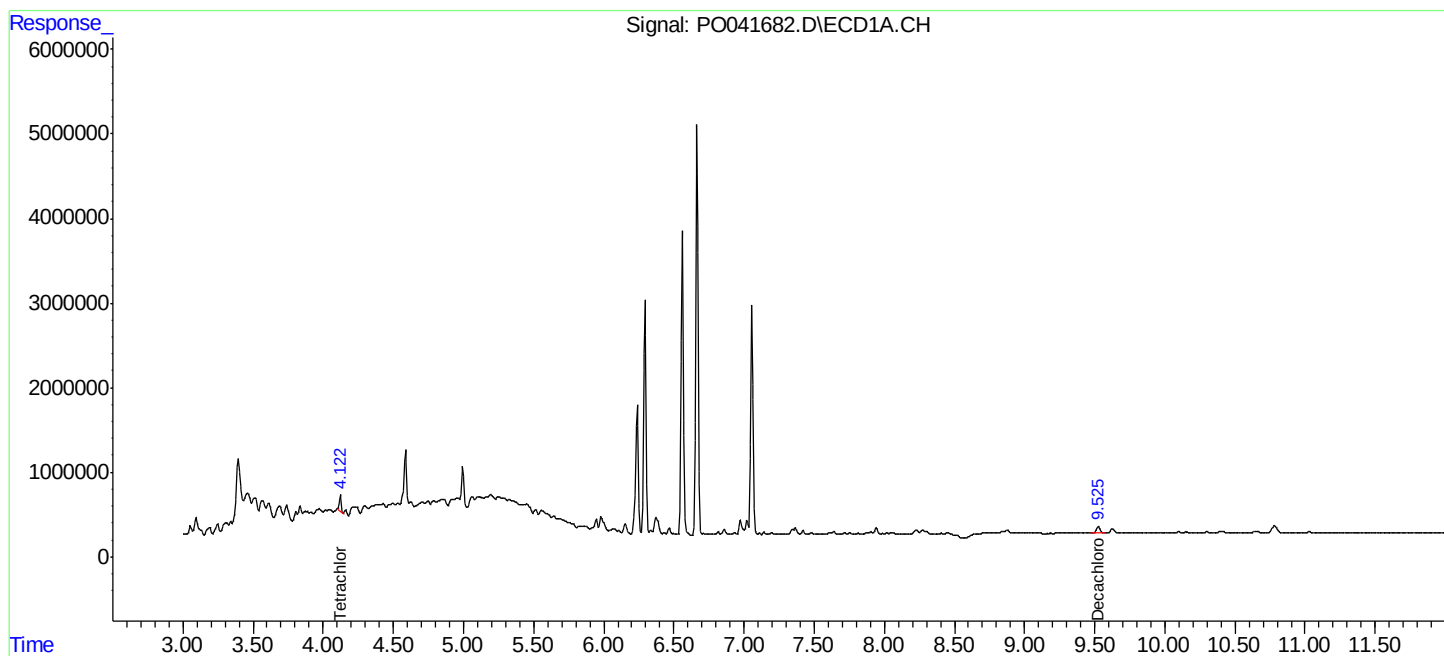

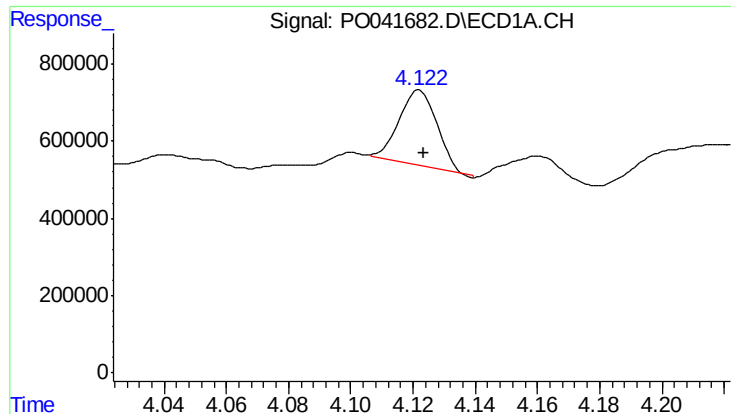


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: -0.001 min
Response: 1641206
Conc: 8.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
ROLLOFF-1-5


Manual Integrations
APPROVED

UGO
1/24/2018 9:26:41 AM

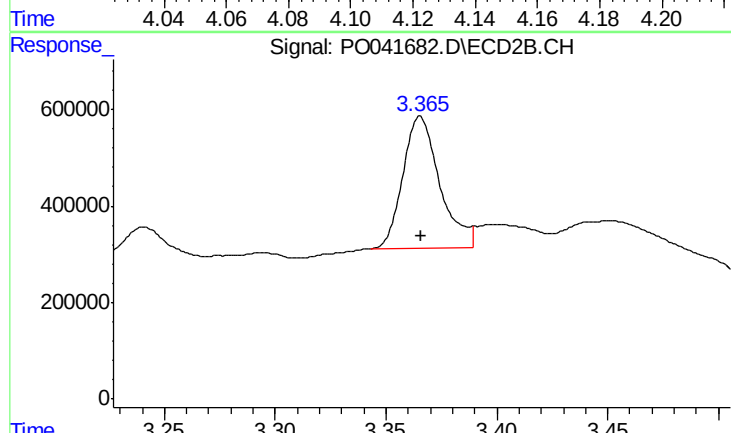


#1 Tetrachloro-m-xylene

R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 3195711
Conc: 11.01 ng/ml m

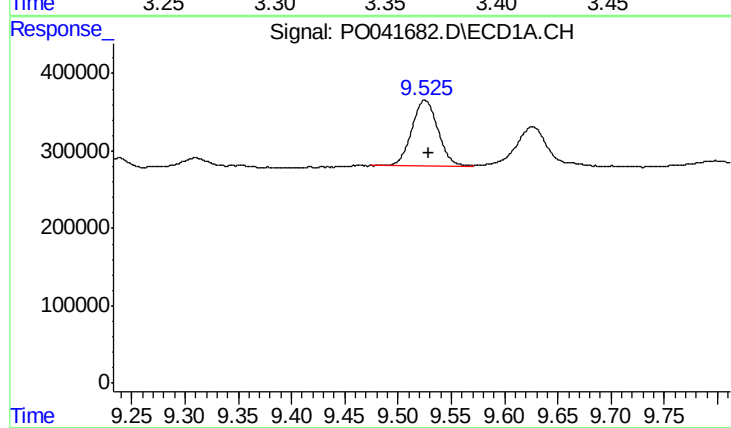

#2 Decachlorobiphenyl

R.T.: 9.525 min
Delta R.T.: -0.003 min
Response: 1445814
Conc: 6.15 ng/ml

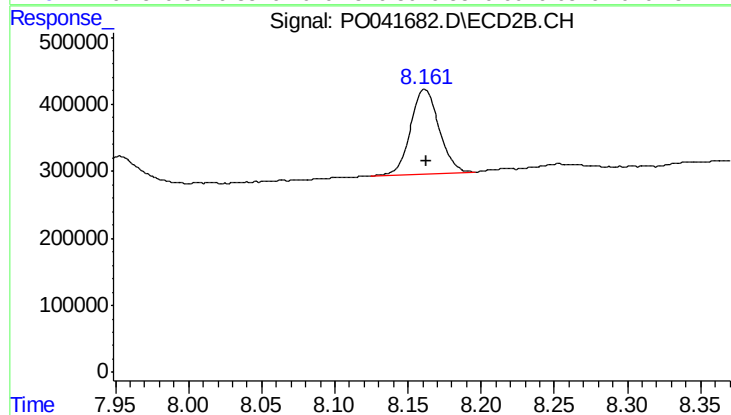

#2 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: -0.002 min
Response: 1731910
Conc: 4.84 ng/ml m