

Data Path : P:\HPCHEM1\ECD 0\Data\P0012318\
 Data File : P0041708.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2018 23:59
 Operator : SM/UA
 Sample : J1210-07
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 R-4220

Manual Integrations
 APPROVED

UGO
 1/24/2018 9:27:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 06:47:07 2018
 Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 23 01:50:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.121	3.365	2469959	3963747	12.797m	13.654m
2) SA Decachlor...	9.523	8.162	2386739	3080293	10.158m	8.613m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0012318\
Data File : P0041708.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2018 23:59
Operator : SM/UA
Sample : J1210-07
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
R-4220


Manual Integrations
APPROVED

UGO
1/24/2018 9:27:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 06:47:07 2018
Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

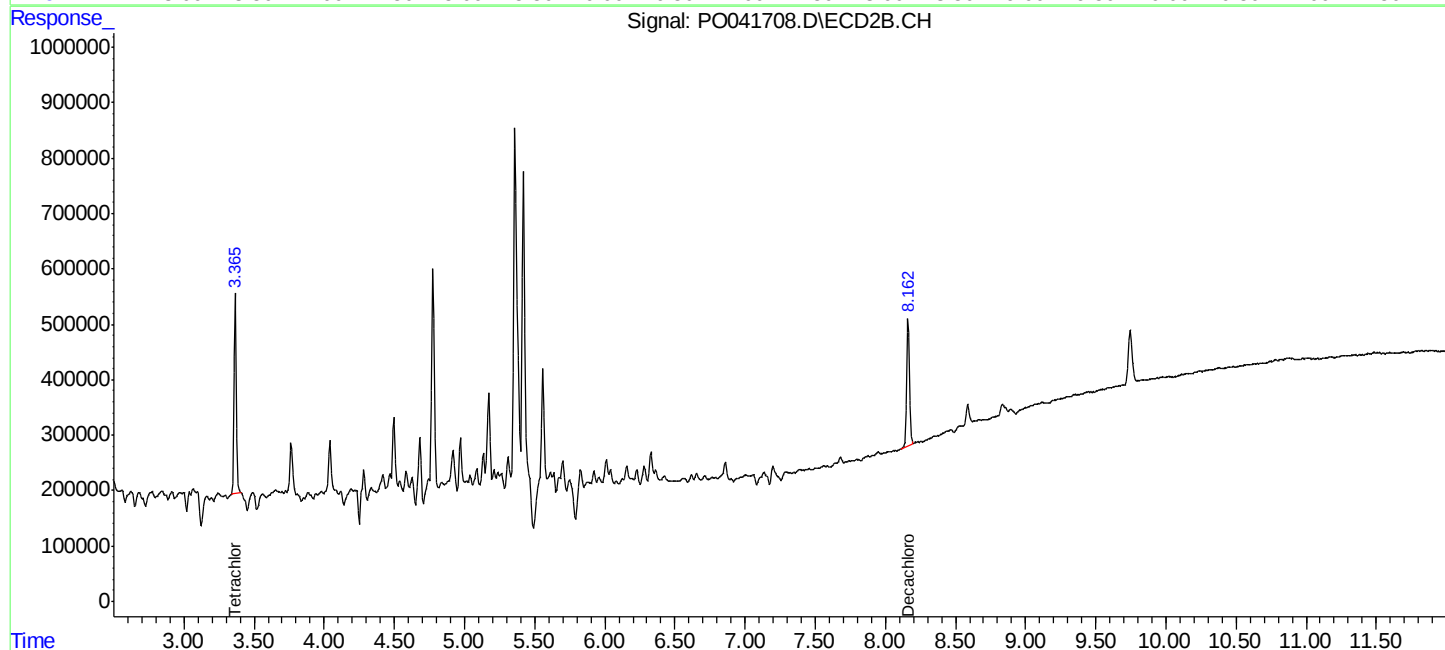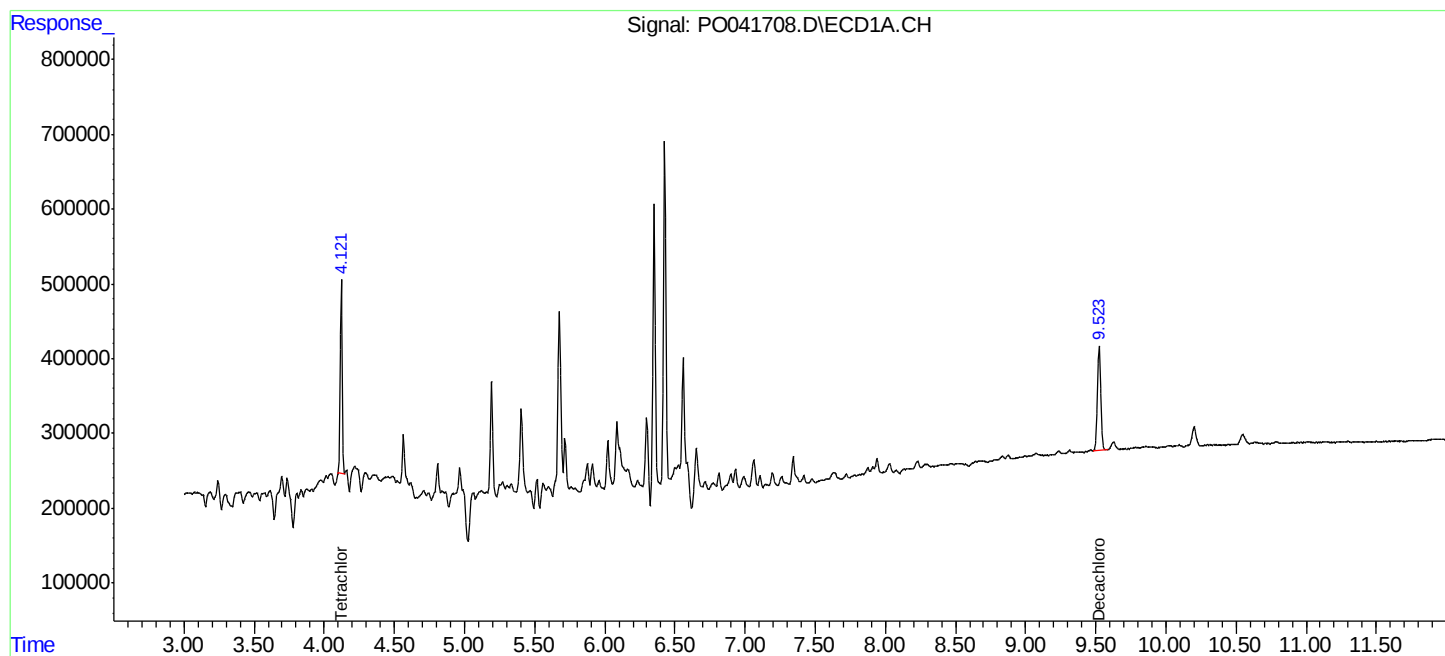

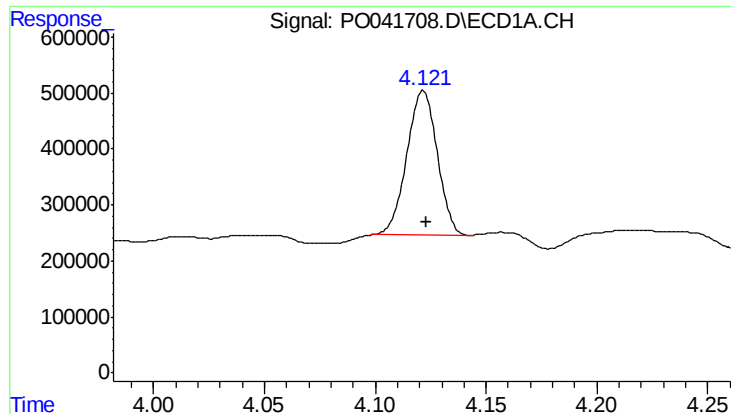


#1 Tetrachloro-m-xylene

R.T.: 4.121 min
Delta R.T.: -0.002 min
Response: 2469959
Conc: 12.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
R-4220


Manual Integrations
APPROVED

UGO
1/24/2018 9:27:21 AM

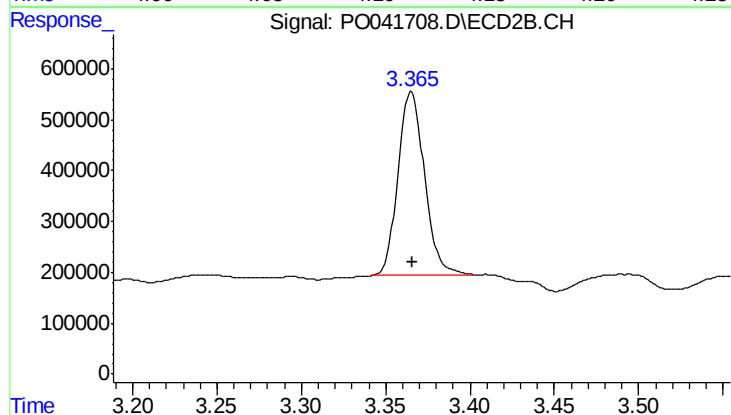


#1 Tetrachloro-m-xylene

R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 3963747
Conc: 13.65 ng/ml m

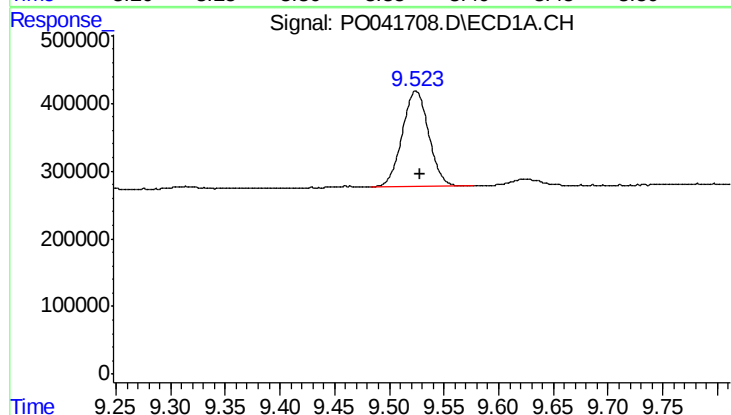

#2 Decachlorobiphenyl

R.T.: 9.523 min
Delta R.T.: -0.006 min
Response: 2386739
Conc: 10.16 ng/ml m

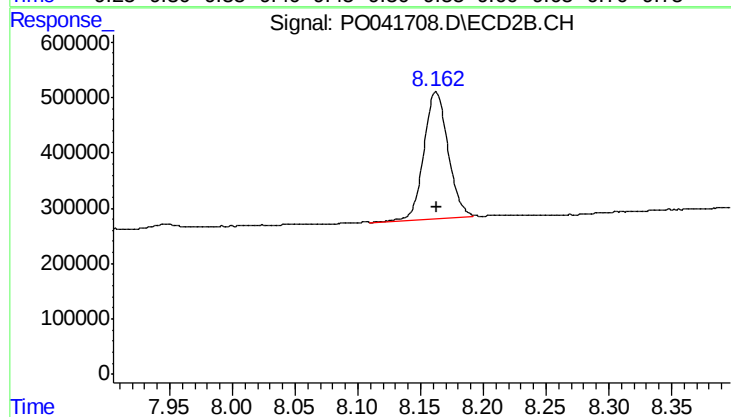

#2 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 3080293
Conc: 8.61 ng/ml m