

Data Path : P:\HPCHEM1\ECD 0\Data\P0012318\
 Data File : P0041727.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jan 2018 4:44
 Operator : SM/UA
 Sample : J1230-07
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CO-1-6

Manual Integrations
 APPROVED

ugo
 1/24/2018 3:23:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 07:03:28 2018
 Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 23 01:50:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.123	3.365	3272438	4946940	16.955	17.041
2) SA Decachlor...	9.528	8.163	3656334	5368544	15.562m	15.012

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0012318\
Data File : P0041727.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jan 2018 4:44
Operator : SM/UA
Sample : J1230-07
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CO-1-6


Manual Integrations
APPROVED

ugo
1/24/2018 3:23:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 07:03:28 2018
Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

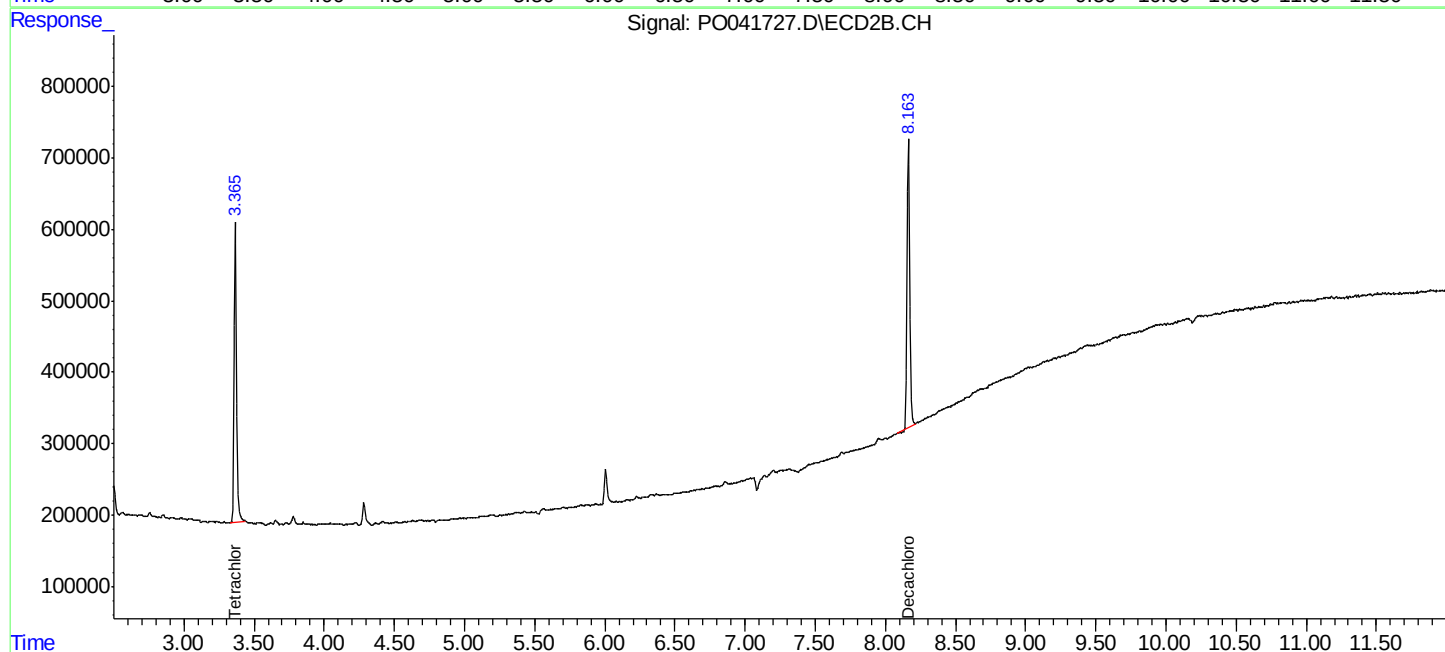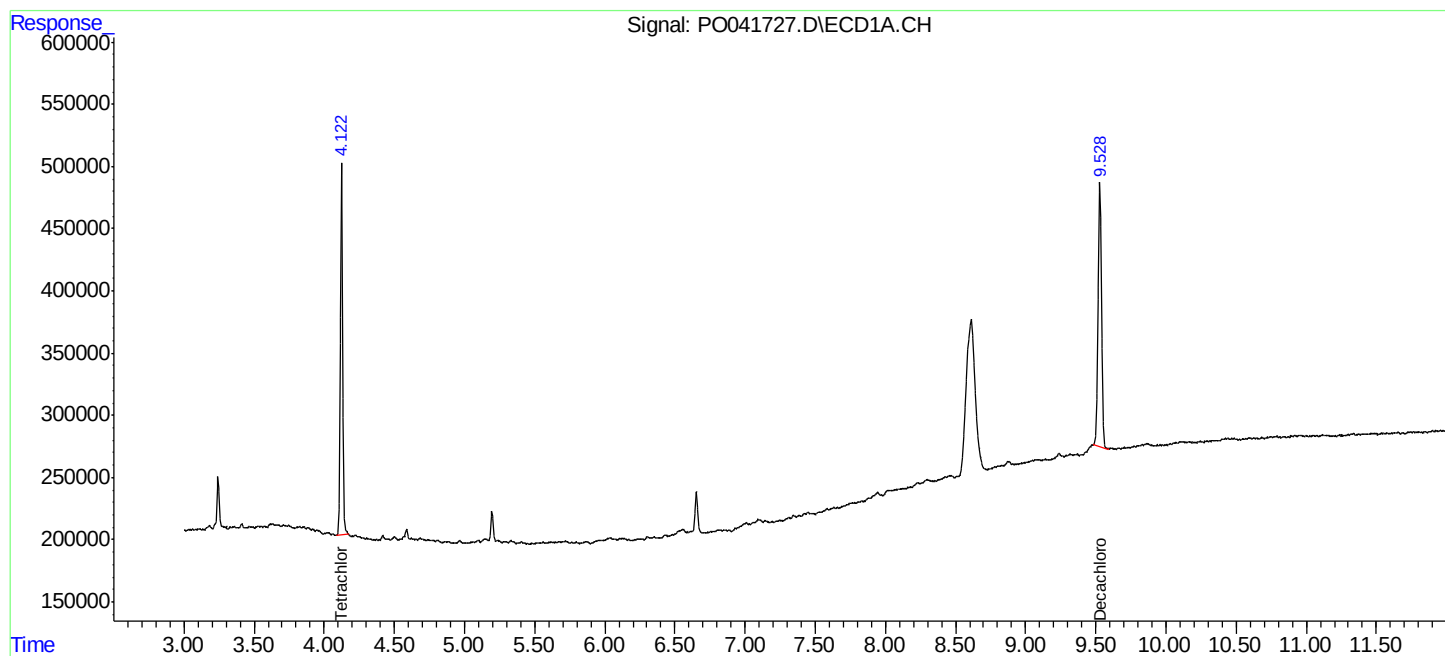

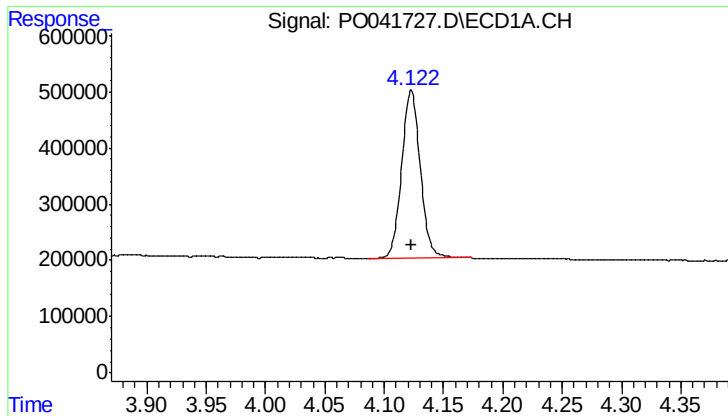


#1 Tetrachloro-m-xylene

R.T.: 4.123 min
Delta R.T.: 0.000 min
Response: 3272438
Conc: 16.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
CO-1-6


Manual Integrations
APPROVED

ugo
1/24/2018 3:23:36 PM

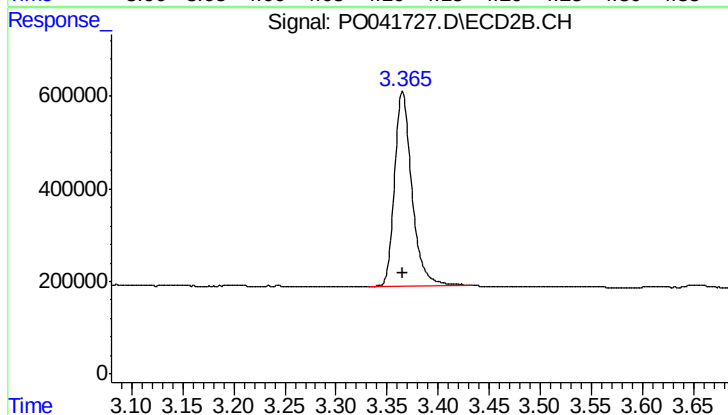


#1 Tetrachloro-m-xylene

R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 4946940
Conc: 17.04 ng/ml

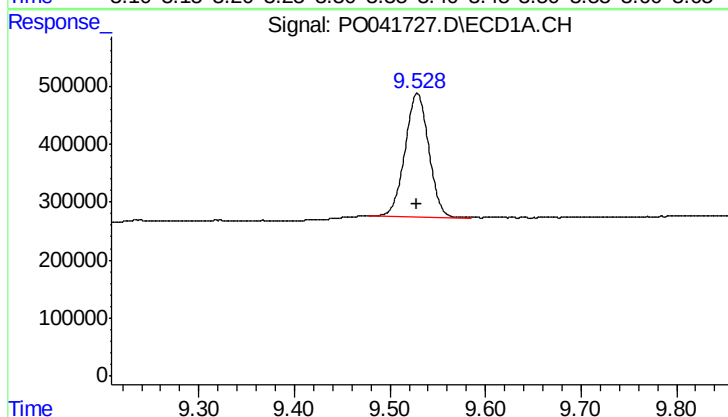

#2 Decachlorobiphenyl

R.T.: 9.528 min
Delta R.T.: 0.000 min
Response: 3656334
Conc: 15.56 ng/ml m

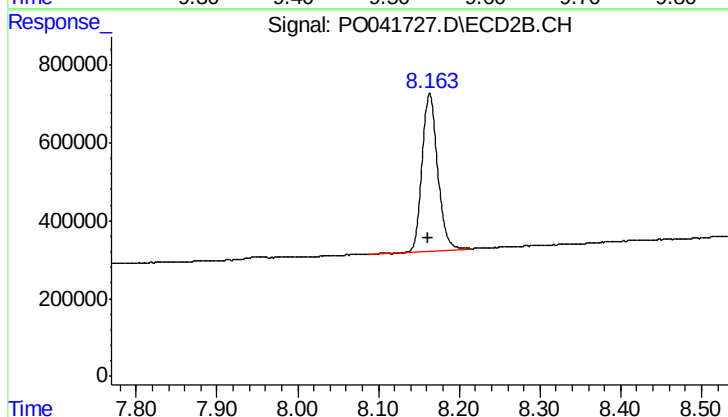

#2 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: 0.000 min
Response: 5368544
Conc: 15.01 ng/ml