

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012519\
 Data File : P0053565.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2019 18:21
 Operator : SM/SJ
 Sample : K1229-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 012319-TIPC-F-D-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 05:40:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jan 28 05:34:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.115	3.173	26015665	4299552	20.078	18.121
2)	SA Decachlor...	9.522	7.789	14285647	4131599	16.321	16.519

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012519\
Data File : P0053565.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2019 18:21
Operator : SM/SJ
Sample : K1229-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
012319-TIPC-F-D-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 05:40:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jan 28 05:34:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

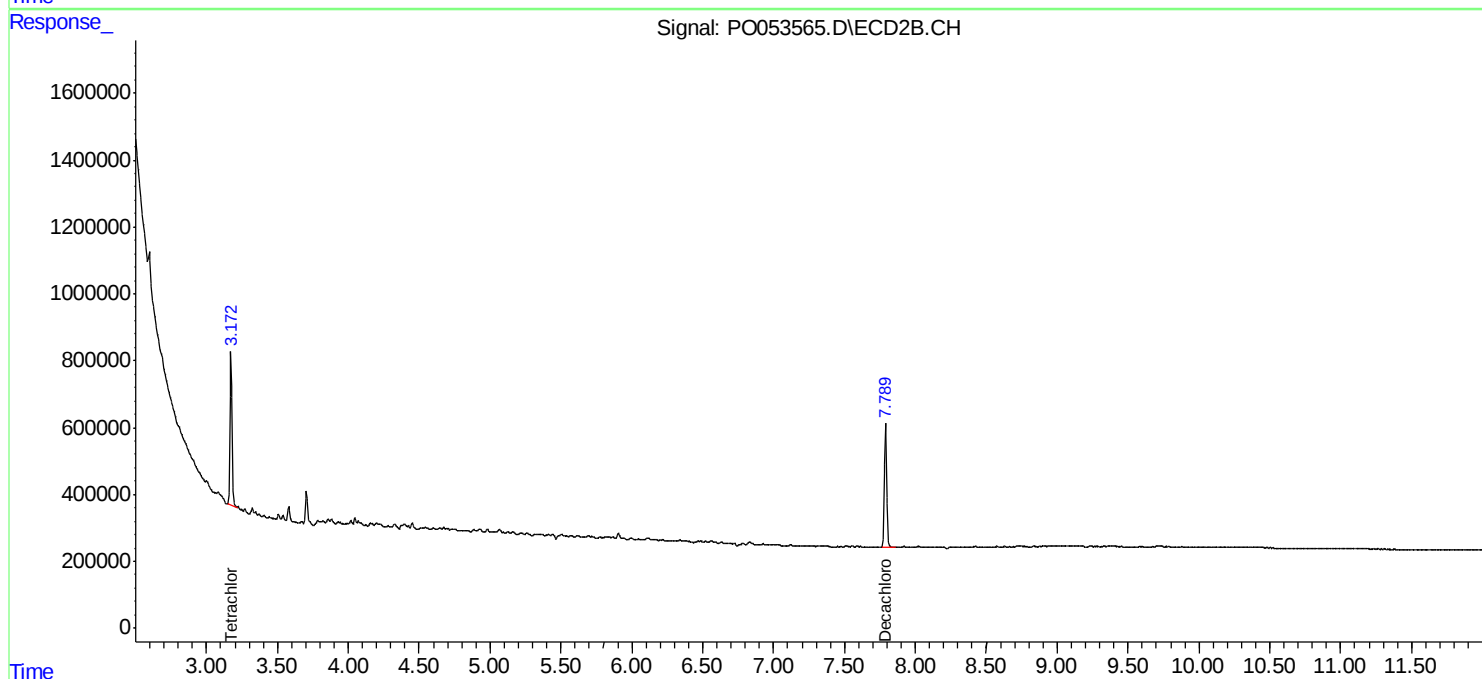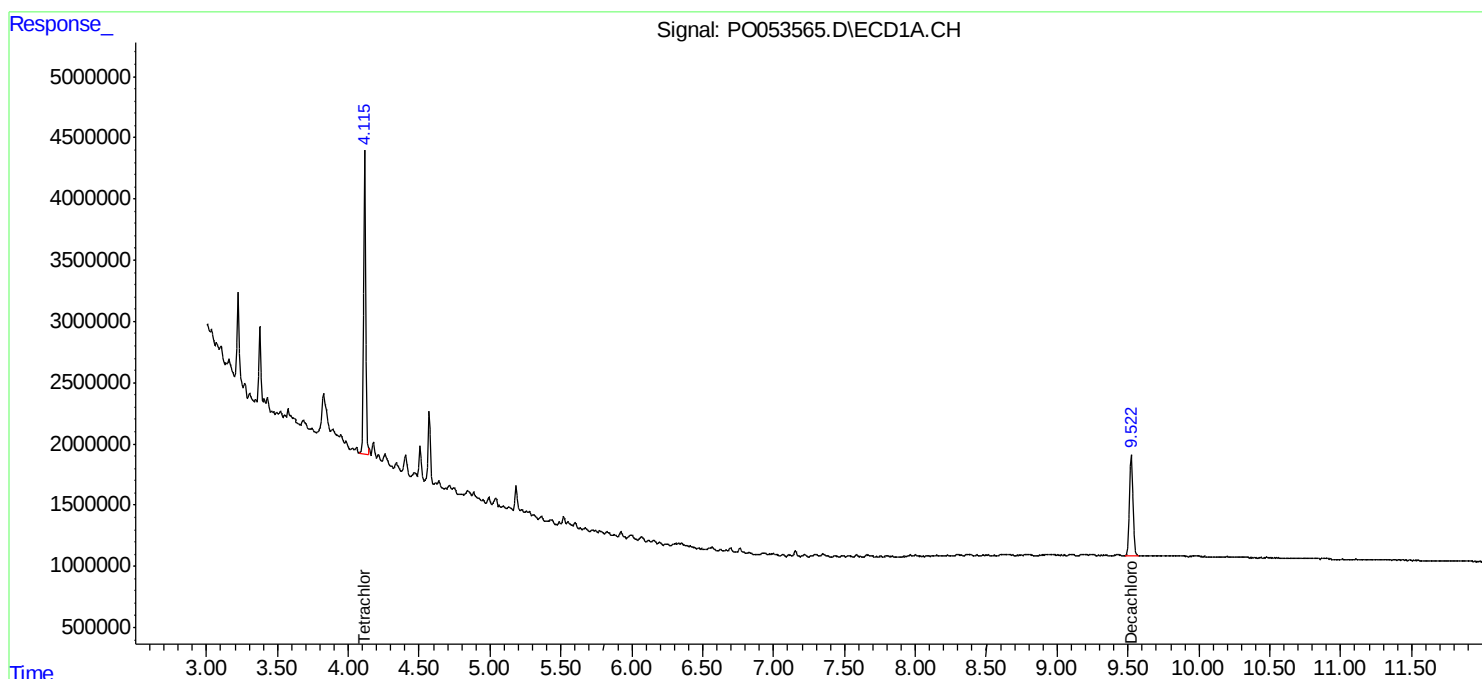


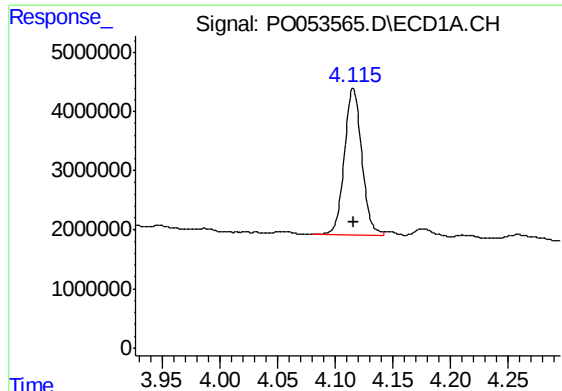

#1 Tetrachloro-m-xylene


R.T.: 4.115 min
Delta R.T.: 0.000 min
Response: 26015665
Conc: 20.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
012319-TIPC-F-D-B

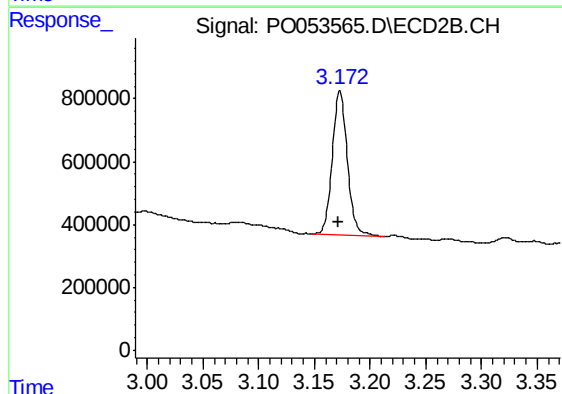


#1 Tetrachloro-m-xylene

R.T.: 3.173 min
Delta R.T.: 0.001 min
Response: 4299552
Conc: 18.12 ng/ml

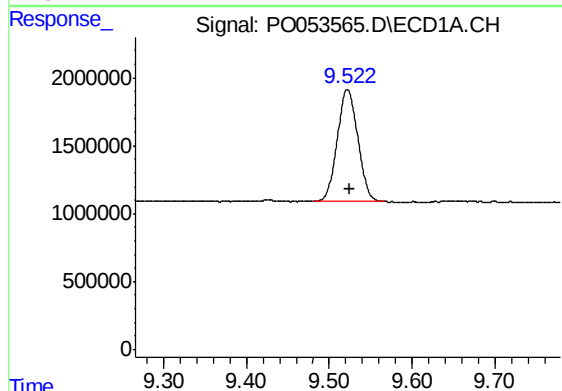

#2 Decachlorobiphenyl

R.T.: 9.522 min
Delta R.T.: -0.002 min
Response: 14285647
Conc: 16.32 ng/ml

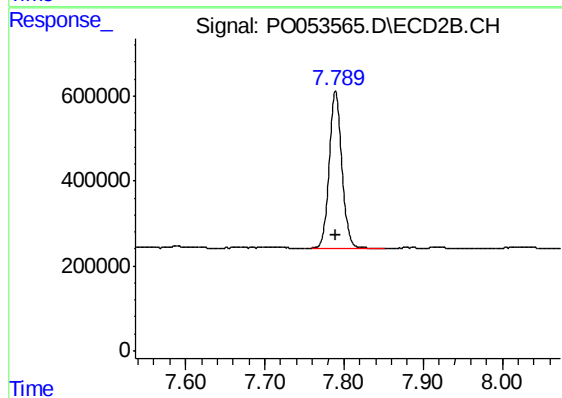

#2 Decachlorobiphenyl

R.T.: 7.789 min
Delta R.T.: 0.000 min
Response: 4131599
Conc: 16.52 ng/ml