

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012519\
 Data File : P0053566.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2019 18:37
 Operator : SM/SJ
 Sample : K1229-02
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 012319-TIPC-F-D-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 05:41:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jan 28 05:34:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.115	3.172	22113877	3977010	17.067	16.762
2) SA Decachlor...	9.523	7.790	12530353	3689036	14.316	14.749

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012519\
Data File : P0053566.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2019 18:37
Operator : SM/SJ
Sample : K1229-02
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
012319-TIPC-F-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 05:41:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jan 28 05:34:06 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

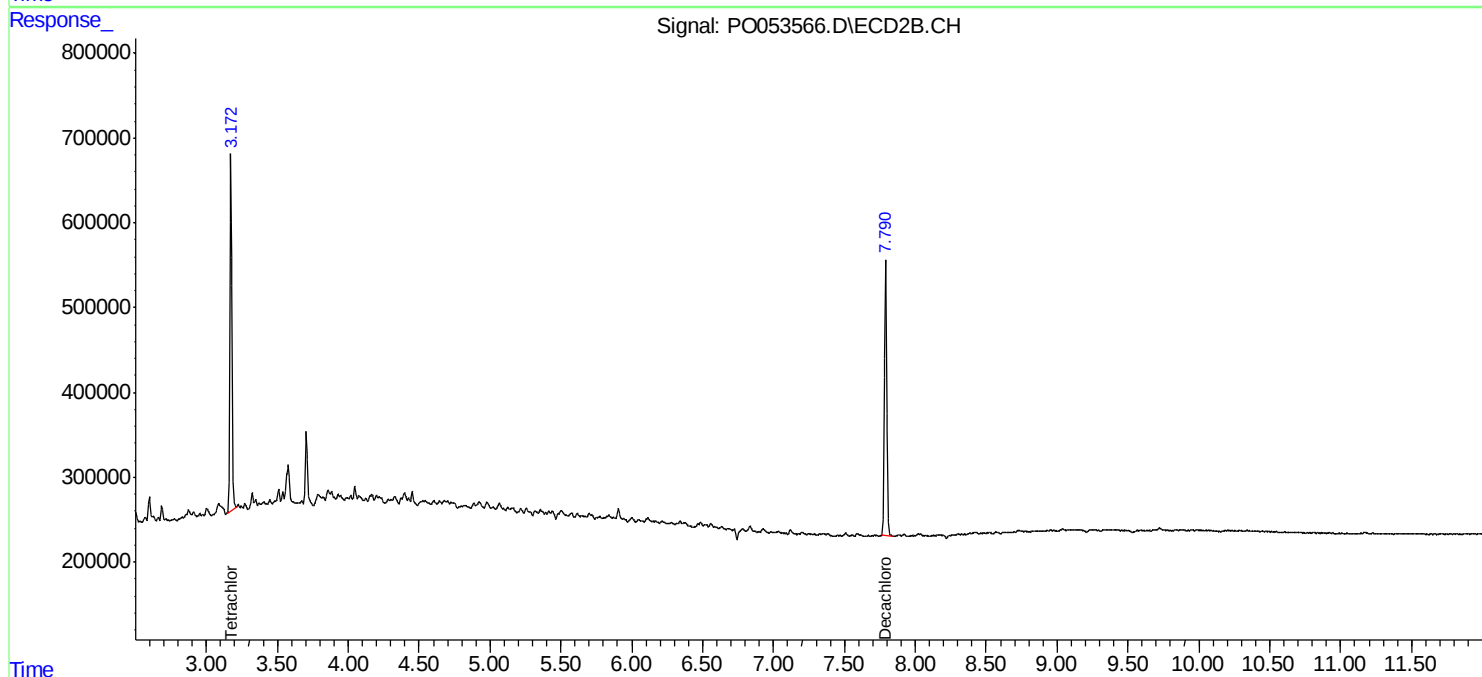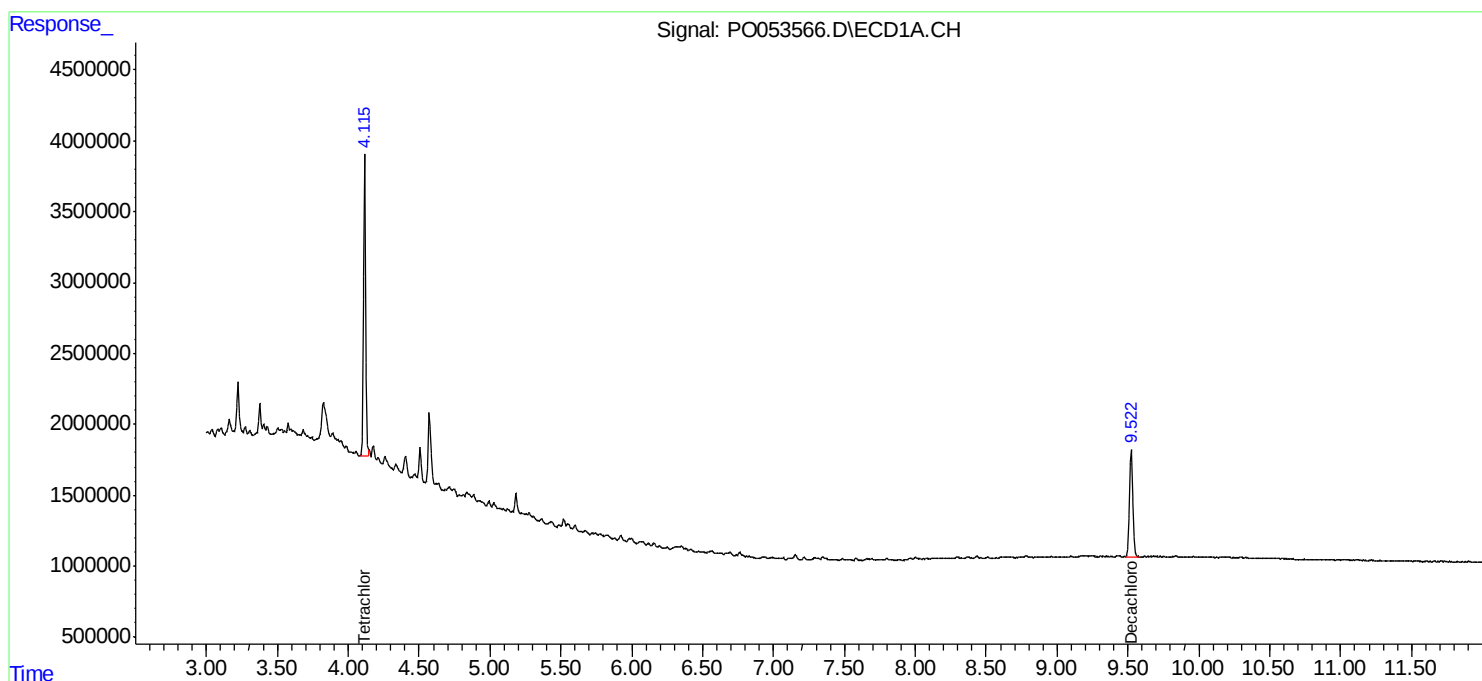


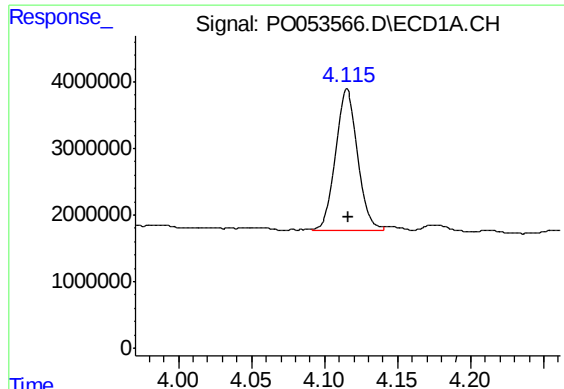

#1 Tetrachloro-m-xylene


R.T.: 4.115 min
Delta R.T.: 0.000 min
Response: 22113877
Conc: 17.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
012319-TIPC-F-D-S

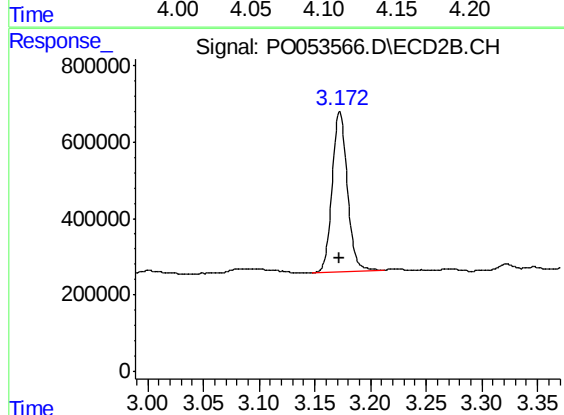


#1 Tetrachloro-m-xylene

R.T.: 3.172 min
Delta R.T.: 0.000 min
Response: 3977010
Conc: 16.76 ng/ml

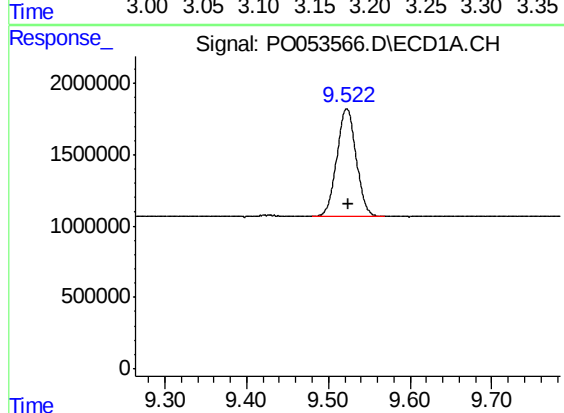

#2 Decachlorobiphenyl

R.T.: 9.523 min
Delta R.T.: -0.001 min
Response: 12530353
Conc: 14.32 ng/ml

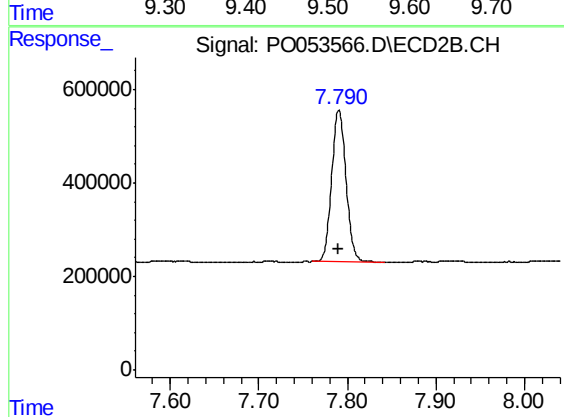

#2 Decachlorobiphenyl

R.T.: 7.790 min
Delta R.T.: 0.000 min
Response: 3689036
Conc: 14.75 ng/ml