

Data Path : P:\HPCHEM1\ECD 0\Data\P0012818\
 Data File : P0041831.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jan 2018 12:47
 Operator : SM/UA
 Sample : J1020-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PL-02-012418-A

Manual Integrations
 APPROVED

ugo
 1/30/2018 10:52:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 13:27:48 2018
 Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 23 01:50:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.119	3.364	3118533	4935180	16.157	17.001
2) SA Decachlor...	9.512	8.156	2654086	2720221	11.296	7.606 #

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\PO012818\
Data File : PO041831.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jan 2018 12:47
Operator : SM/UA
Sample : J1020-09
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PL-02-012418-A


Manual Integrations
APPROVED

ugo
1/30/2018 10:52:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 13:27:48 2018
Quant Method : P:\HPCHEM1\ECD_0\PO012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

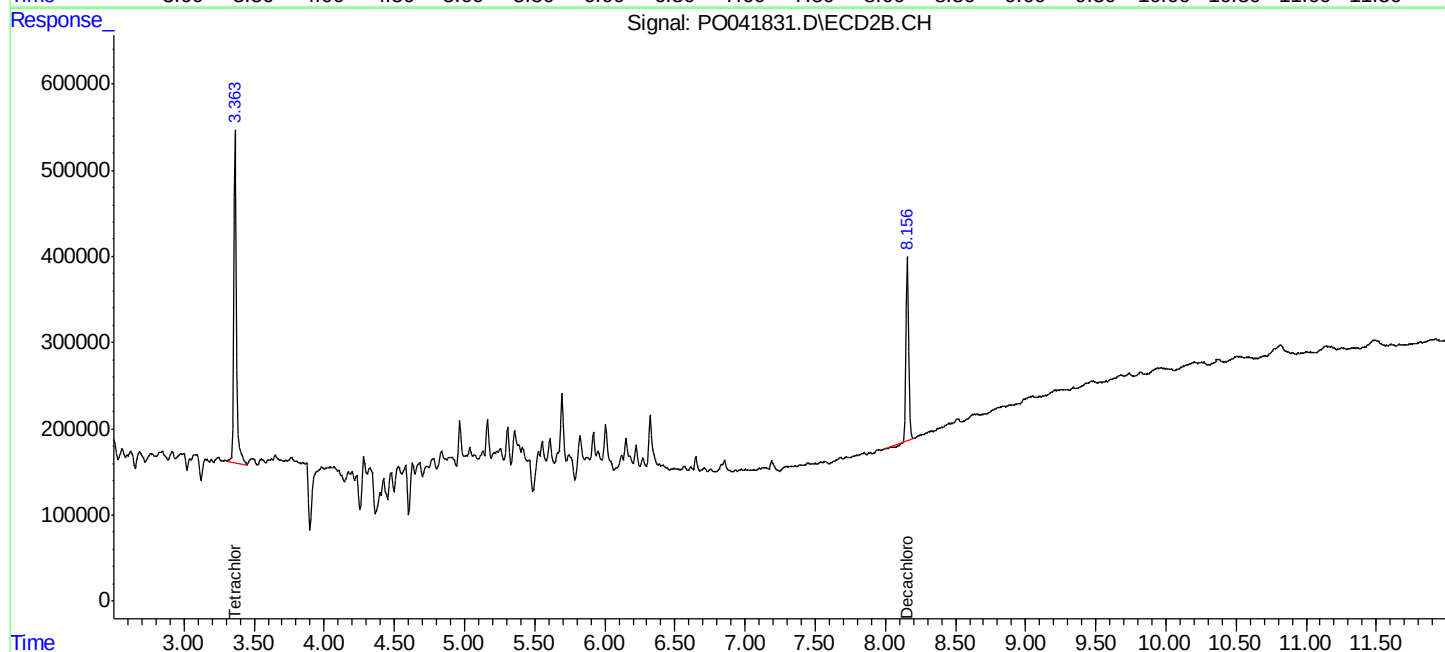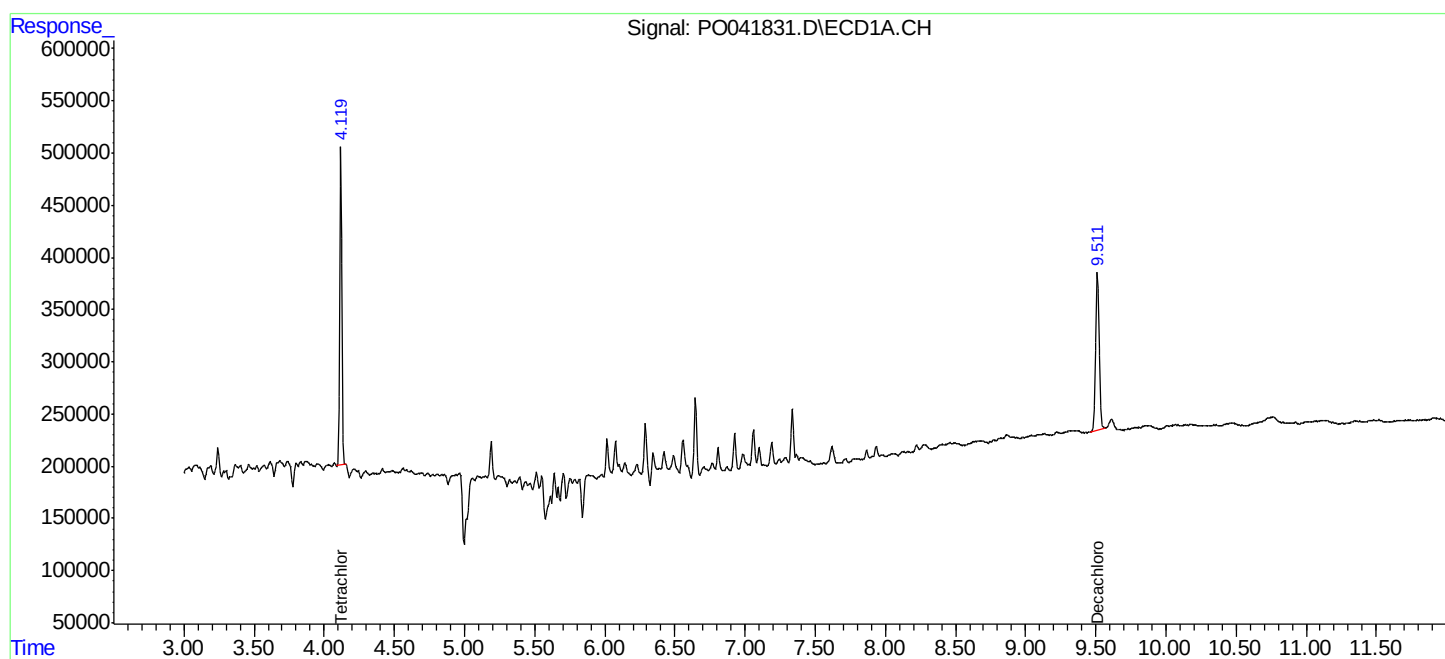

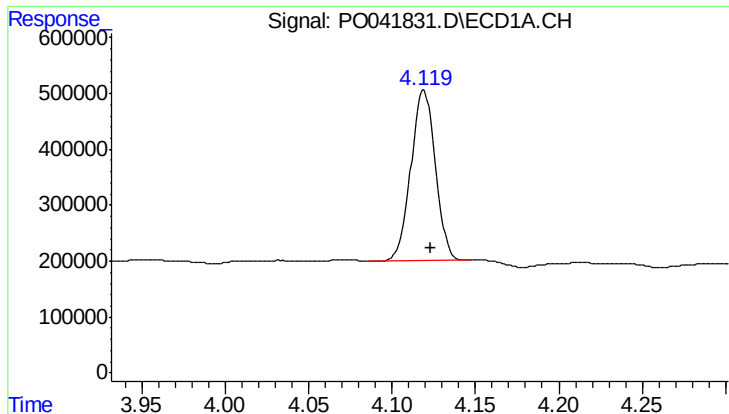


#1 Tetrachloro-m-xylene

R.T.: 4.119 min
Delta R.T.: -0.004 min
Response: 3118533
Conc: 16.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
PL-02-012418-A


Manual Integrations
APPROVED

ugo
1/30/2018 10:52:51 AM

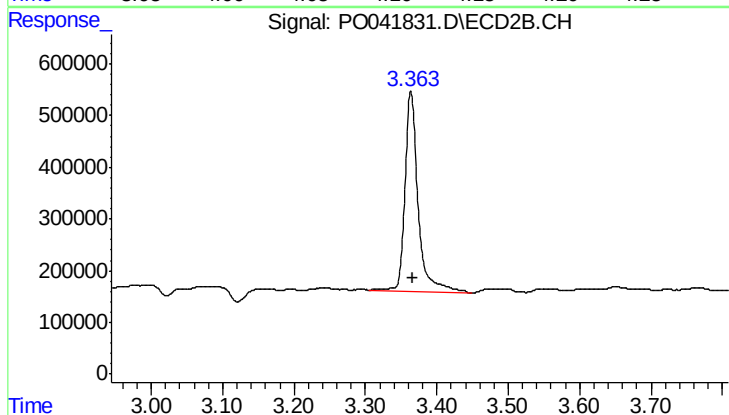


#1 Tetrachloro-m-xylene

R.T.: 3.364 min
Delta R.T.: -0.002 min
Response: 4935180
Conc: 17.00 ng/ml

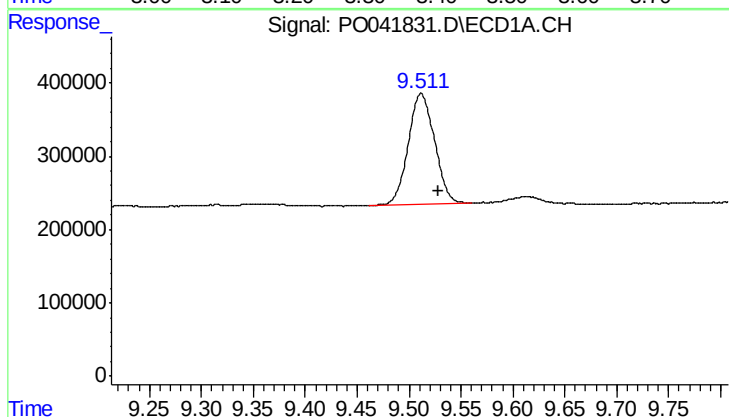

#2 Decachlorobiphenyl

R.T.: 9.512 min
Delta R.T.: -0.017 min
Response: 2654086
Conc: 11.30 ng/ml

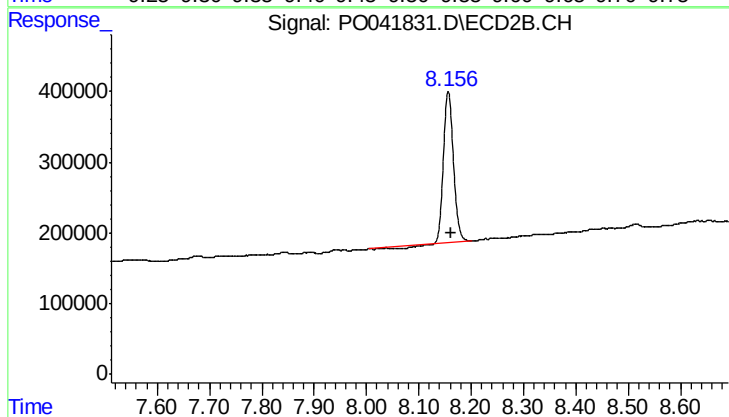

#2 Decachlorobiphenyl

R.T.: 8.156 min
Delta R.T.: -0.006 min
Response: 2720221
Conc: 7.61 ng/ml