

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012819\
 Data File : P0053599.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2019 20:14
 Operator : SM/SJ
 Sample : K1258-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-01-AA01-BB01-AA01A-AA0

Manual Integrations
 APPROVED

Sohil
 1/29/2019 11:29:45 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:48:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jan 28 05:58:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.111	3.170	29603134	4298968	22.847	18.119
2) SA Decachlor...	9.513	7.785	14370813	3722904	16.419m	14.885

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012819\
Data File : P0053599.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2019 20:14
Operator : SM/SJ
Sample : K1258-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-AA01-BB01-AA01A-AA0


Manual Integrations
APPROVED

Sohil
1/29/2019 11:29:45 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:48:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jan 28 05:58:35 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

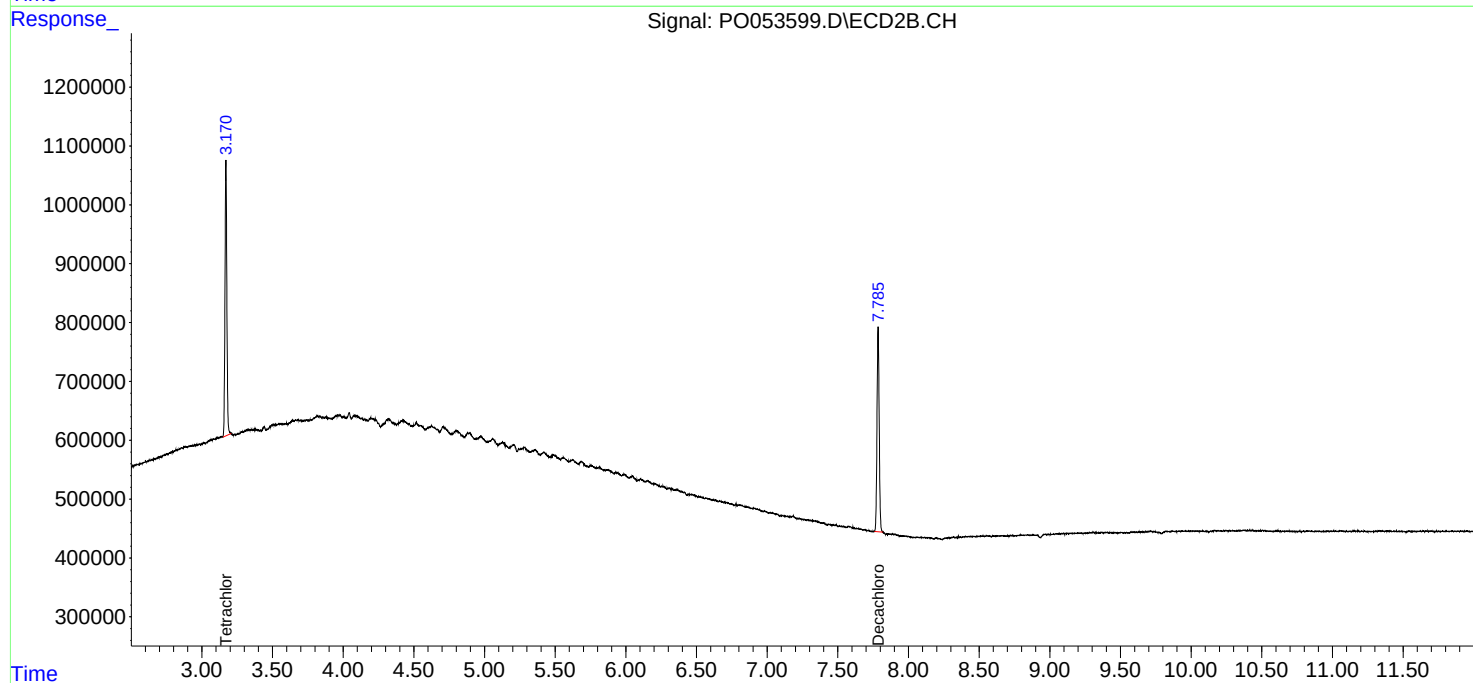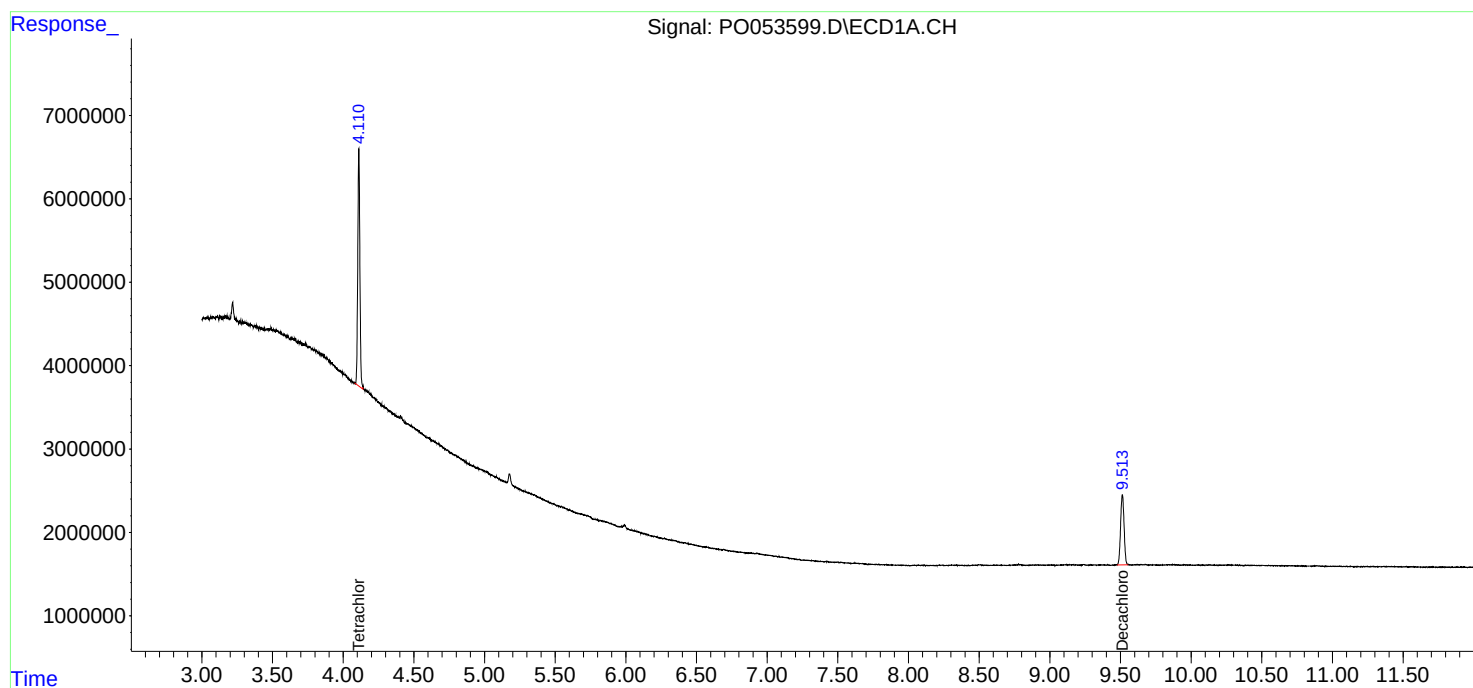

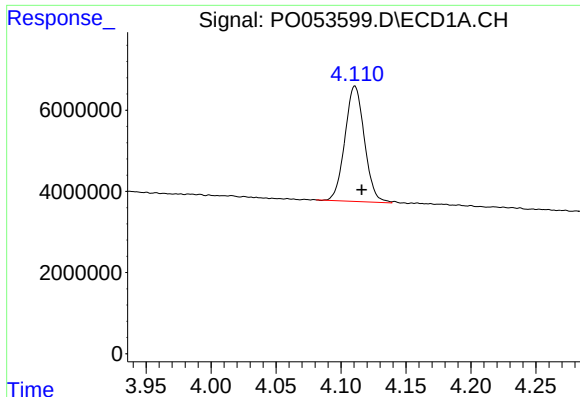


#1 Tetrachloro-m-xylene

R.T.: 4.111 min
Delta R.T.: -0.005 min
Response: 29603134
Conc: 22.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-AA01-BB01-AA01A-AA0


Manual Integrations
APPROVED

Sohil
1/29/2019 11:29:45 AM

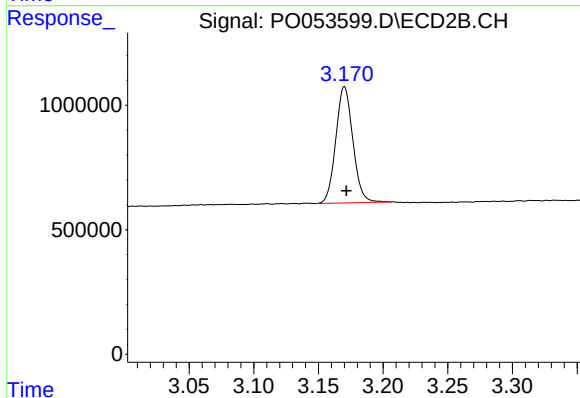


#1 Tetrachloro-m-xylene

R.T.: 3.170 min
Delta R.T.: -0.002 min
Response: 4298968
Conc: 18.12 ng/ml

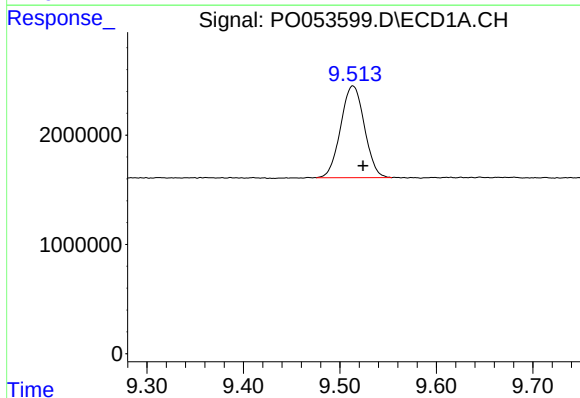

#2 Decachlorobiphenyl

R.T.: 9.513 min
Delta R.T.: -0.011 min
Response: 14370813
Conc: 16.42 ng/ml m

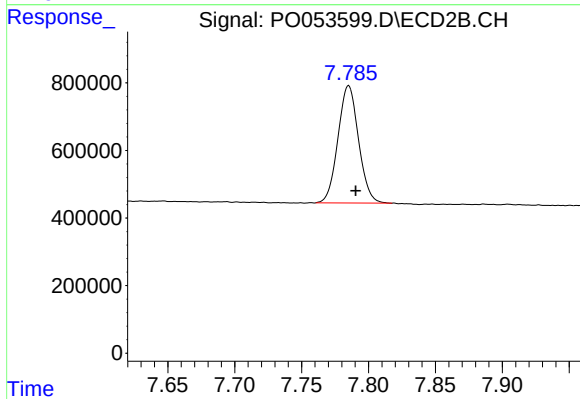

#2 Decachlorobiphenyl

R.T.: 7.785 min
Delta R.T.: -0.005 min
Response: 3722904
Conc: 14.88 ng/ml