

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012819\
 Data File : P0053600.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2019 20:31
 Operator : SM/SJ
 Sample : K1259-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-01-A01-B01-A01A-A01B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:48:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jan 28 05:58:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.111	3.170	31035129	4443371	23.952	18.727
2) SA Decachlor...	9.514	7.786	15161648	4042416	17.322	16.162

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012819\
Data File : PO053600.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2019 20:31
Operator : SM/SJ
Sample : K1259-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-A01-B01-A01A-A01B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:48:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jan 28 05:58:35 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

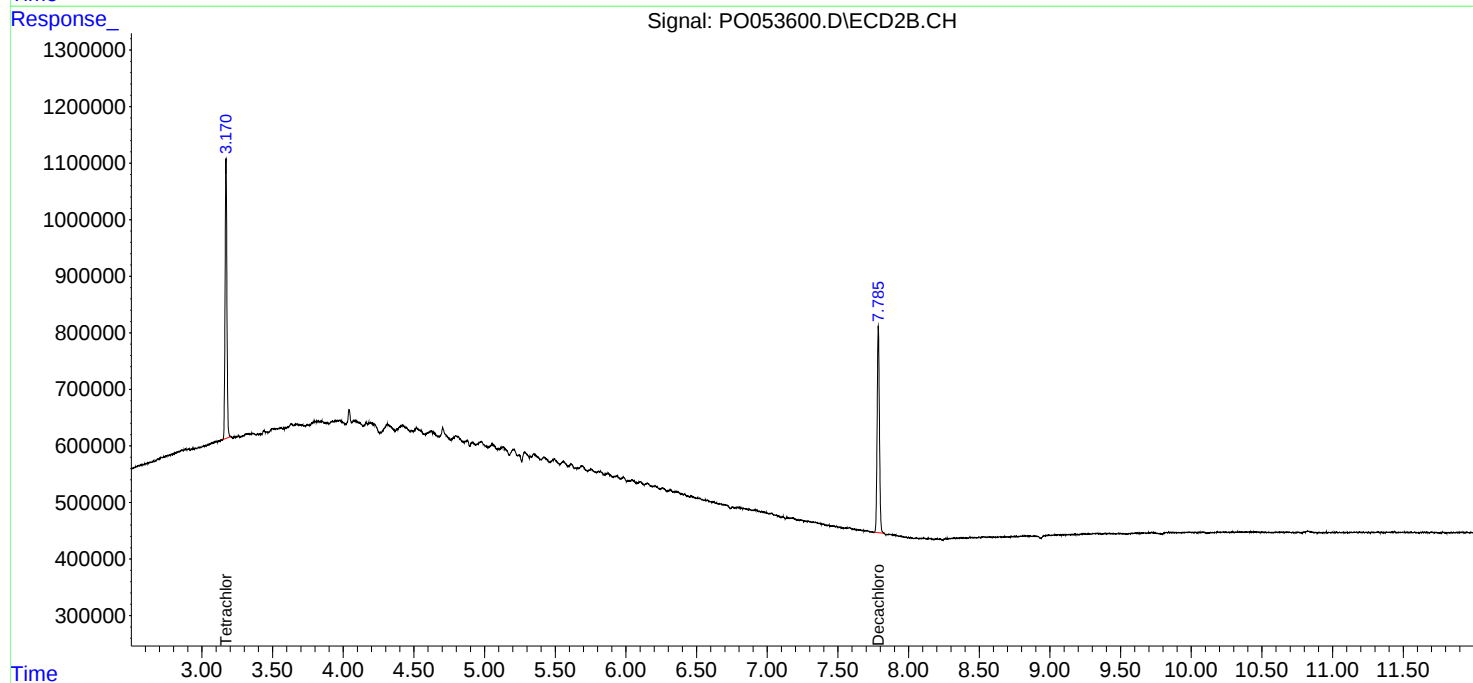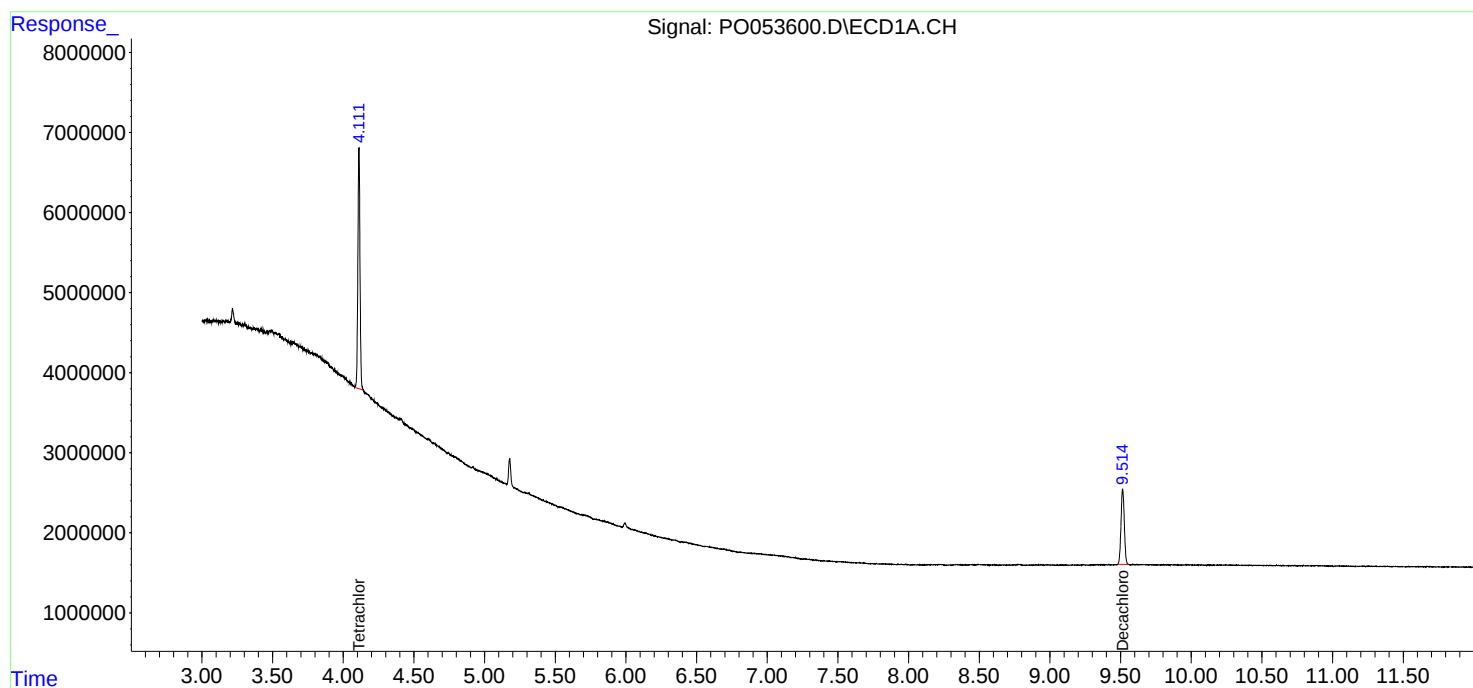


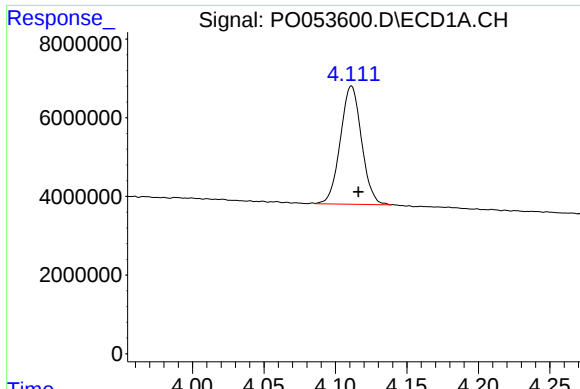

#1 Tetrachloro-m-xylene


R.T.: 4.111 min
Delta R.T.: -0.005 min
Response: 31035129
Conc: 23.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-A01-B01-A01A-A01B

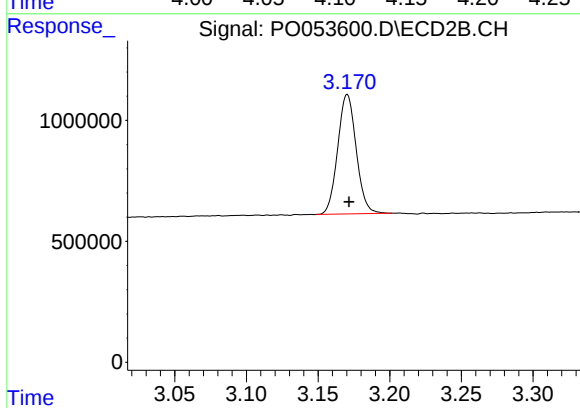


#1 Tetrachloro-m-xylene

R.T.: 3.170 min
Delta R.T.: -0.001 min
Response: 4443371
Conc: 18.73 ng/ml

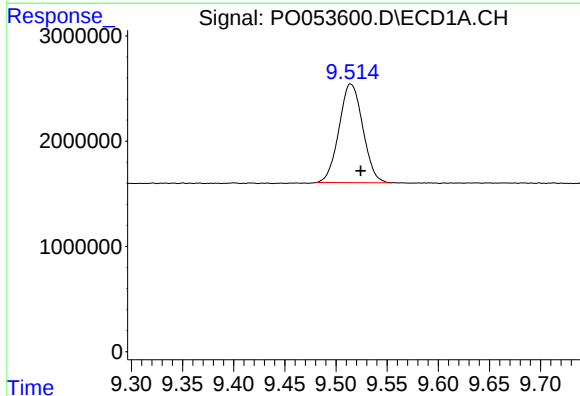

#2 Decachlorobiphenyl

R.T.: 9.514 min
Delta R.T.: -0.010 min
Response: 15161648
Conc: 17.32 ng/ml

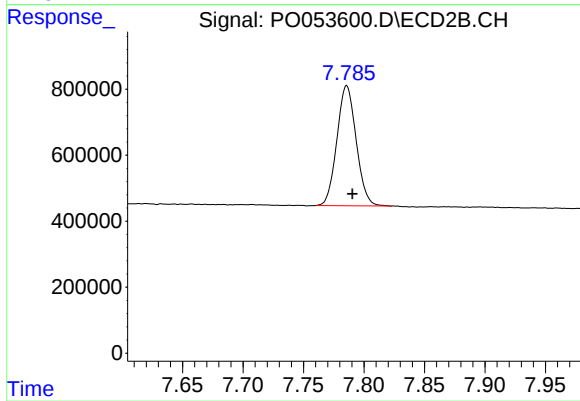

#2 Decachlorobiphenyl

R.T.: 7.786 min
Delta R.T.: -0.005 min
Response: 4042416
Conc: 16.16 ng/ml