

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
 Data File : P0066049.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2020 23:03
 Operator : DD\AJ
 Sample : L1289-29
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-35-34-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 01:36:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.147	3.424	755318	1049761	32.574	39.522
2)	SA Decachlor...	9.638	8.321	1119586	1627527	26.896	33.491
Target Compounds							
7)	L1 AR-1016-5	0.000	4.929	0	25276	N.D.	23.444 #
9)	L2 AR-1221-2	4.446	3.717	11548	19685	52.351	77.464 #
15)	L3 AR-1232-5	0.000	4.929	0	25276	N.D.	63.431 #
20)	L4 AR-1242-5	6.142	5.293	79893	29380	95.948	26.540 #
24)	L5 AR-1248-4	6.142	4.929	79893	25276	59.295	19.807 #
25)	L5 AR-1248-5	6.142	5.293	79893	29380	61.816	21.050 #
26)	L6 AR-1254-1	6.142	5.293	79893	29380	60.192	13.140 #
28)	L6 AR-1254-3	6.725	0.000	20997	0	8.635	N.D. #
29)	L6 AR-1254-4	6.995	0.000	44200	0	21.090	N.D. #
32)	L7 AR-1260-2	0.000	6.117	0	17159	N.D.	5.415 #
35)	L7 AR-1260-5	0.000	6.987	0	17150	N.D.	2.821 #
37)	L8 AR-1262-2	0.000	6.987	0	17150	N.D.	2.712 #
38)	L8 AR-1262-3	0.000	7.267	0	33588	N.D.	13.115 #
39)	L8 AR-1262-4	0.000	7.330	0	24228	N.D.	5.152 #
40)	L8 AR-1262-5	0.000	7.823	0	2195	N.D.	1.044 #
41)	L9 AR-1268-1	0.000	7.267	0	33588	N.D.	4.311 #
42)	L9 AR-1268-2	0.000	7.330	0	24228	N.D.	3.345 #
43)	L9 AR-1268-3	0.000	7.534	0	28707	N.D.	4.796 #
44)	L9 AR-1268-4	0.000	7.823	0	2195	N.D.	0.900 #
45)	L9 AR-1268-5	0.000	8.093	0	14035	N.D.	0.777 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
Data File : P0066049.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2020 23:03
Operator : DD\AJ
Sample : L1289-29
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 01:36:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

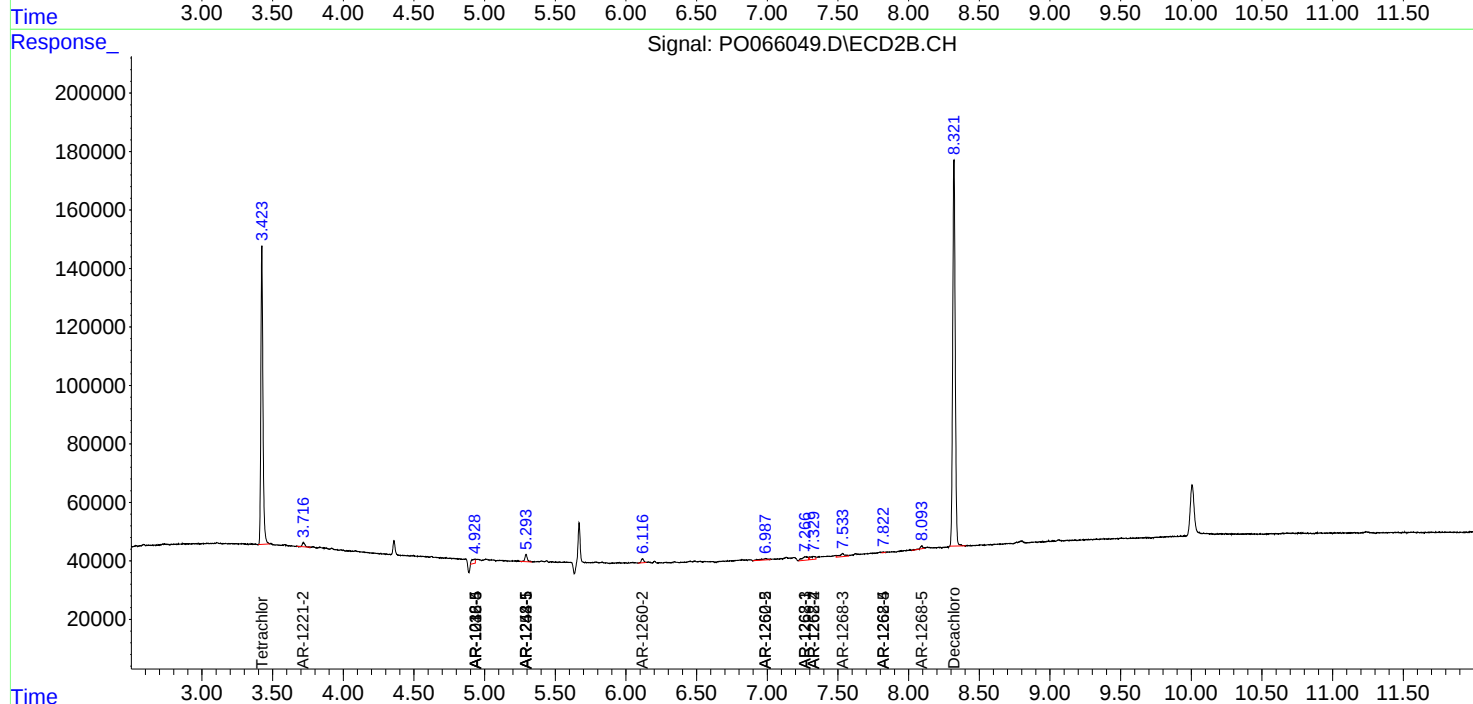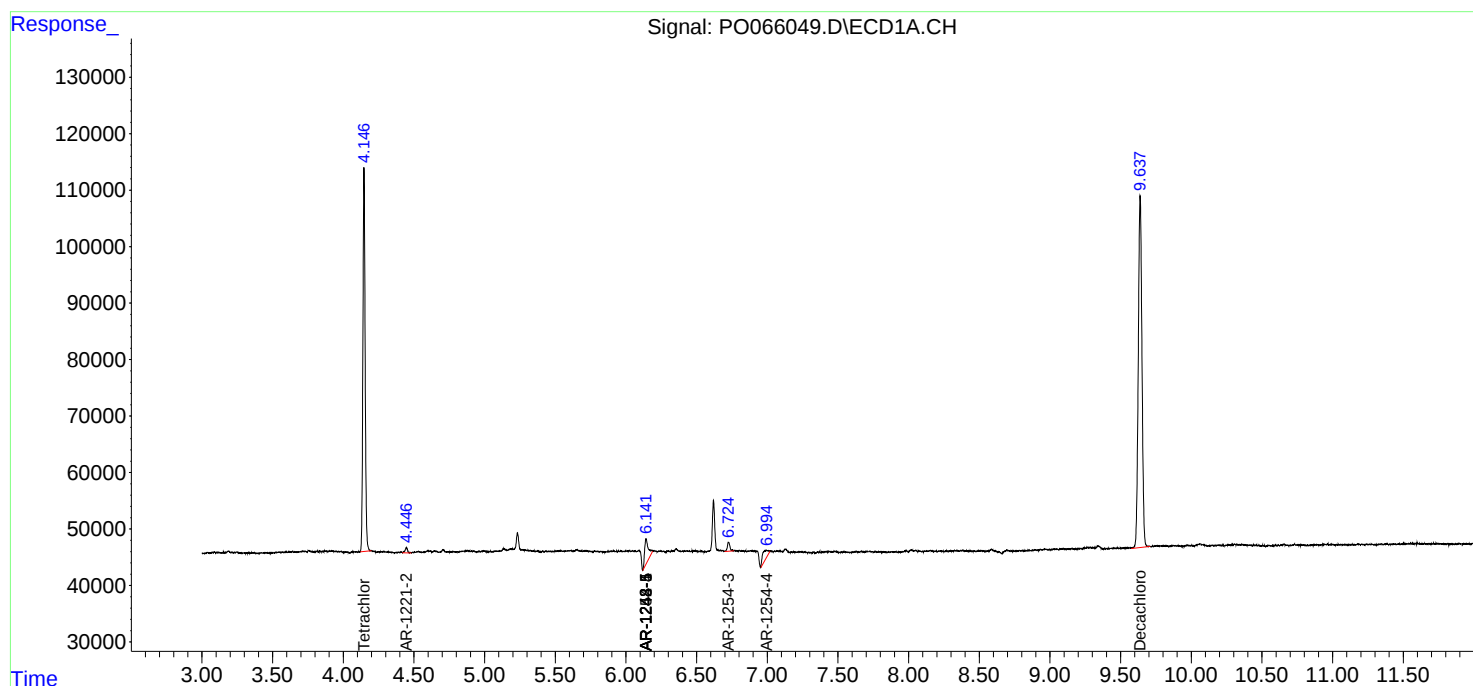


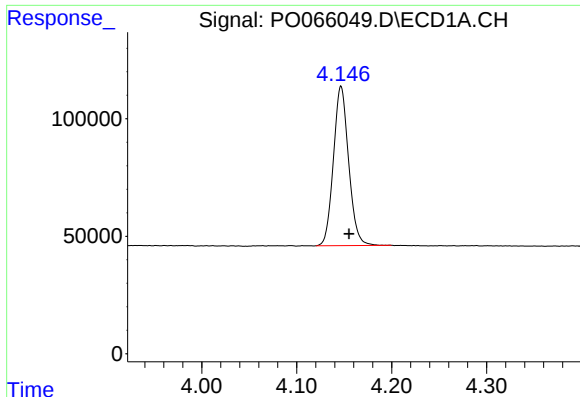

#1 Tetrachloro-m-xylene


R.T.: 4.147 min
Delta R.T.: -0.008 min
Response: 755318
Conc: 32.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

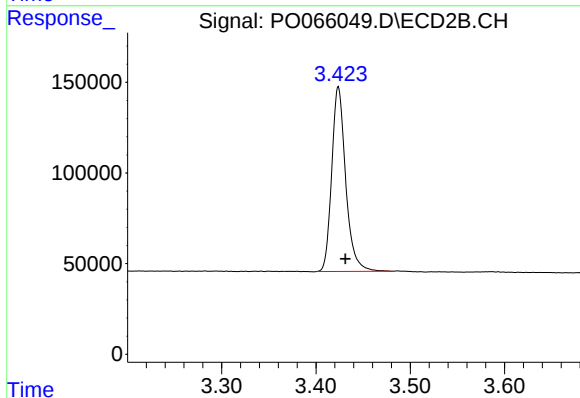


#1 Tetrachloro-m-xylene

R.T.: 3.424 min
Delta R.T.: -0.007 min
Response: 1049761
Conc: 39.52 ng/ml

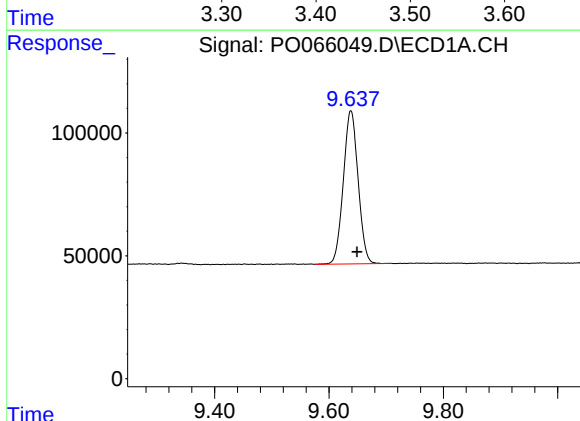


#2 Decachlorobiphenyl

R.T.: 9.638 min
Delta R.T.: -0.011 min
Response: 1119586
Conc: 26.90 ng/ml

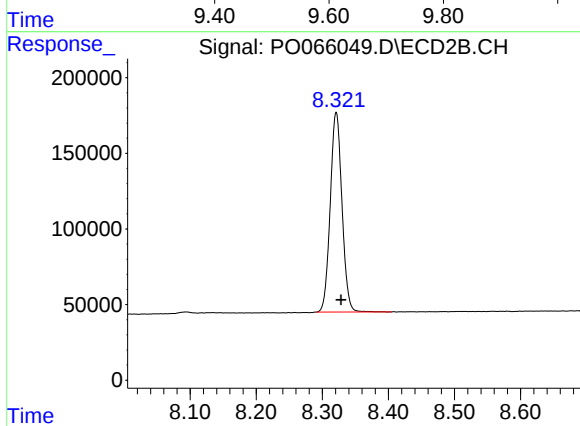

#2 Decachlorobiphenyl


R.T.: 8.321 min
Delta R.T.: -0.008 min
Response: 1627527
Conc: 33.49 ng/ml

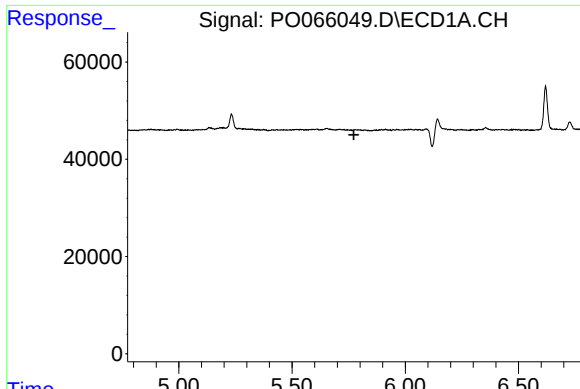

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

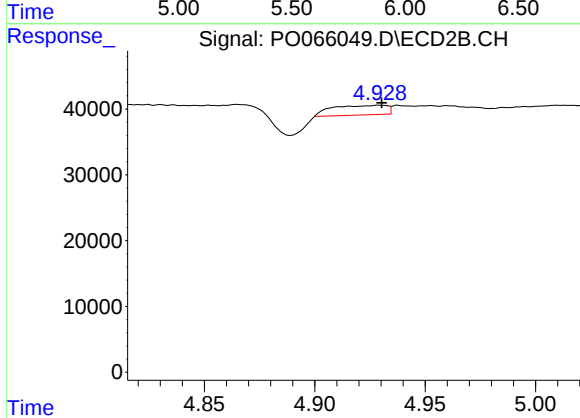


#7 AR-1016-5

R.T.: 4.929 min
Delta R.T.: -0.001 min
Response: 25276
Conc: 23.44 ng/ml

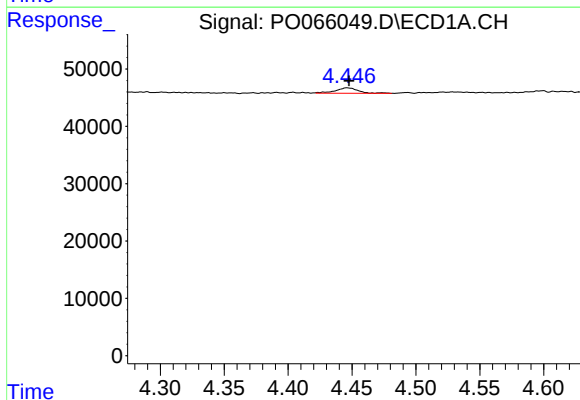


#9 AR-1221-2

R.T.: 4.446 min
Delta R.T.: -0.001 min
Response: 11548
Conc: 52.35 ng/ml

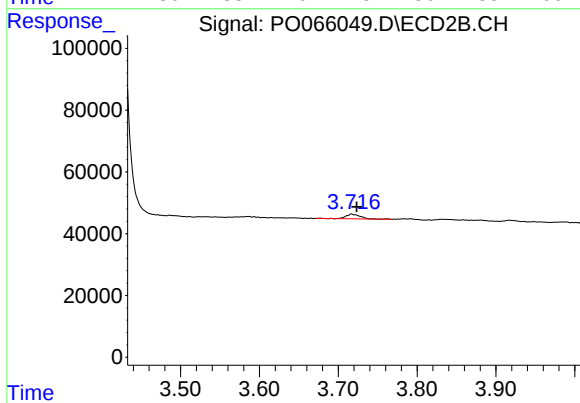

#9 AR-1221-2


R.T.: 3.717 min
Delta R.T.: -0.007 min
Response: 19685
Conc: 77.46 ng/ml

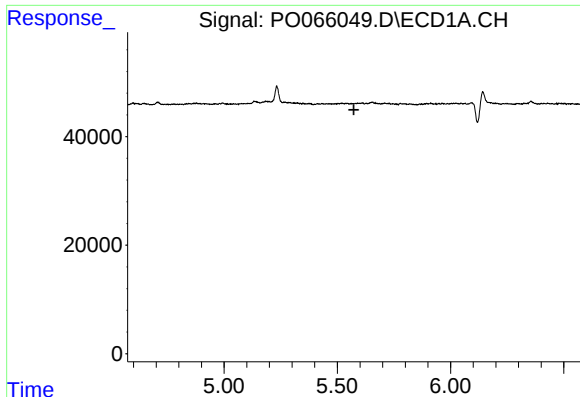

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

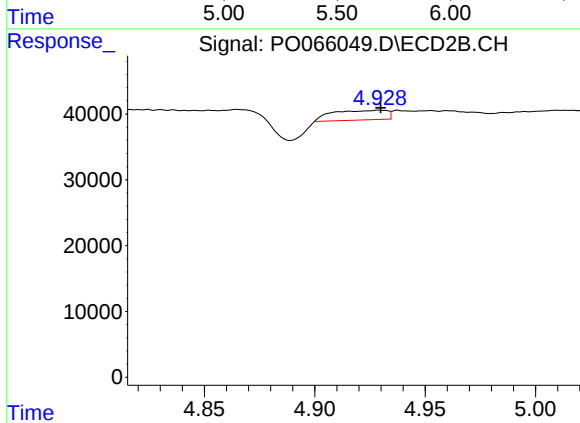


#15 AR-1232-5

R.T.: 4.929 min
Delta R.T.: 0.000 min
Response: 25276
Conc: 63.43 ng/ml

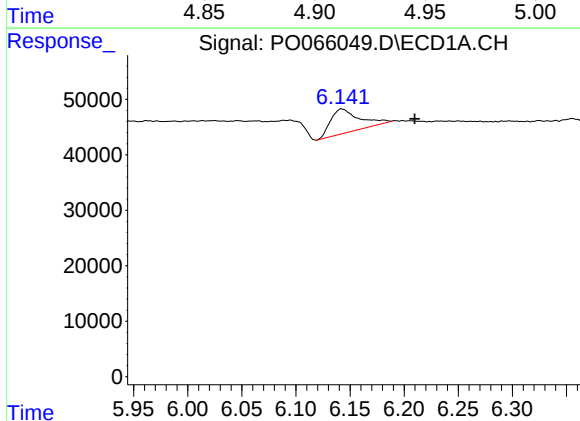


#20 AR-1242-5

R.T.: 6.142 min
Delta R.T.: -0.068 min
Response: 79893
Conc: 95.95 ng/ml

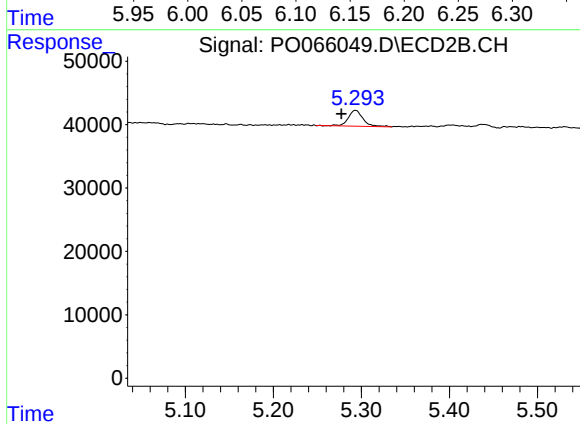

#20 AR-1242-5


R.T.: 5.293 min
Delta R.T.: 0.016 min
Response: 29380
Conc: 26.54 ng/ml

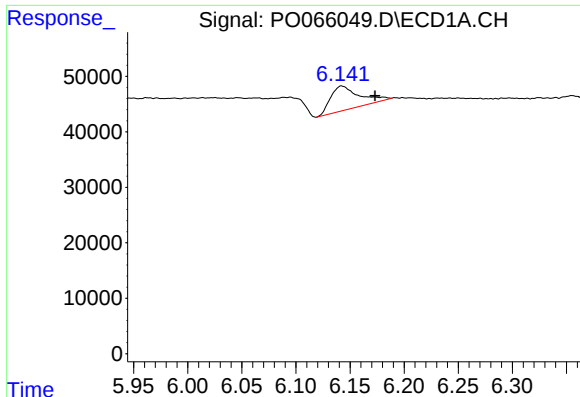

#24 AR-1248-4


R.T.: 6.142 min
Delta R.T.: -0.031 min
Response: 79893
Conc: 59.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

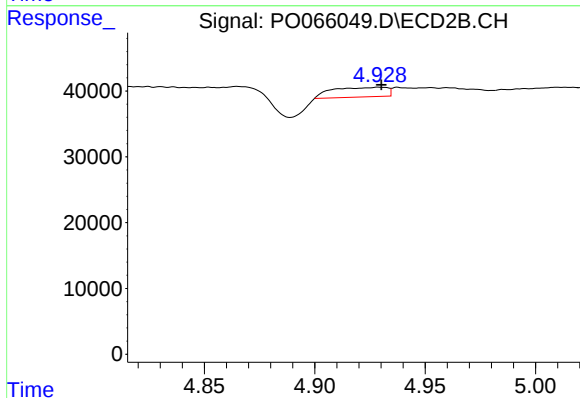


#24 AR-1248-4

R.T.: 4.929 min
Delta R.T.: -0.001 min
Response: 25276
Conc: 19.81 ng/ml

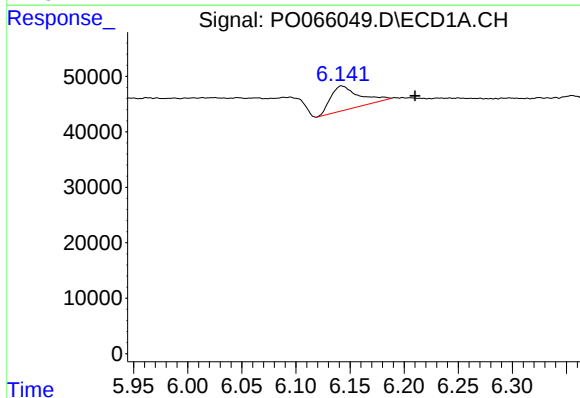


#25 AR-1248-5

R.T.: 6.142 min
Delta R.T.: -0.068 min
Response: 79893
Conc: 61.82 ng/ml

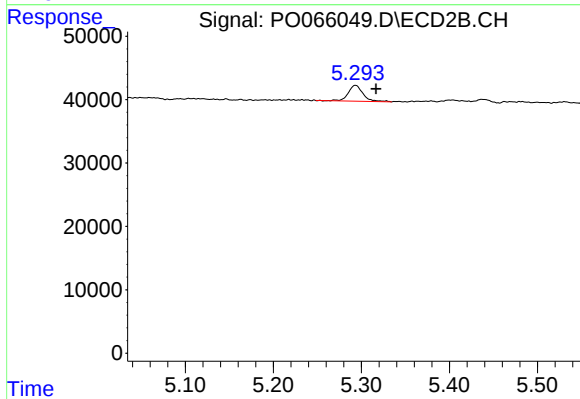

#25 AR-1248-5


R.T.: 5.293 min
Delta R.T.: -0.023 min
Response: 29380
Conc: 21.05 ng/ml

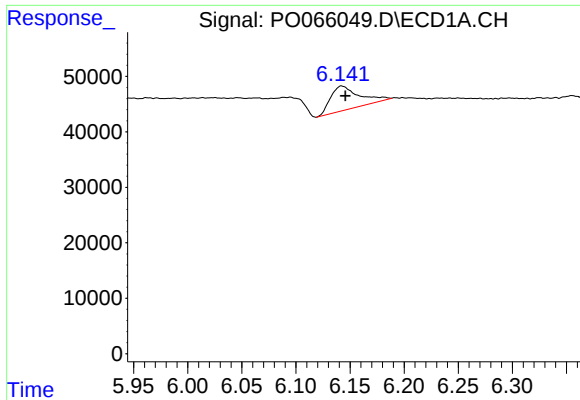

#26 AR-1254-1


R.T.: 6.142 min
Delta R.T.: -0.003 min
Response: 79893
Conc: 60.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

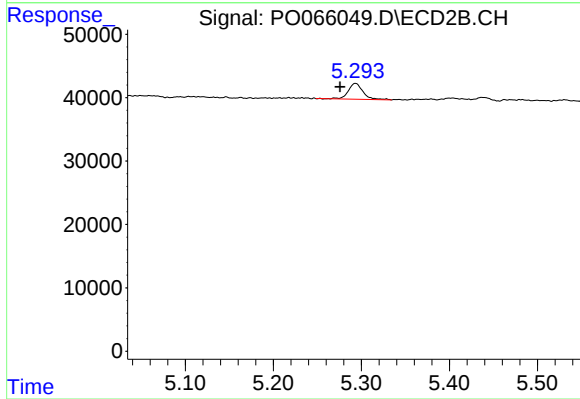


#26 AR-1254-1

R.T.: 5.293 min
Delta R.T.: 0.017 min
Response: 29380
Conc: 13.14 ng/ml

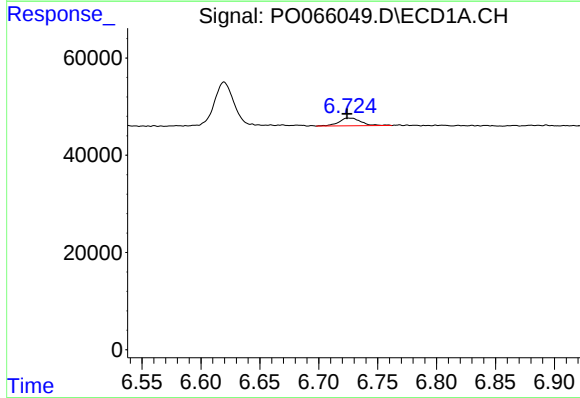


#28 AR-1254-3

R.T.: 6.725 min
Delta R.T.: 0.001 min
Response: 20997
Conc: 8.63 ng/ml

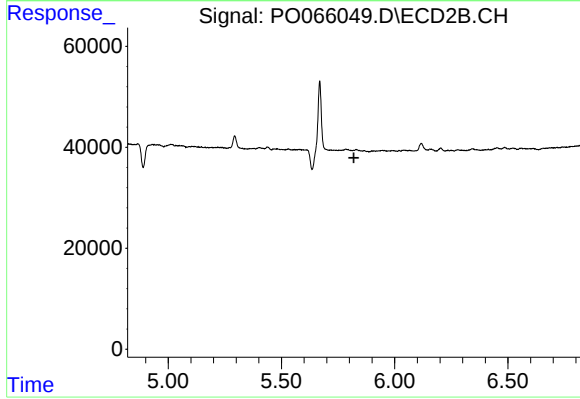

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 5.820 min
Response: 0
Conc: N.D.

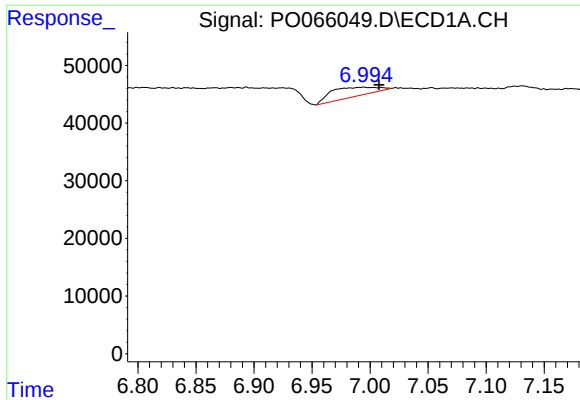

#29 AR-1254-4


R.T.: 6.995 min
Delta R.T.: -0.013 min
Response: 44200
Conc: 21.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

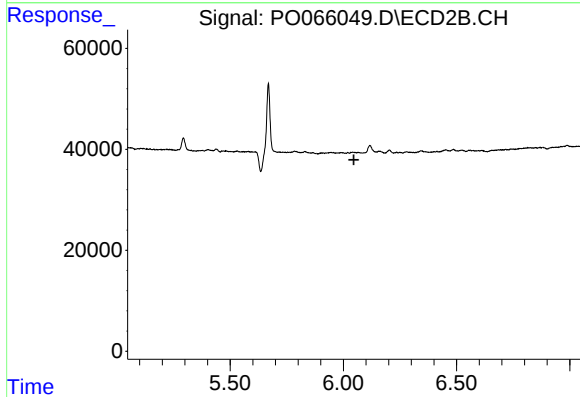


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.046 min
Response: 0
Conc: N.D.

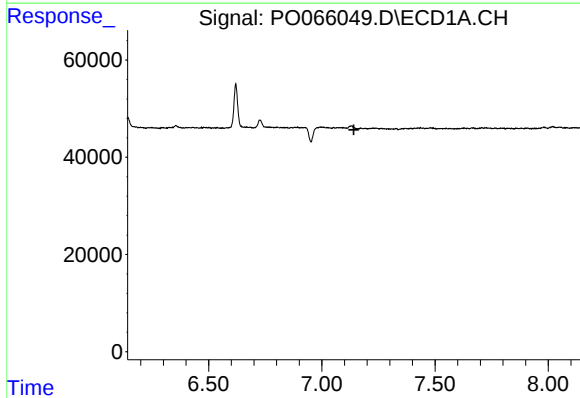


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.142 min
Response: 0
Conc: N.D.

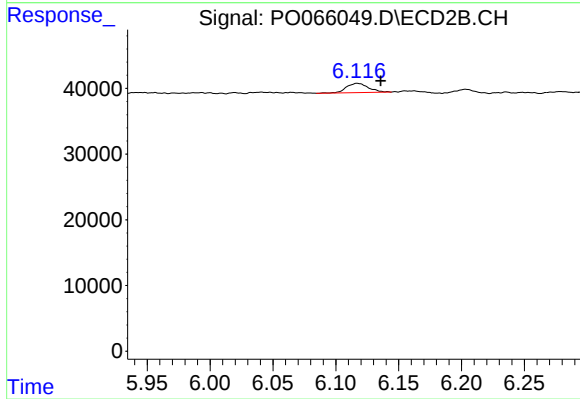

#32 AR-1260-2


R.T.: 6.117 min
Delta R.T.: -0.019 min
Response: 17159
Conc: 5.42 ng/ml

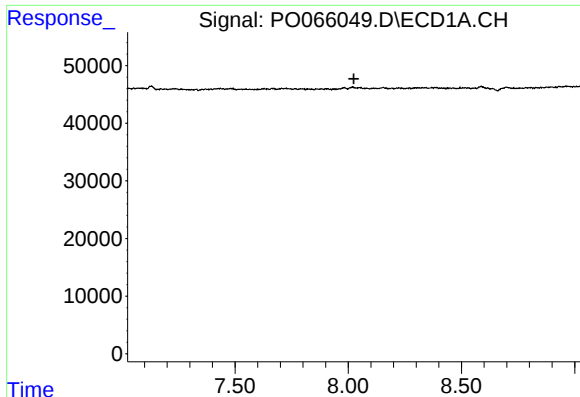

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.025 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

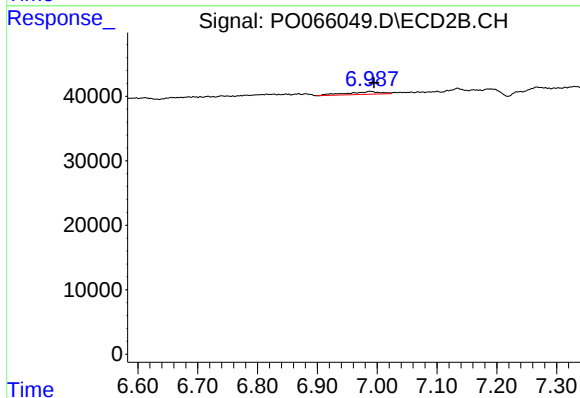


#35 AR-1260-5

R.T.: 6.987 min
Delta R.T.: -0.007 min
Response: 17150
Conc: 2.82 ng/ml

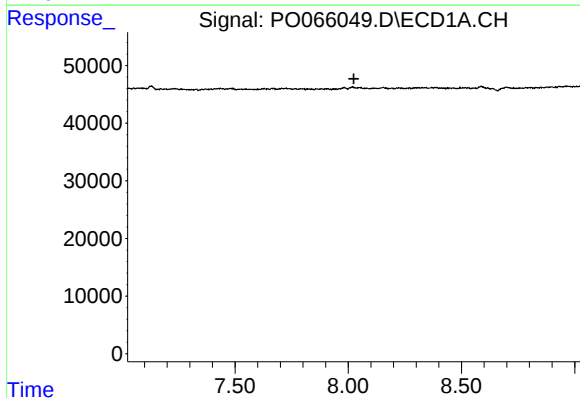


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.025 min
Response: 0
Conc: N.D.

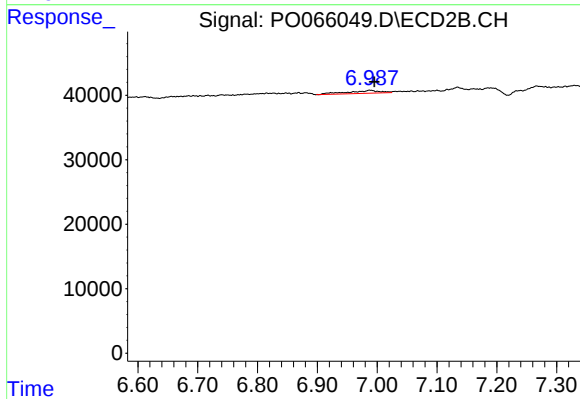

#37 AR-1262-2


R.T.: 6.987 min
Delta R.T.: -0.008 min
Response: 17150
Conc: 2.71 ng/ml

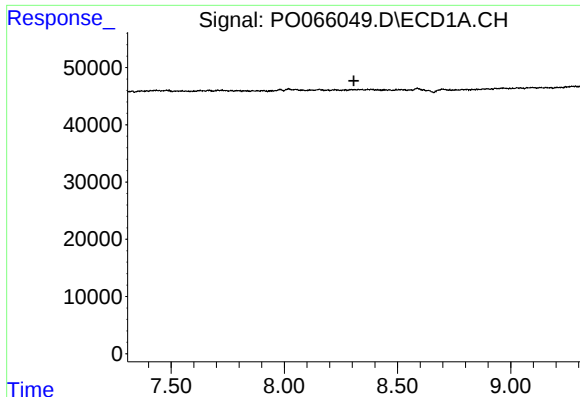

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.307 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

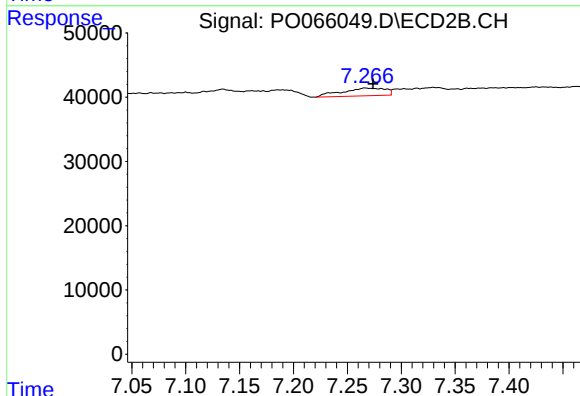


#38 AR-1262-3

R.T.: 7.267 min
Delta R.T.: -0.007 min
Response: 33588
Conc: 13.12 ng/ml

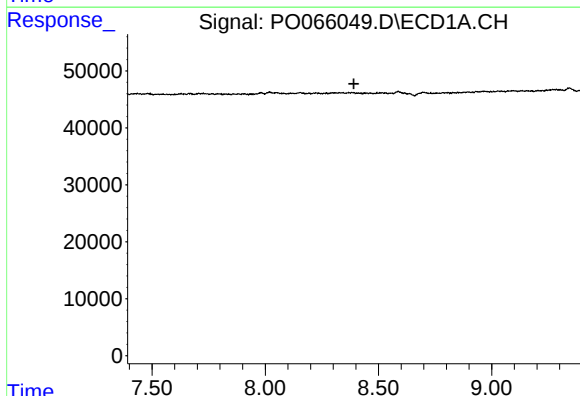


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.391 min
Response: 0
Conc: N.D.

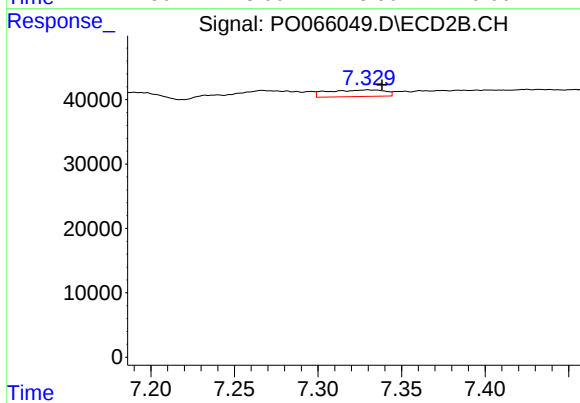

#39 AR-1262-4


R.T.: 7.330 min
Delta R.T.: -0.009 min
Response: 24228
Conc: 5.15 ng/ml

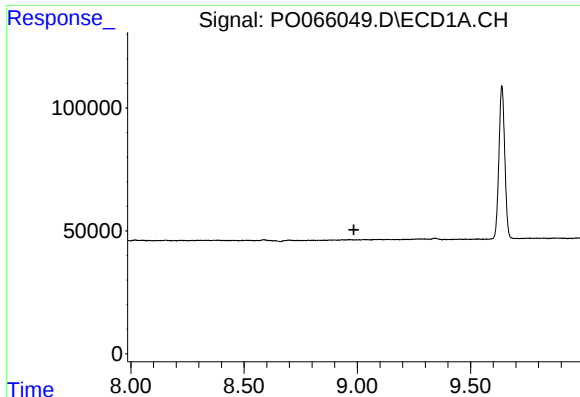

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 8.985 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

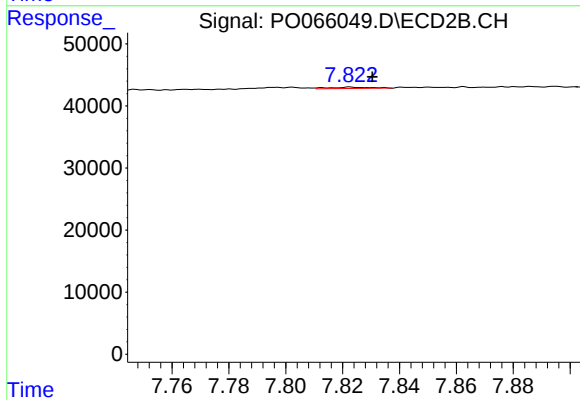


#40 AR-1262-5

R.T.: 7.823 min
Delta R.T.: -0.008 min
Response: 2195
Conc: 1.04 ng/ml

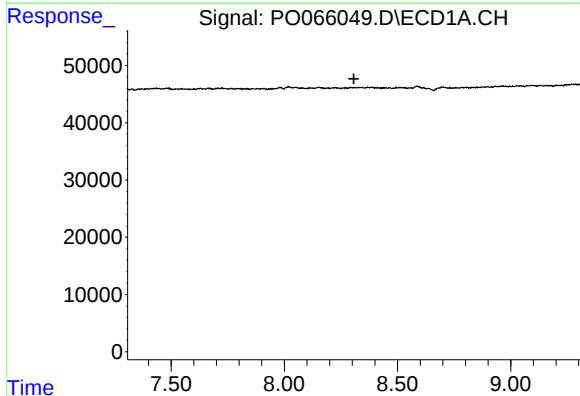


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.307 min
Response: 0
Conc: N.D.

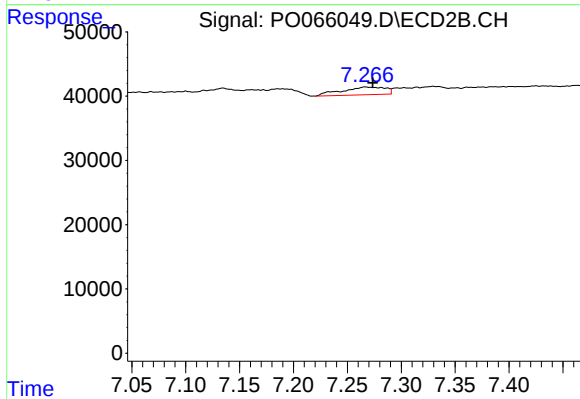

#41 AR-1268-1


R.T.: 7.267 min
Delta R.T.: -0.007 min
Response: 33588
Conc: 4.31 ng/ml

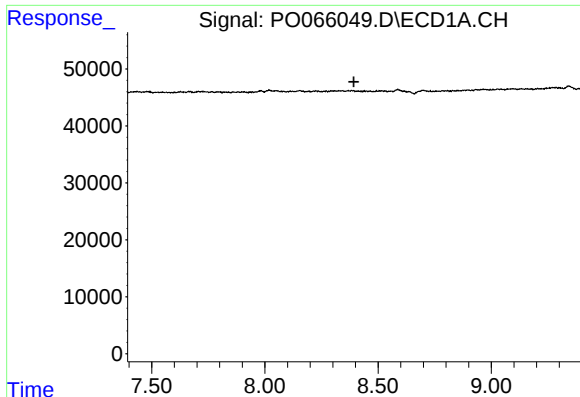

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

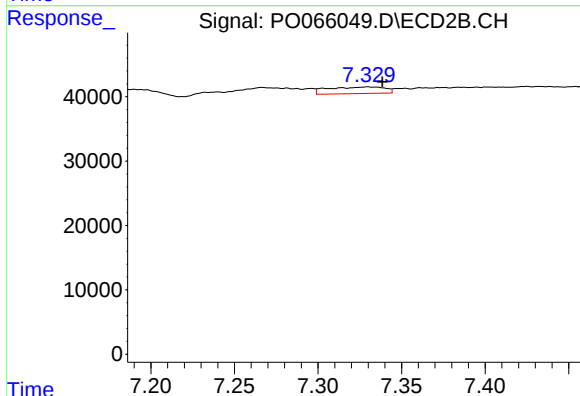


#42 AR-1268-2

R.T.: 7.330 min
Delta R.T.: -0.009 min
Response: 24228
Conc: 3.35 ng/ml

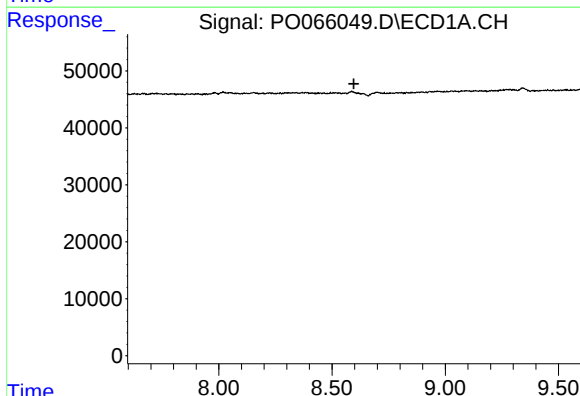


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.597 min
Response: 0
Conc: N.D.

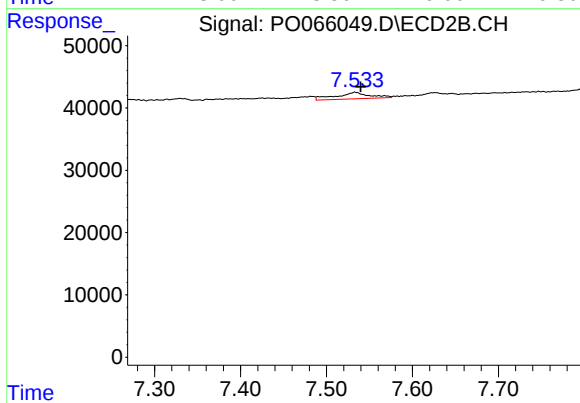

#43 AR-1268-3


R.T.: 7.534 min
Delta R.T.: -0.006 min
Response: 28707
Conc: 4.80 ng/ml

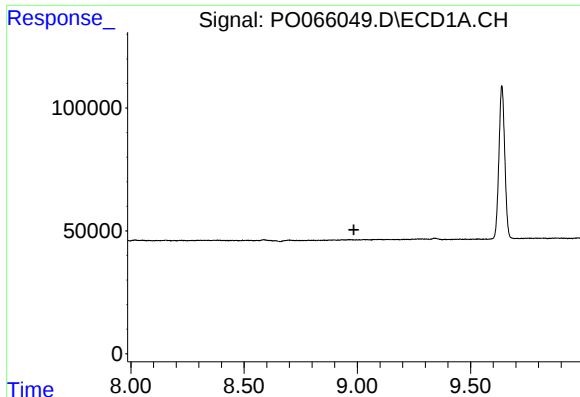

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 8.985 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

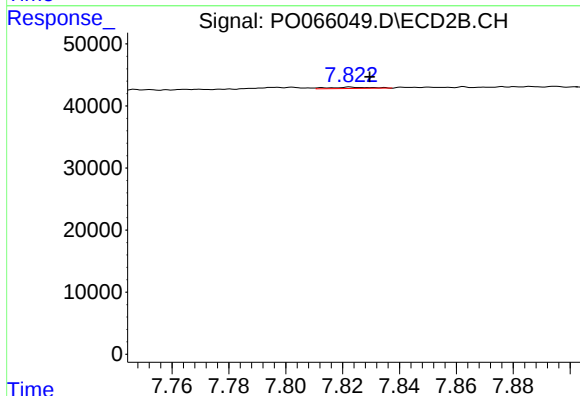


#44 AR-1268-4

R.T.: 7.823 min
Delta R.T.: -0.007 min
Response: 2195
Conc: 0.90 ng/ml

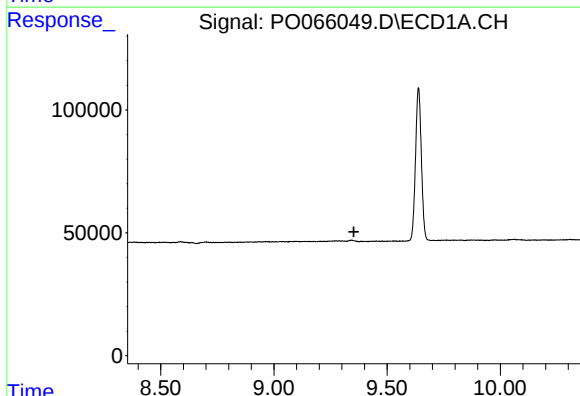

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.353 min
Response: 0
Conc: N.D.

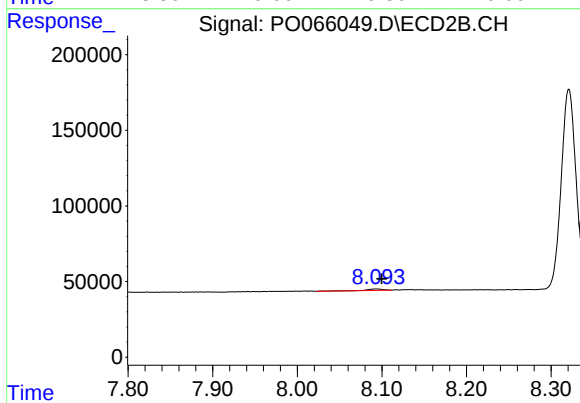

#45 AR-1268-5

R.T.: 8.093 min
Delta R.T.: -0.007 min
Response: 14035
Conc: 0.78 ng/ml