

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
 Data File : P0066025.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2020 13:51
 Operator : DD\AJ
 Sample : L1268-06
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 17562

Manual Integrations
 APPROVED

mohammad
 2/3/2020 3:56:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 15:19:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.159	3.439	622009	664510	26.825m	25.018
2) SA Decachlor...	9.650	8.328	710476	965001	17.068	19.858

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
Data File : P0066025.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2020 13:51
Operator : DD\AJ
Sample : L1268-06
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
17562


Manual Integrations
APPROVED

mohammad
2/3/2020 3:56:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 15:19:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

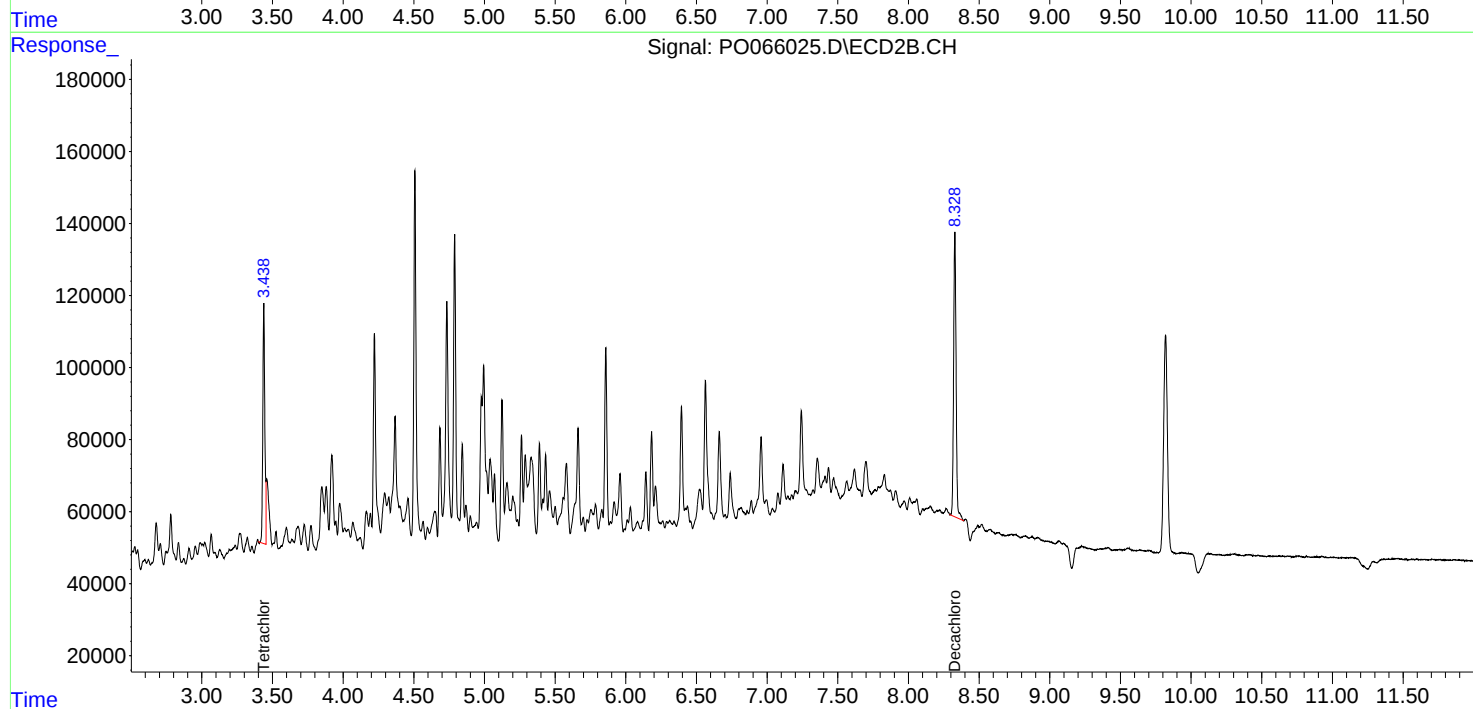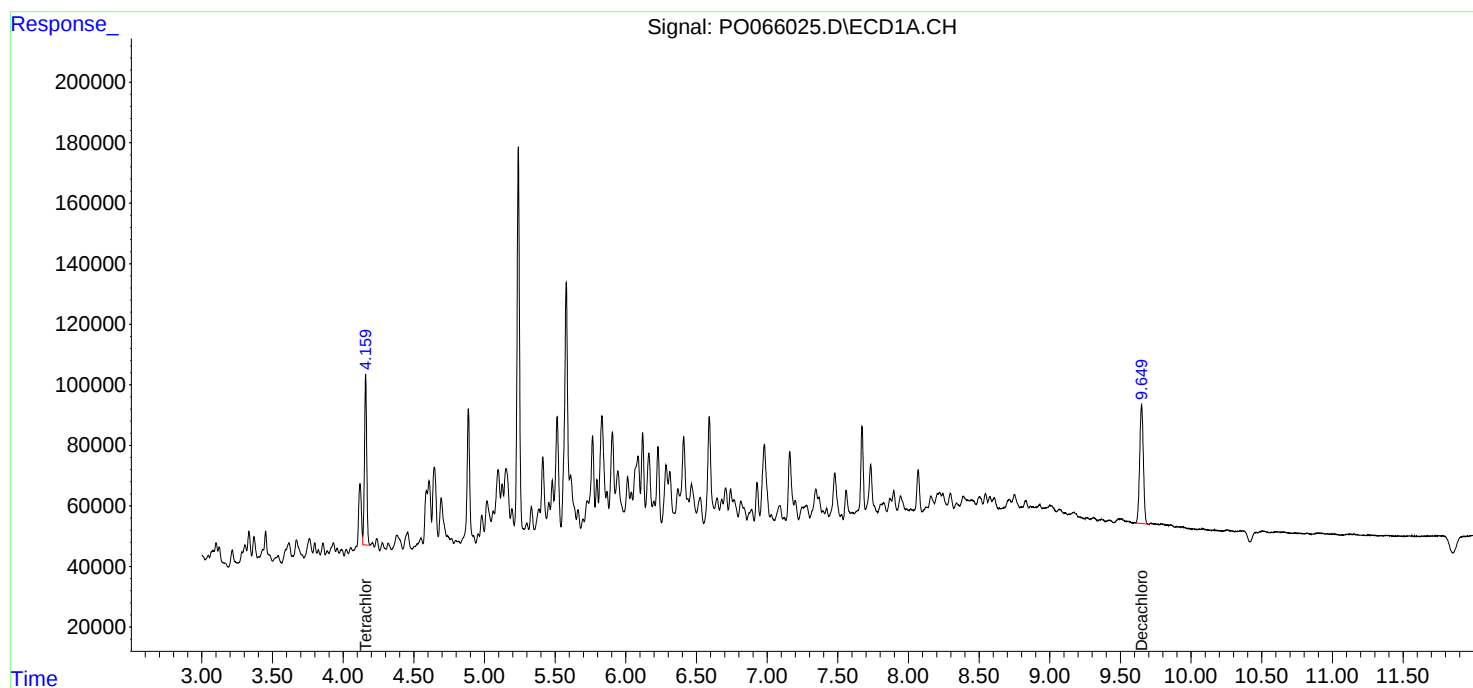

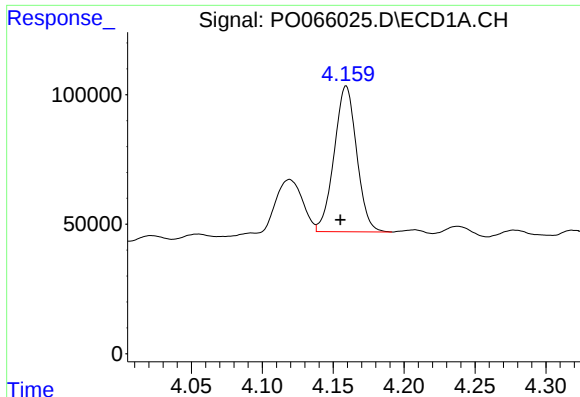


#1 Tetrachloro-m-xylene

R.T.: 4.159 min
Delta R.T.: 0.004 min
Response: 622009
Conc: 26.82 ng/ml m

Instrument :
ECD_O
ClientSampleId :
17562


Manual Integrations
APPROVED

mohammad
2/3/2020 3:56:18 PM

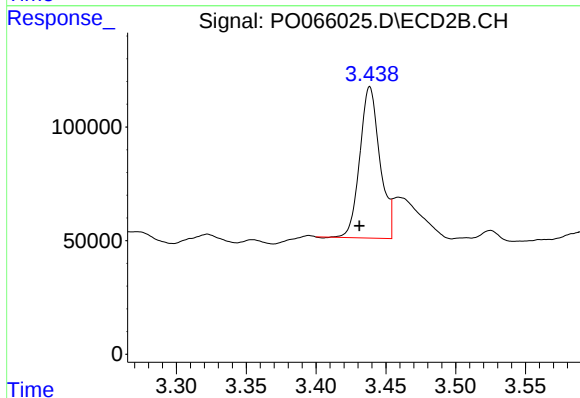


#1 Tetrachloro-m-xylene

R.T.: 3.439 min
Delta R.T.: 0.007 min
Response: 664510
Conc: 25.02 ng/ml

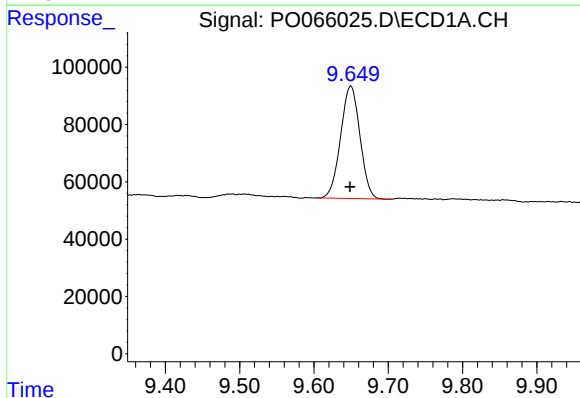

#2 Decachlorobiphenyl

R.T.: 9.650 min
Delta R.T.: 0.000 min
Response: 710476
Conc: 17.07 ng/ml

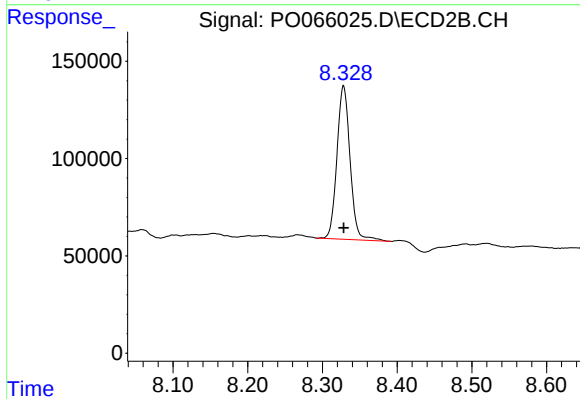

#2 Decachlorobiphenyl

R.T.: 8.328 min
Delta R.T.: 0.000 min
Response: 965001
Conc: 19.86 ng/ml