

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
 Data File : P0066032.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2020 15:54
 Operator : DD\AJ
 Sample : L1243-08RE
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CTY-SB-BC-0-3.5RE

Manual Integrations
 APPROVED

mohammad
 1/30/2020 3:26:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 17:10:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.153	3.429	905078	1187013	39.032m	44.689
2) SA Decachlor...	9.648	8.329	677619	901150	16.278	18.544

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
Data File : P0066032.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2020 15:54
Operator : DD\AJ
Sample : L1243-08RE
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CTY-SB-BC-0-3.5RE


Manual Integrations
APPROVED

mohammad
1/30/2020 3:26:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 17:10:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

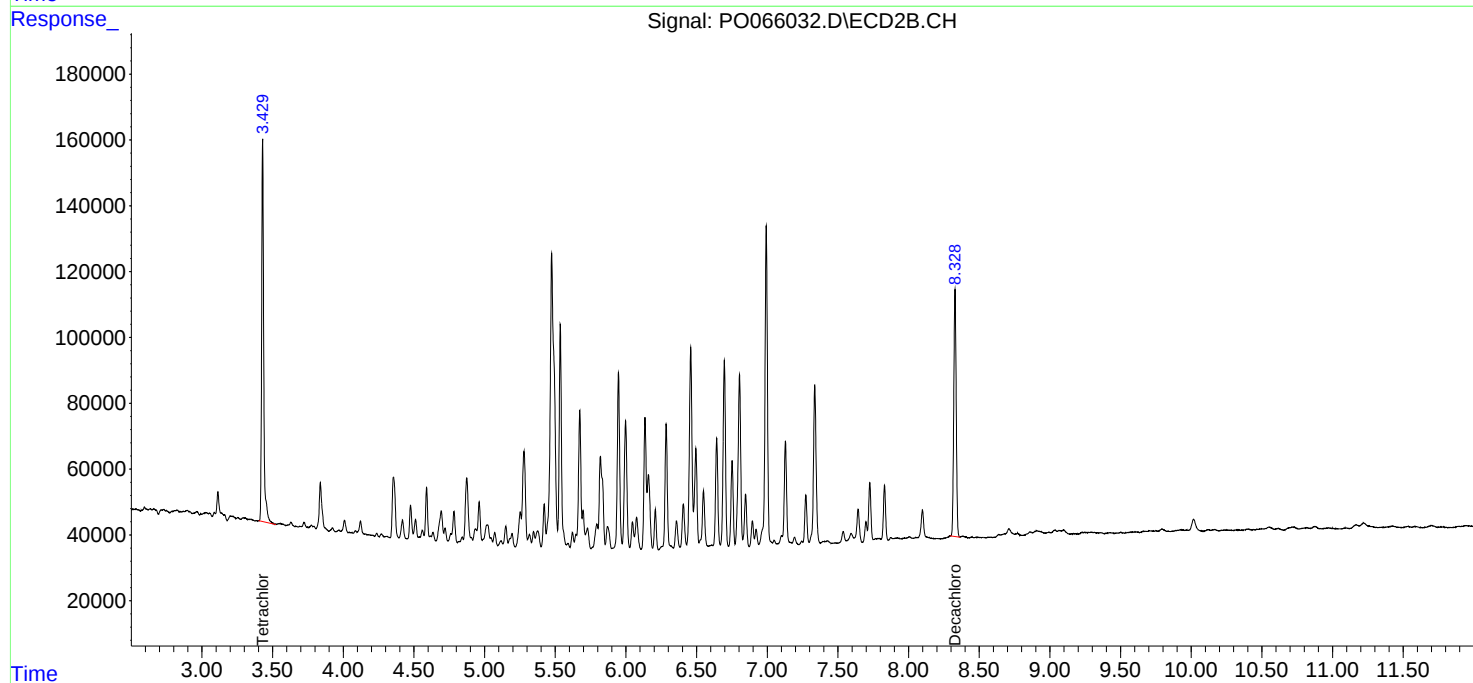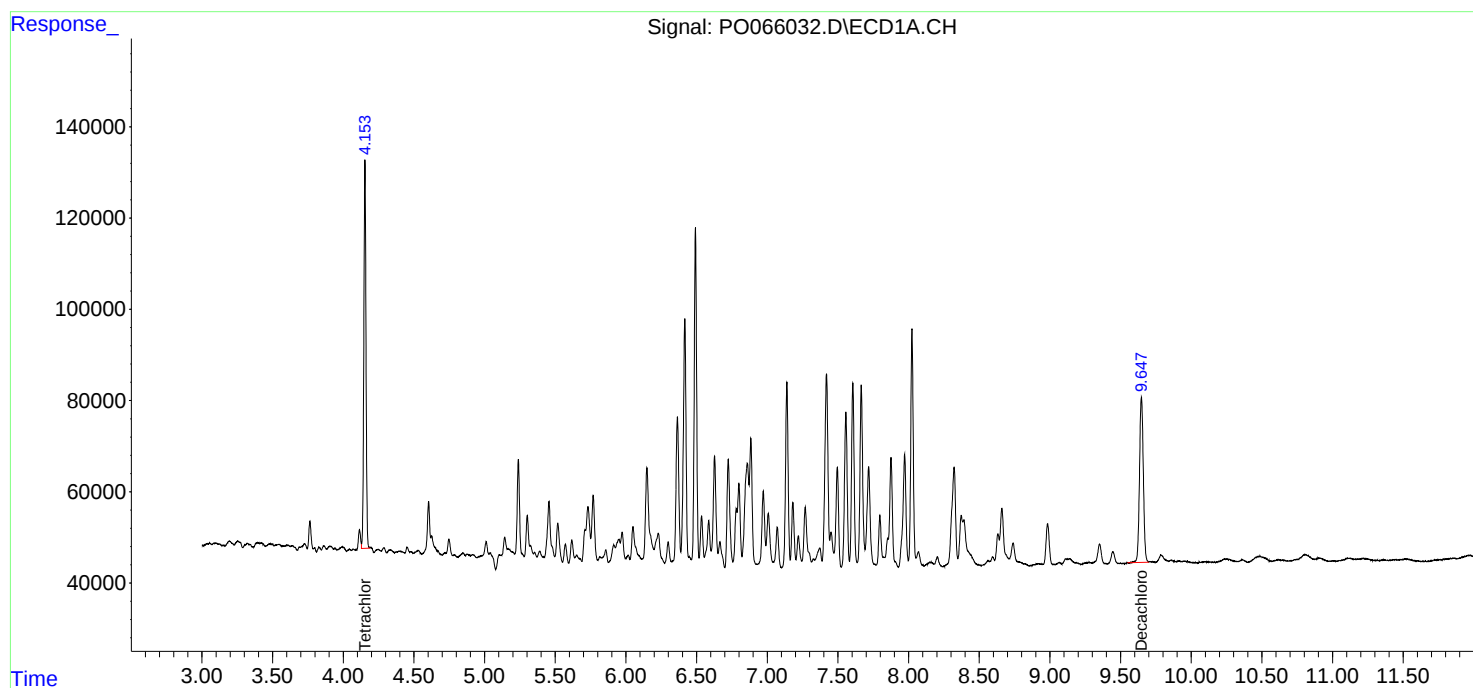

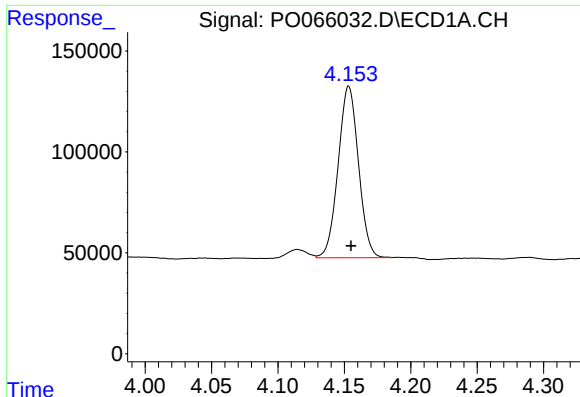


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: -0.002 min
Response: 905078
Conc: 39.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CTY-SB-BC-0-3.5RE


Manual Integrations
APPROVED

mohammad
1/30/2020 3:26:12 PM

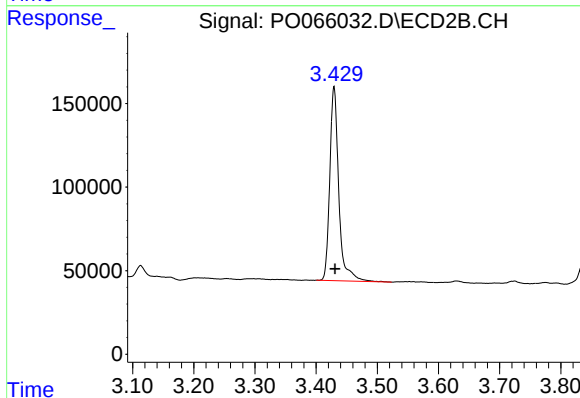


#1 Tetrachloro-m-xylene

R.T.: 3.429 min
Delta R.T.: -0.002 min
Response: 1187013
Conc: 44.69 ng/ml

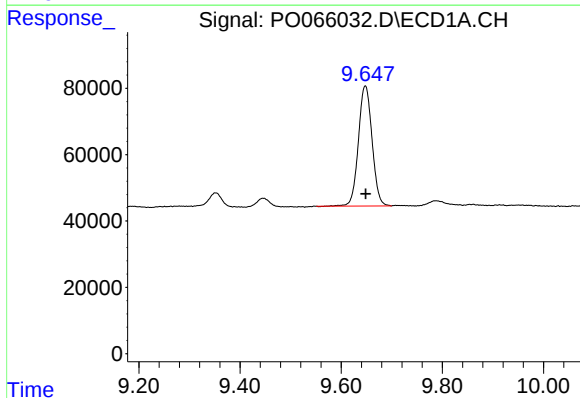

#2 Decachlorobiphenyl

R.T.: 9.648 min
Delta R.T.: -0.001 min
Response: 677619
Conc: 16.28 ng/ml

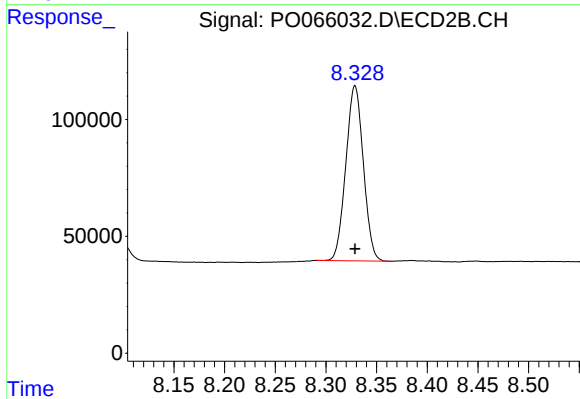

#2 Decachlorobiphenyl

R.T.: 8.329 min
Delta R.T.: 0.000 min
Response: 901150
Conc: 18.54 ng/ml