

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
 Data File : P0066035.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2020 19:09
 Operator : DD\AJ
 Sample : L1245-01RE
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20200063-AMENDED-COMP-1RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 01:31:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.148	3.426	643229	855506	27.740	32.209
2) SA Decachlor...	9.640	8.321	934770	1199225	22.456	24.677

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
Data File : P0066035.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2020 19:09
Operator : DD\AJ
Sample : L1245-01RE
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20200063-AMENDED-COMP-1RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 01:31:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

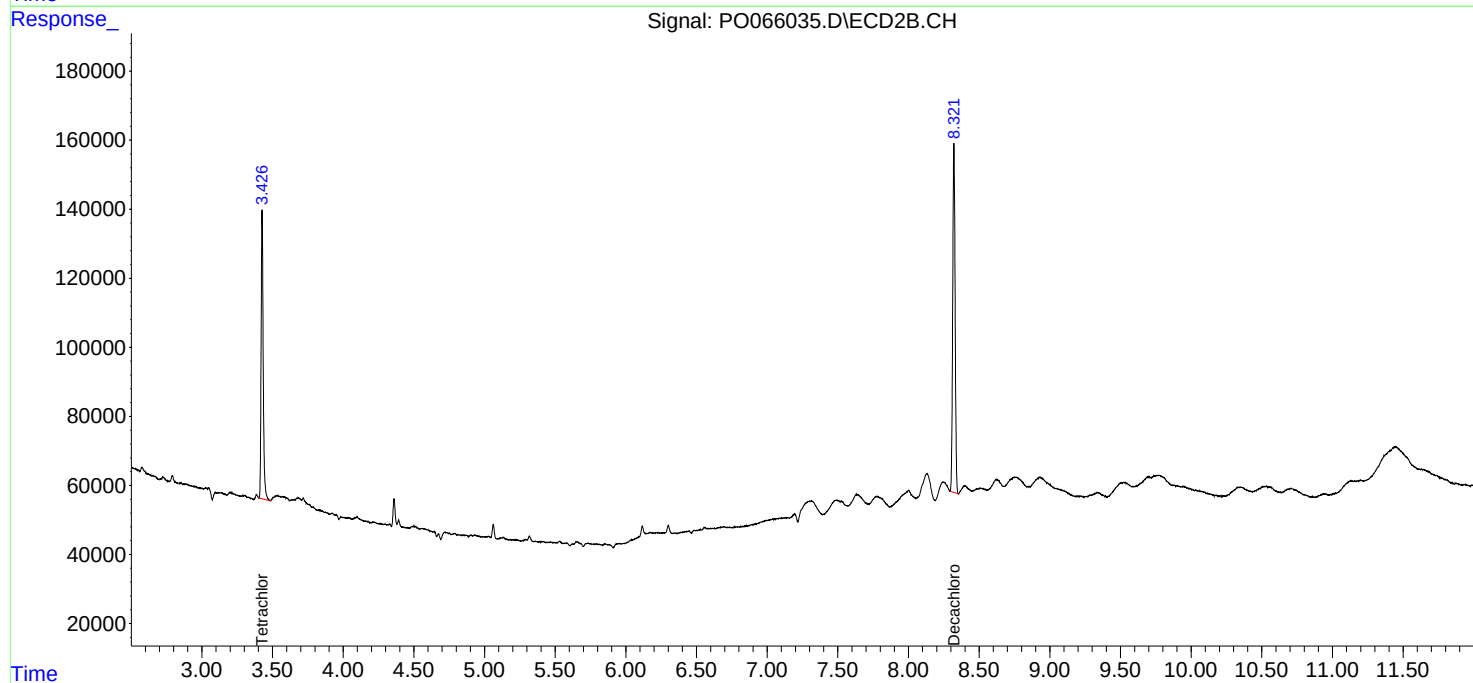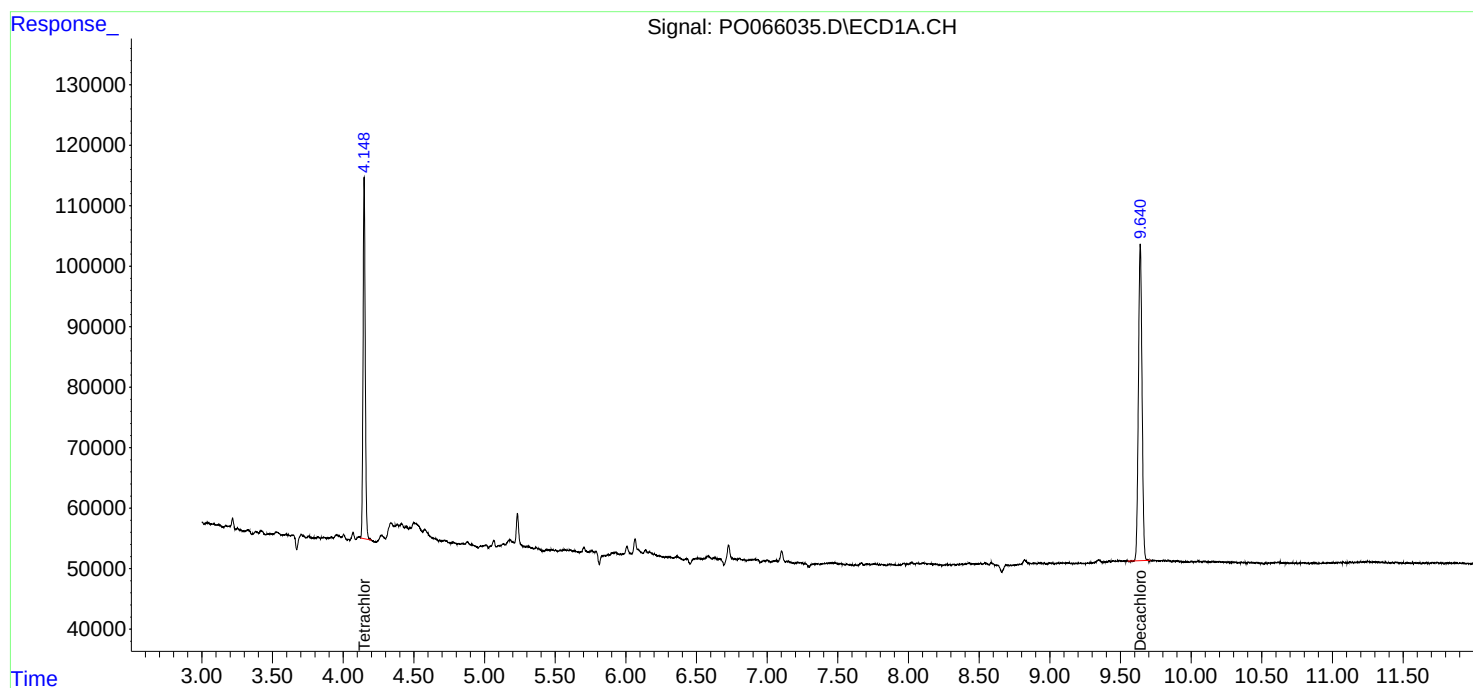


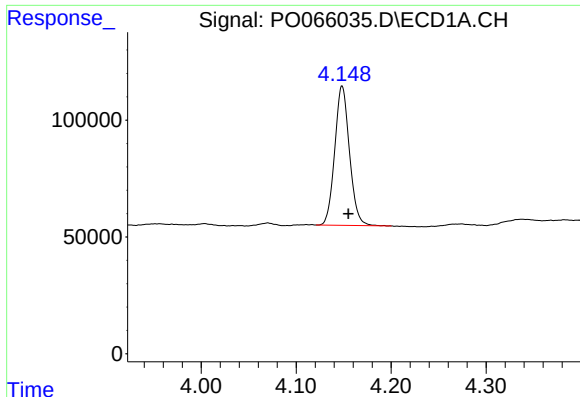

#1 Tetrachloro-m-xylene


R.T.: 4.148 min
Delta R.T.: -0.007 min
Response: 643229
Conc: 27.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
20200063-AMENDED-COMP-1RE

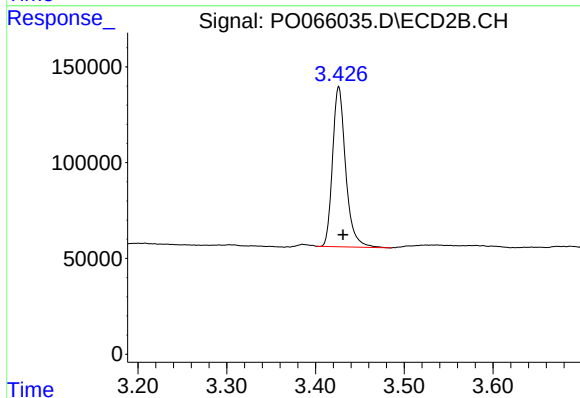


#1 Tetrachloro-m-xylene

R.T.: 3.426 min
Delta R.T.: -0.005 min
Response: 855506
Conc: 32.21 ng/ml

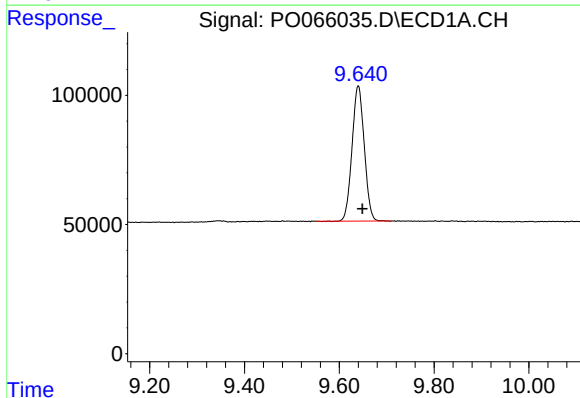

#2 Decachlorobiphenyl

R.T.: 9.640 min
Delta R.T.: -0.009 min
Response: 934770
Conc: 22.46 ng/ml

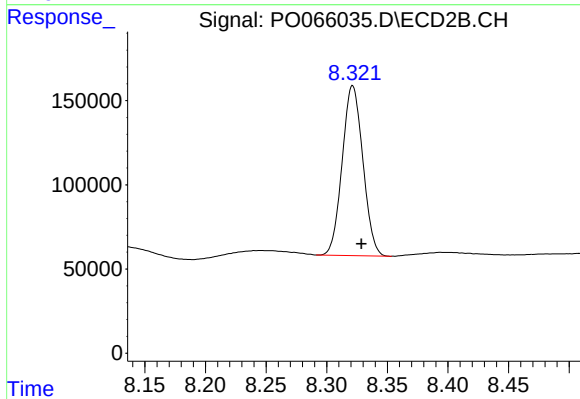

#2 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: -0.007 min
Response: 1199225
Conc: 24.68 ng/ml