

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
 Data File : P0066049.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Jan 2020 23:03
 Operator : DD\AJ
 Sample : L1289-29
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-35-34-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 01:36:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.147	3.424	755318	1049761	32.574	39.522
2) SA Decachlor...	9.638	8.321	1119586	1627527	26.896	33.491

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
Data File : P0066049.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2020 23:03
Operator : DD\AJ
Sample : L1289-29
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 01:36:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

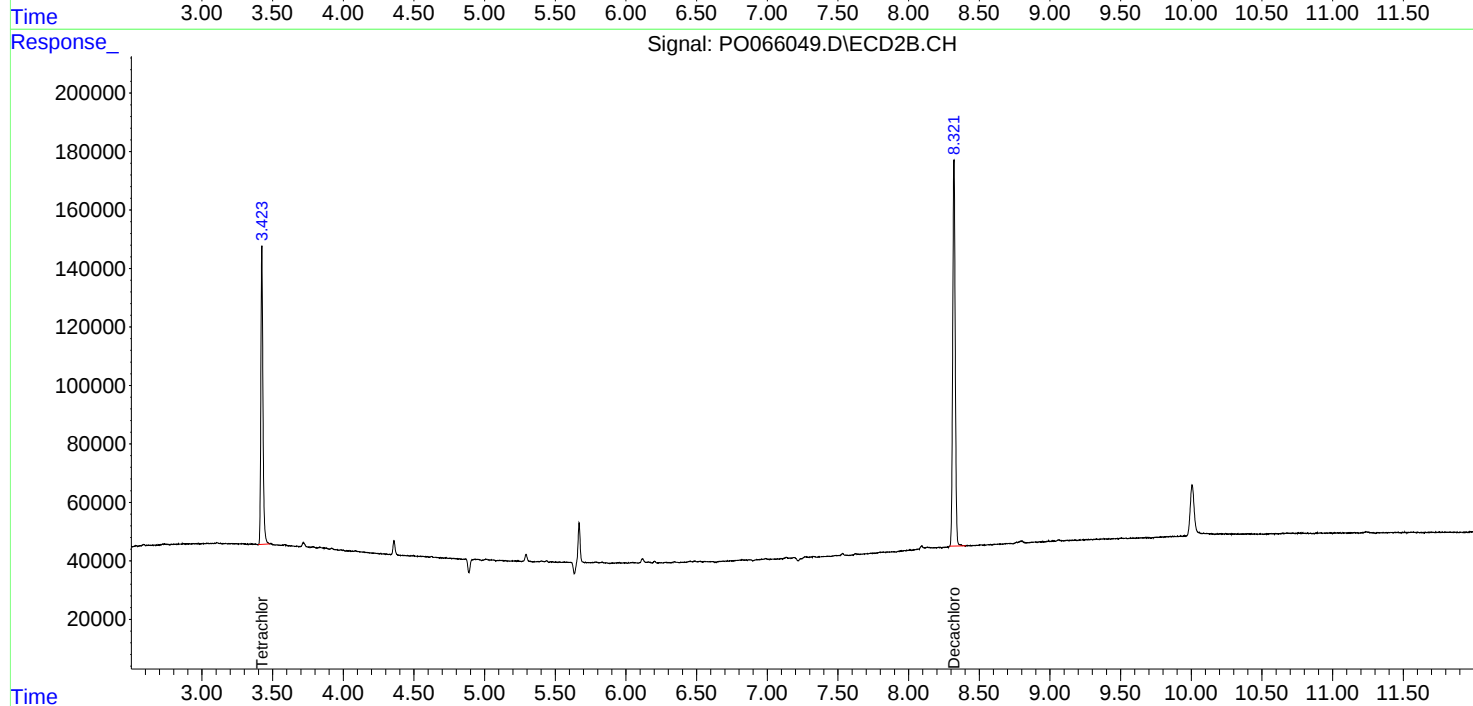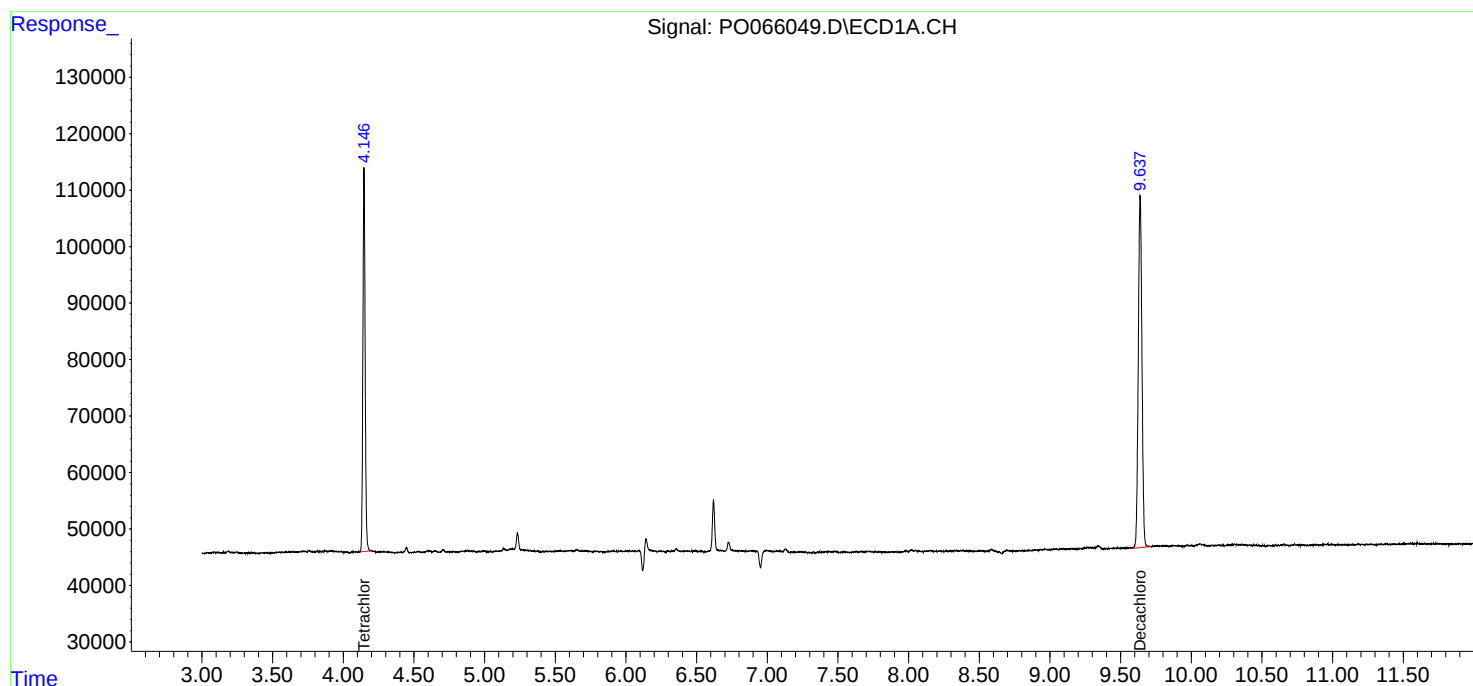


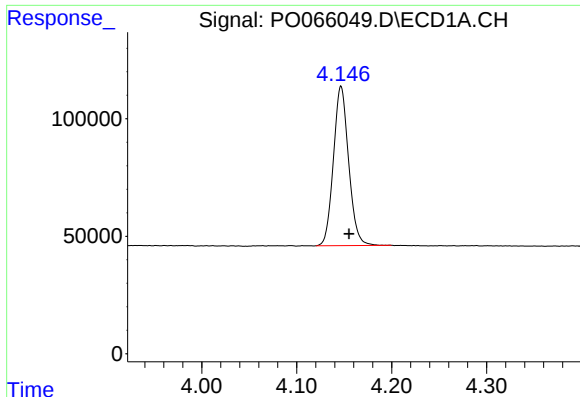

#1 Tetrachloro-m-xylene


R.T.: 4.147 min
Delta R.T.: -0.008 min
Response: 755318
Conc: 32.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-35-34-COMP

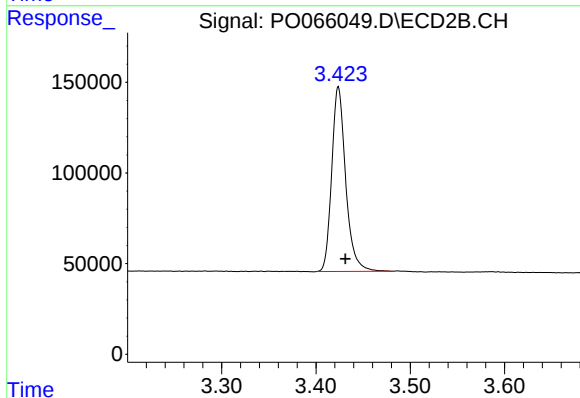


#1 Tetrachloro-m-xylene

R.T.: 3.424 min
Delta R.T.: -0.007 min
Response: 1049761
Conc: 39.52 ng/ml

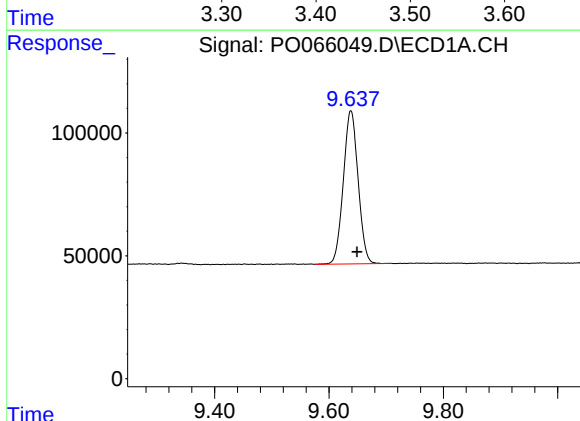

#2 Decachlorobiphenyl

R.T.: 9.638 min
Delta R.T.: -0.011 min
Response: 1119586
Conc: 26.90 ng/ml

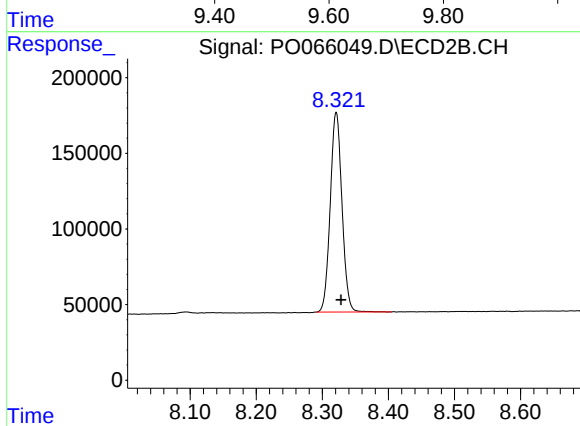

#2 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: -0.008 min
Response: 1627527
Conc: 33.49 ng/ml