

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
 Data File : P0066061.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jan 2020 2:58
 Operator : DD\AJ
 Sample : L1274-01
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BORING-B1-SAMPLE-S1

Manual Integrations
 APPROVED

mohammad
 1/30/2020 3:27:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:16:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.147	3.424	947762	1255753	40.873m	47.277m
2) SA Decachlor...	9.636	8.320	800882	1125889	19.239	23.168

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012920\
Data File : P0066061.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2020 2:58
Operator : DD\AJ
Sample : L1274-01
Misc :
ALS Vial : 66 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BORING-B1-SAMPLE-S1


Manual Integrations
APPROVED

mohammad
1/30/2020 3:27:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:16:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

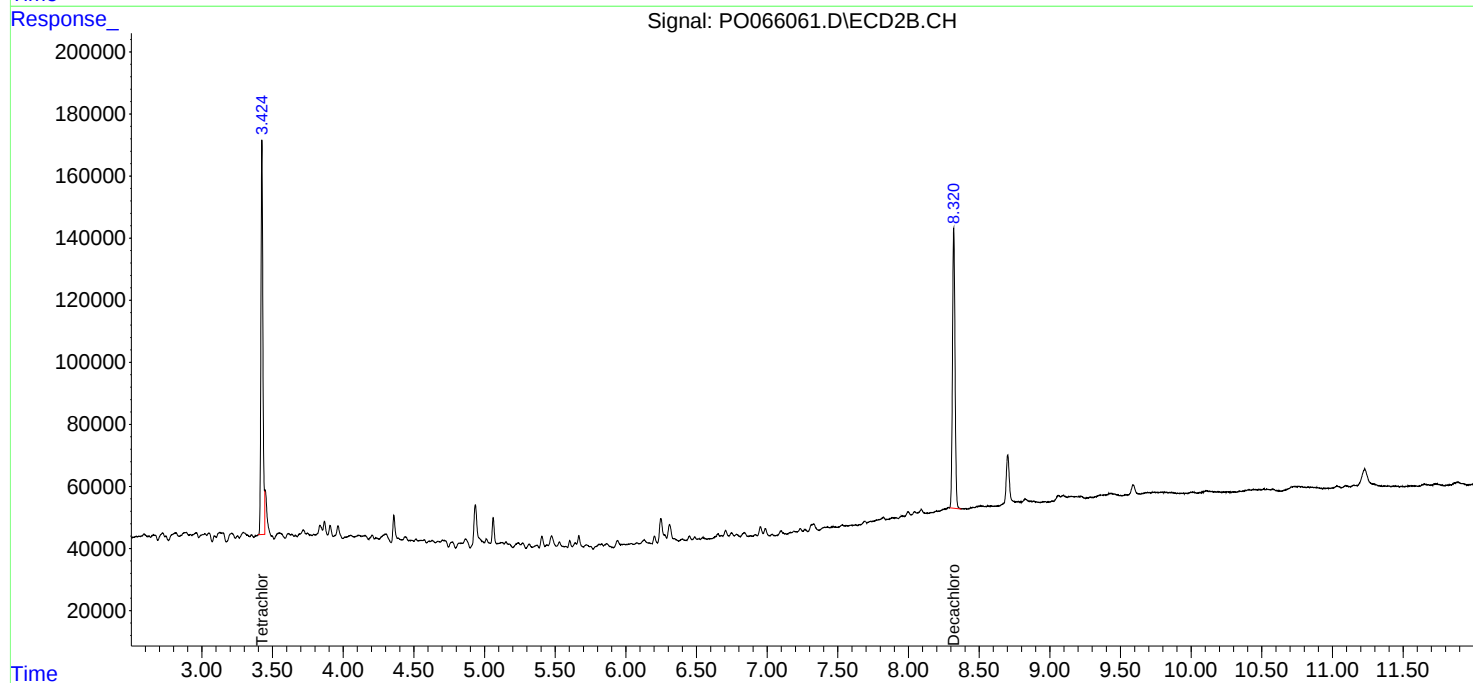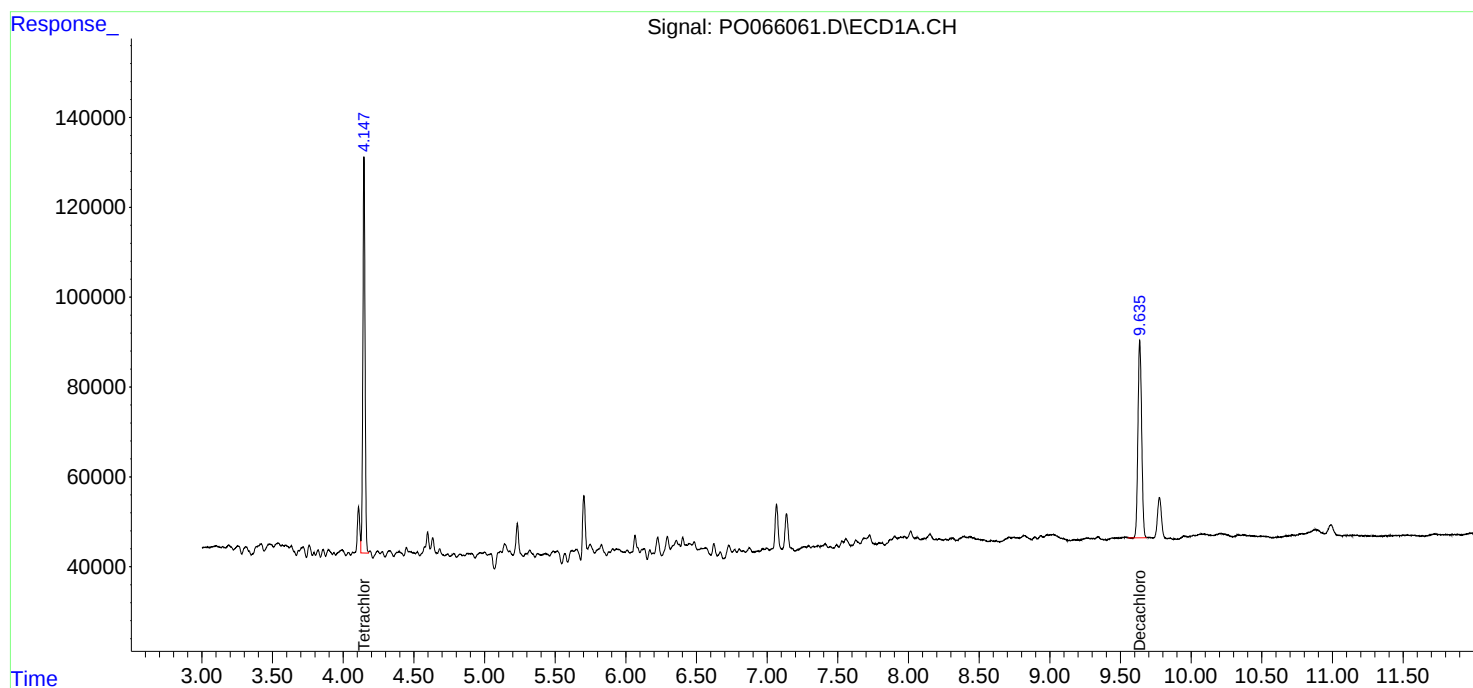

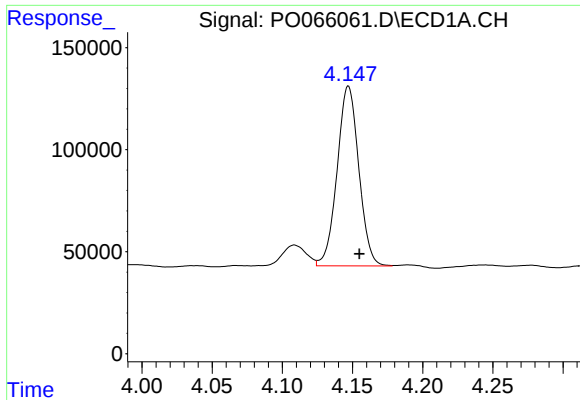


#1 Tetrachloro-m-xylene

R.T.: 4.147 min
Delta R.T.: -0.008 min
Response: 947762
Conc: 40.87 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BORING-B1-SAMPLE-S1


Manual Integrations
APPROVED

mohammad
1/30/2020 3:27:43 PM

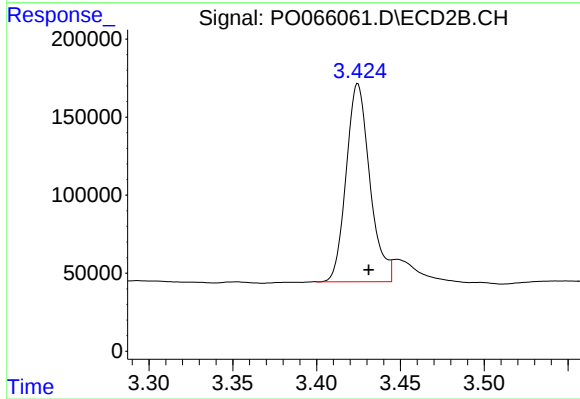


#1 Tetrachloro-m-xylene

R.T.: 3.424 min
Delta R.T.: -0.007 min
Response: 1255753
Conc: 47.28 ng/ml m

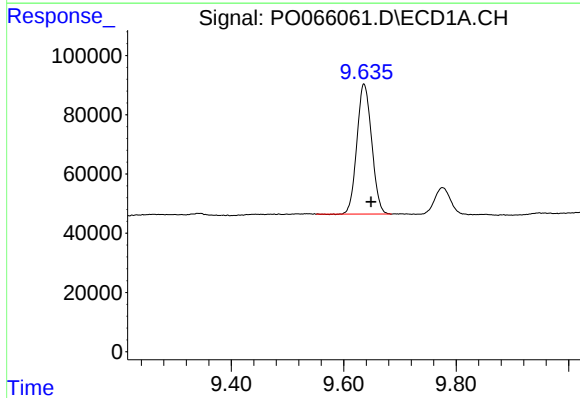

#2 Decachlorobiphenyl

R.T.: 9.636 min
Delta R.T.: -0.013 min
Response: 800882
Conc: 19.24 ng/ml

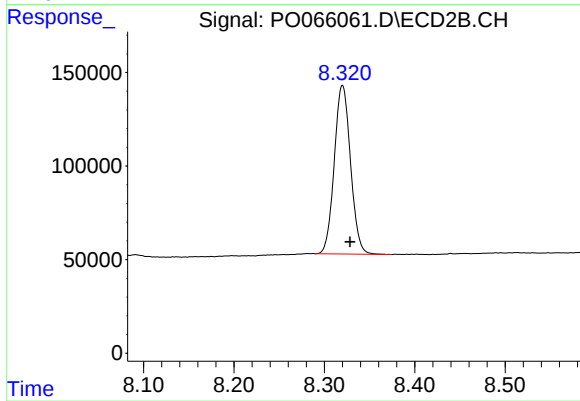

#2 Decachlorobiphenyl

R.T.: 8.320 min
Delta R.T.: -0.009 min
Response: 1125889
Conc: 23.17 ng/ml