

Data Path : P:\HPCHEM1\ECD 0\Data\P0013018\
Data File : P0041911.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2018 20:33
Operator : SM/UA
Sample : J1290-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-45-9.5-10.0

Manual Integrations
APPROVED

ugo
1/30/2018 3:28:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 22:23:36 2018
Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.121	3.365	4429303	6761209	22.949m	23.291m
2)	SA Decachlor...	9.524	8.161	3759819	4237178	16.002	11.848m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\P0013018\
Data File : P0041911.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Jan 2018 20:33
Operator : SM/UA
Sample : J1290-20
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-45-9.5-10.0


Manual Integrations
APPROVED

ugo
1/30/2018 3:28:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 22:23:36 2018
Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

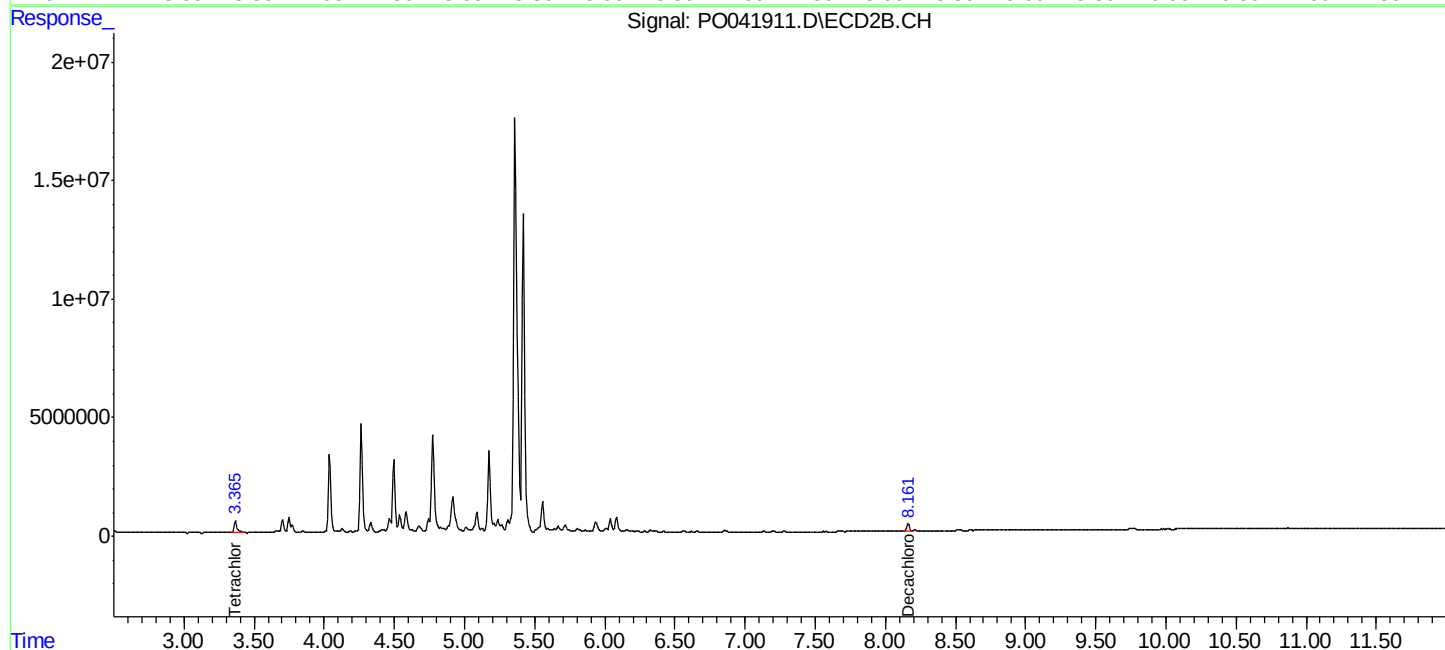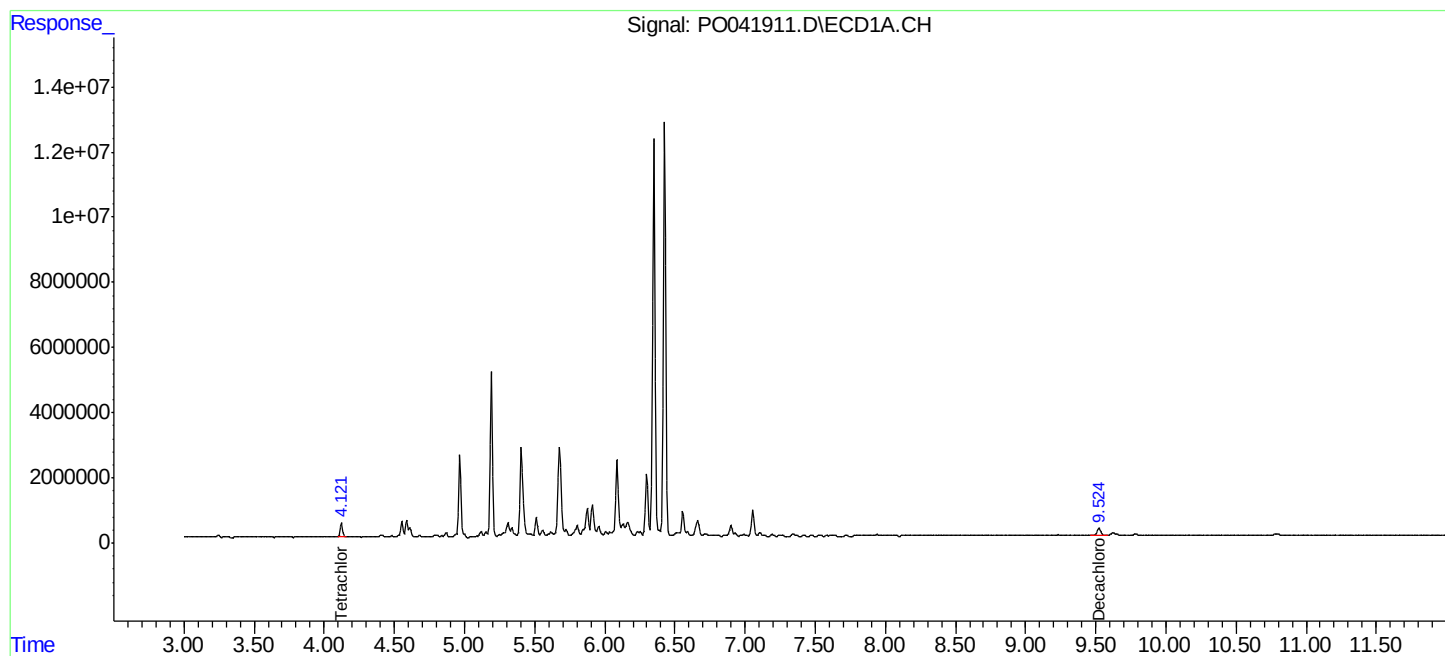

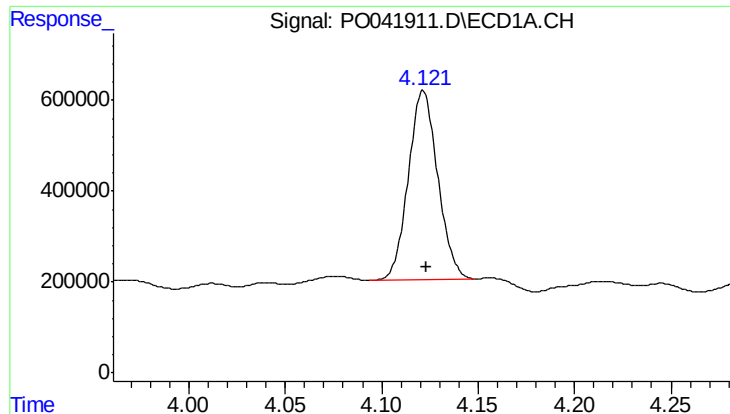


#1 Tetrachloro-m-xylene

R.T.: 4.121 min
Delta R.T.: -0.002 min
Response: 4429303
Conc: 22.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-45-9.5-10.0


Manual Integrations
APPROVED

ugo
1/30/2018 3:28:18 PM

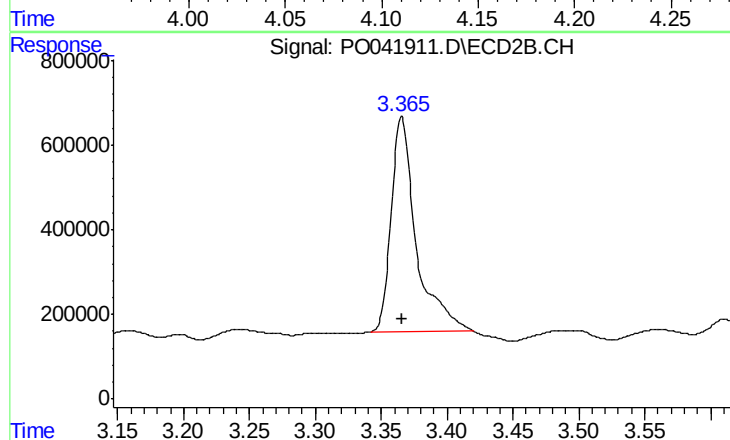


#1 Tetrachloro-m-xylene

R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 6761209
Conc: 23.29 ng/ml m

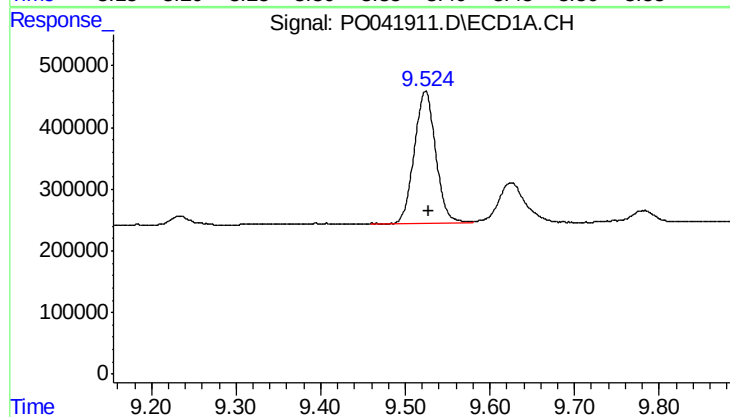

#2 Decachlorobiphenyl

R.T.: 9.524 min
Delta R.T.: -0.005 min
Response: 3759819
Conc: 16.00 ng/ml

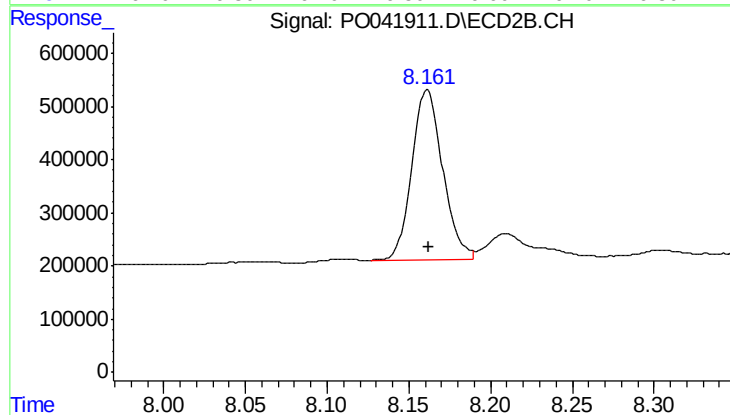

#2 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: -0.002 min
Response: 4237178
Conc: 11.85 ng/ml m