

Data Path : P:\HPCHEM1\ECD_0\Data\P0013118\
 Data File : P0041926.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Jan 2018 10:50
 Operator : SM/UA
 Sample : J1290-05RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-48-9.5-10.0RE

Manual Integrations
 APPROVED

ugo
 1/31/2018 9:12:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 13:25:54 2018
 Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 23 01:50:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.120	3.364	2872789	4914181	14.884	16.928m
2) SA Decachlor...	9.524	8.160	1961973	2102018	8.350	5.878m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0013118\
Data File : P0041926.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2018 10:50
Operator : SM/UA
Sample : J1290-05RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-48-9.5-10.0RE


Manual Integrations
APPROVED

ugo
1/31/2018 9:12:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 13:25:54 2018
Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

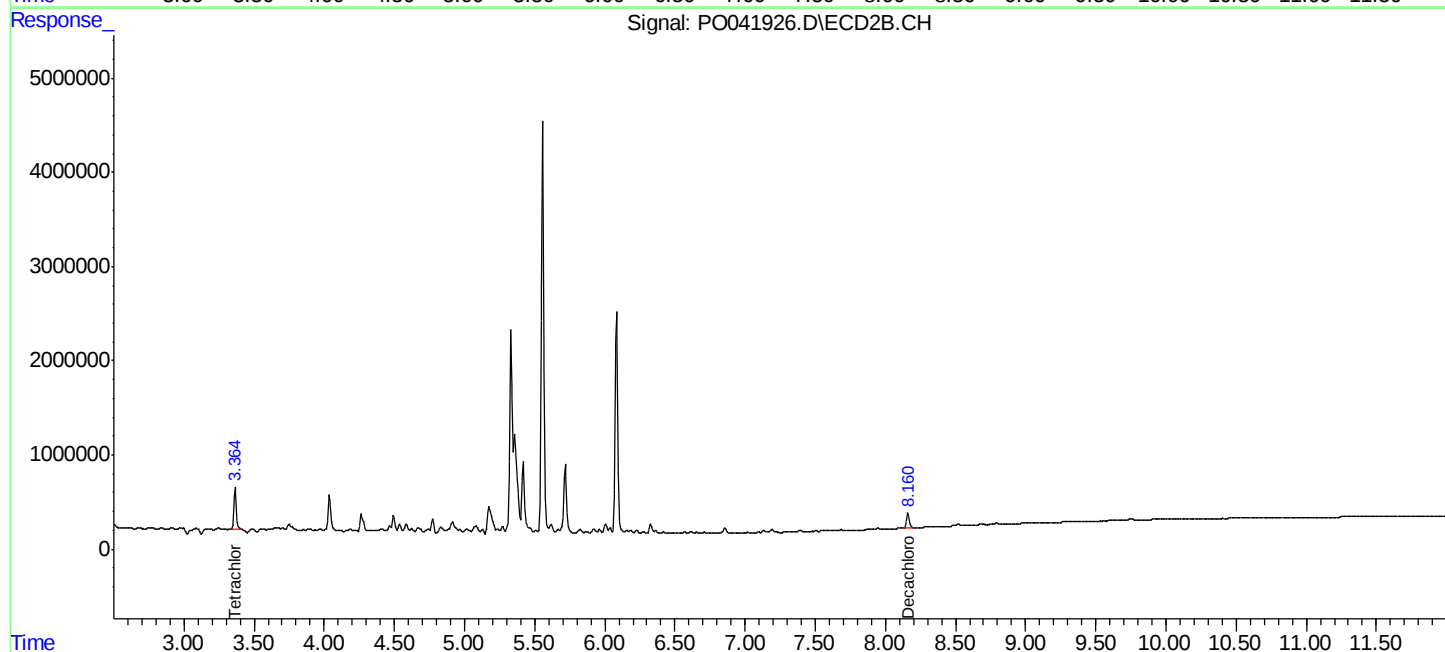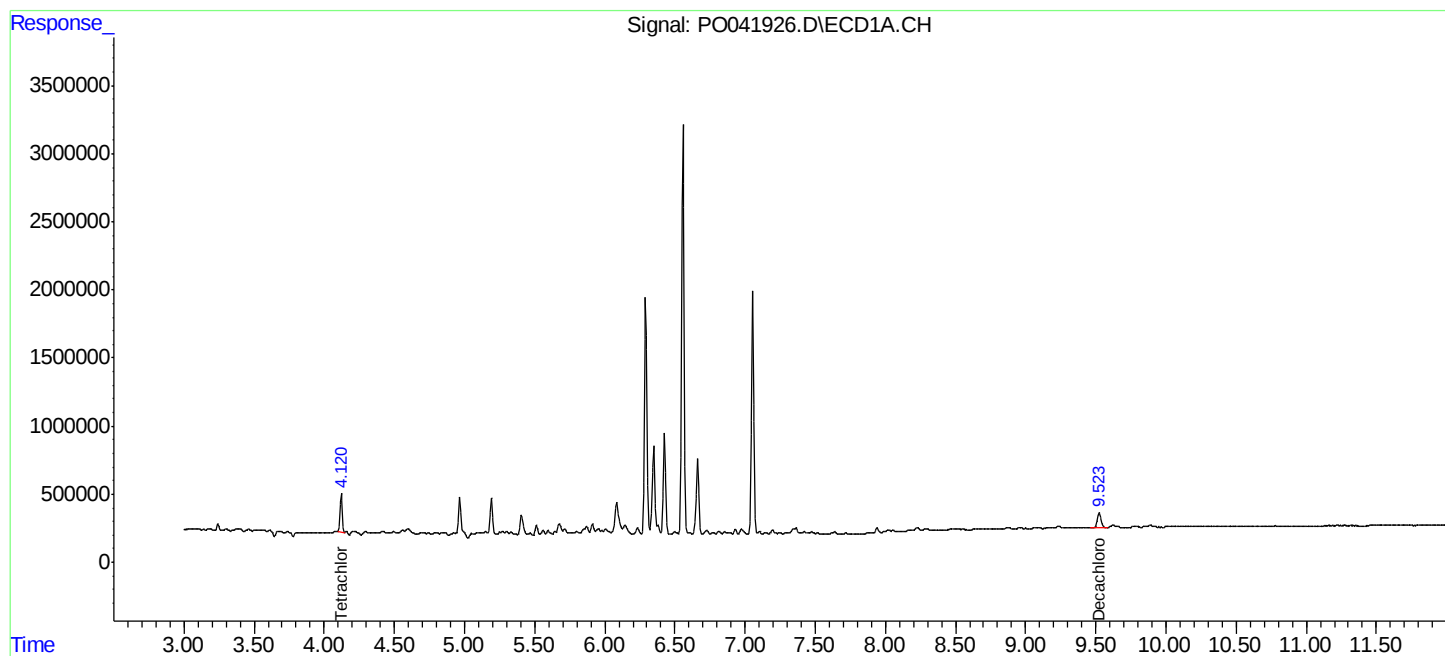

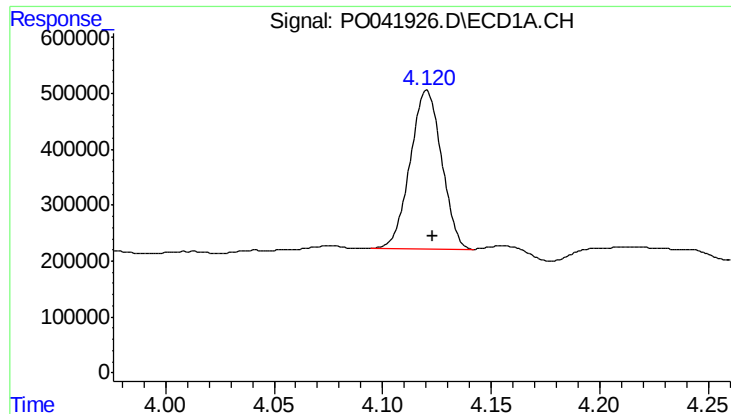


#1 Tetrachloro-m-xylene

R.T.: 4.120 min
Delta R.T.: -0.003 min
Response: 2872789
Conc: 14.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-48-9.5-10.0RE


Manual Integrations
APPROVED

ugo
1/31/2018 9:12:20 PM

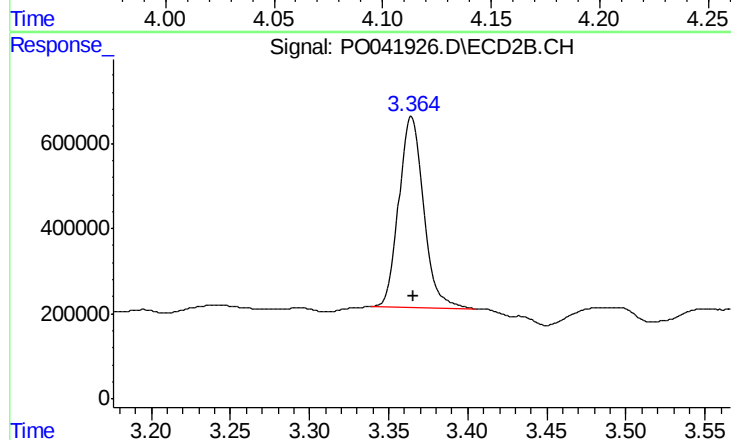


#1 Tetrachloro-m-xylene

R.T.: 3.364 min
Delta R.T.: -0.002 min
Response: 4914181
Conc: 16.93 ng/ml m

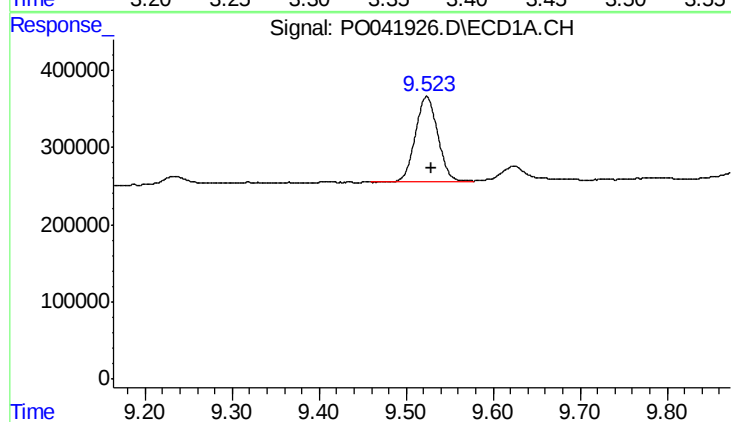

#2 Decachlorobiphenyl

R.T.: 9.524 min
Delta R.T.: -0.005 min
Response: 1961973
Conc: 8.35 ng/ml

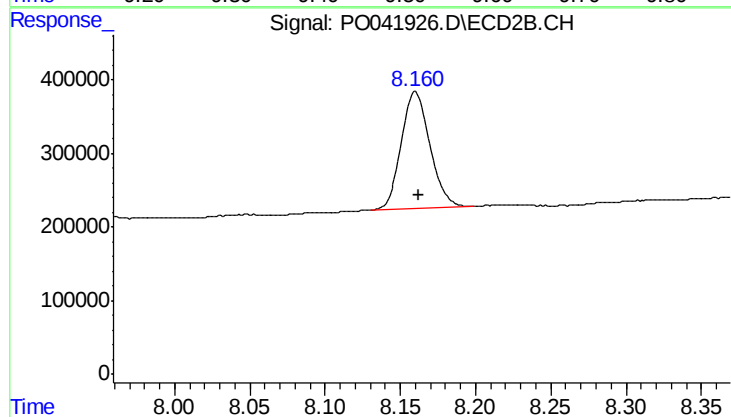

#2 Decachlorobiphenyl

R.T.: 8.160 min
Delta R.T.: -0.003 min
Response: 2102018
Conc: 5.88 ng/ml m