

Data Path : P:\HPCHEM1\ECD_0\Data\P0013118\
Data File : P0041936.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2018 13:21
Operator : SM/UA
Sample : J1290-20RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-45-9.5-10.0RE

Manual Integrations
APPROVED

ugo
1/31/2018 9:12:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 14:12:29 2018
Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.122	3.365	5582535	6312288	28.924	21.745m
2)	SA Decachlor...	9.525	8.160	3609620	4198633	15.363	11.741m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0013118\
Data File : P0041936.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Jan 2018 13:21
Operator : SM/UA
Sample : J1290-20RE
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-45-9.5-10.0RE


Manual Integrations
APPROVED

ugo
1/31/2018 9:12:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 14:12:29 2018
Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

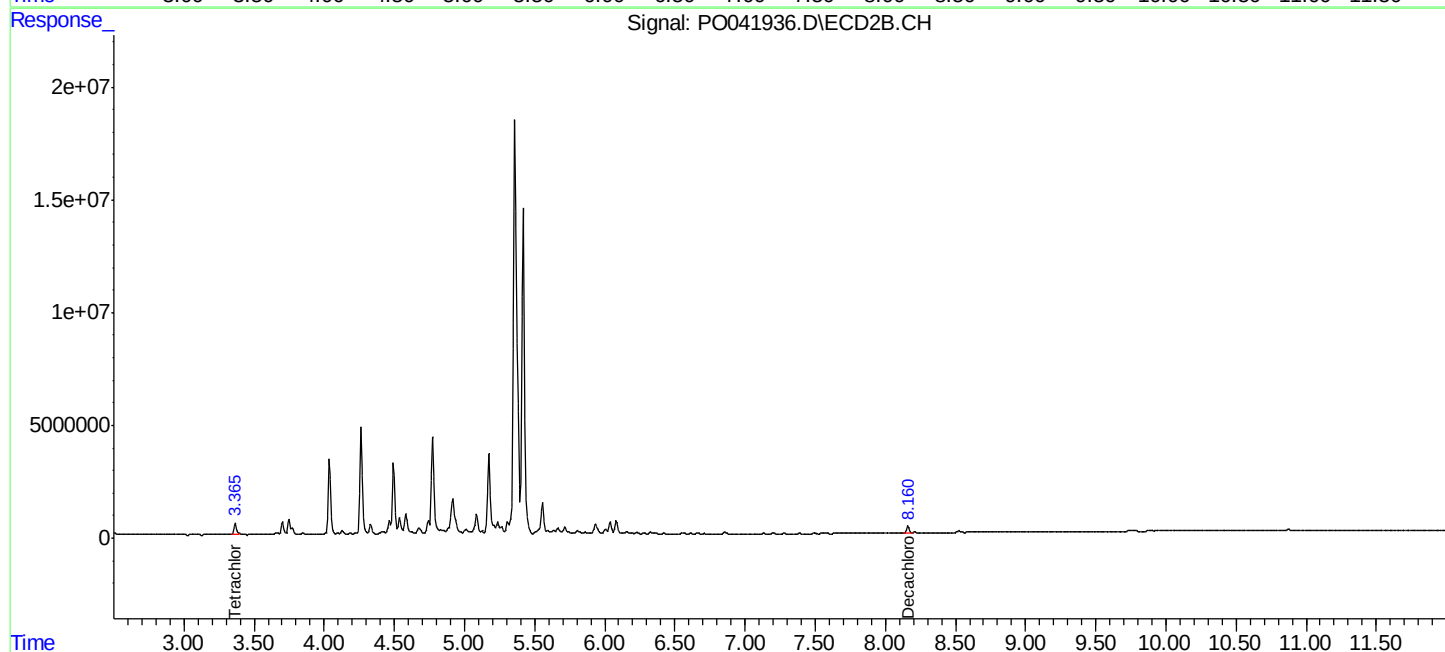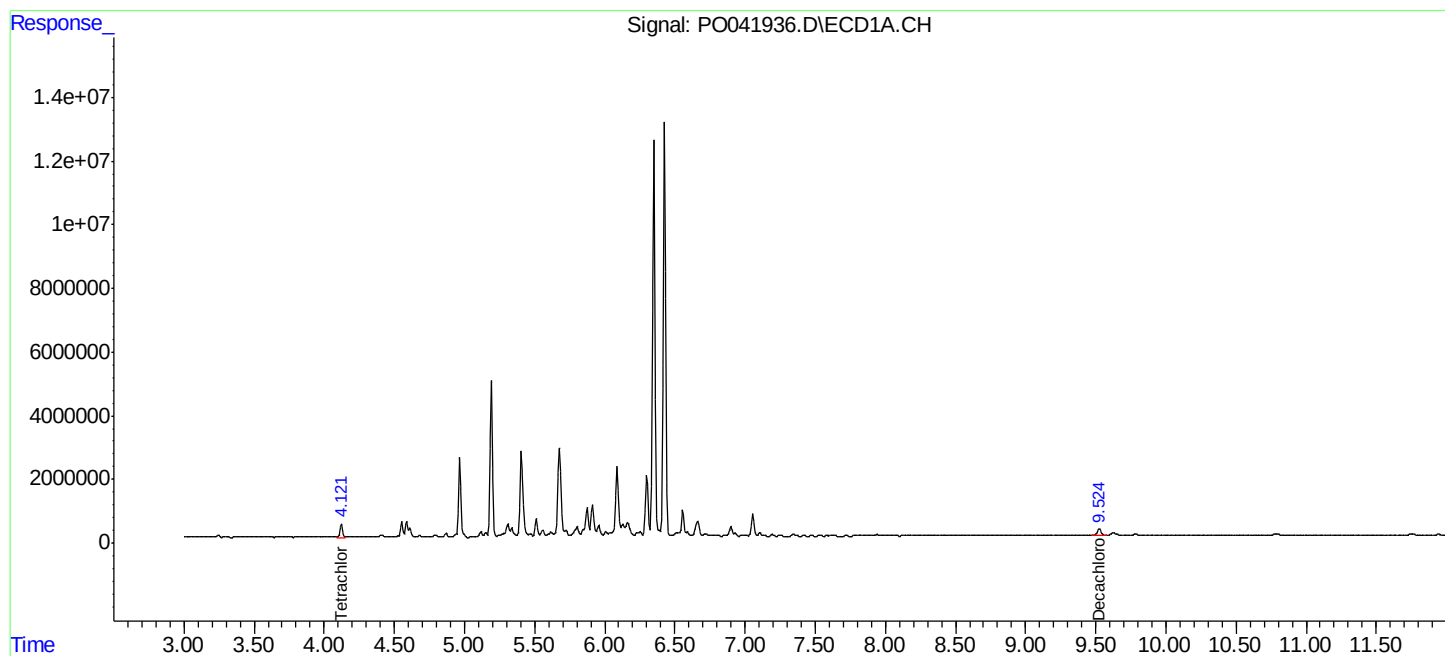

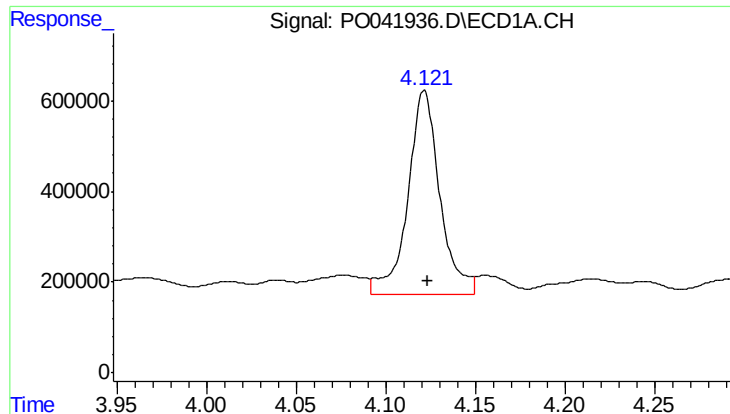


#1 Tetrachloro-m-xylene

R.T.: 4.122 min
Delta R.T.: -0.002 min
Response: 5582535
Conc: 28.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-45-9.5-10.0RE


Manual Integrations
APPROVED

ugo
1/31/2018 9:12:49 PM

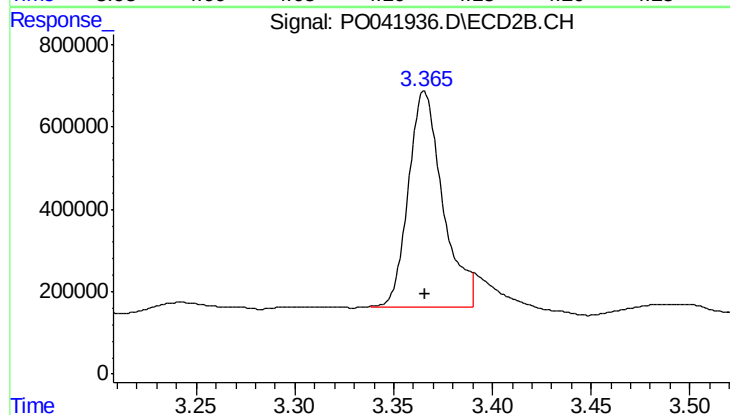


#1 Tetrachloro-m-xylene

R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 6312288
Conc: 21.74 ng/ml m

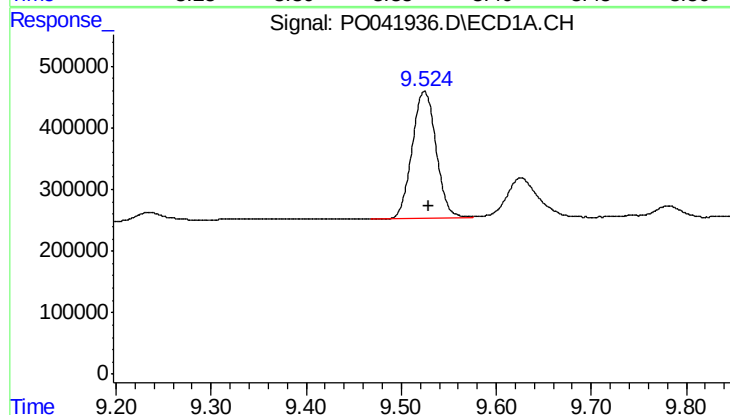

#2 Decachlorobiphenyl

R.T.: 9.525 min
Delta R.T.: -0.004 min
Response: 3609620
Conc: 15.36 ng/ml

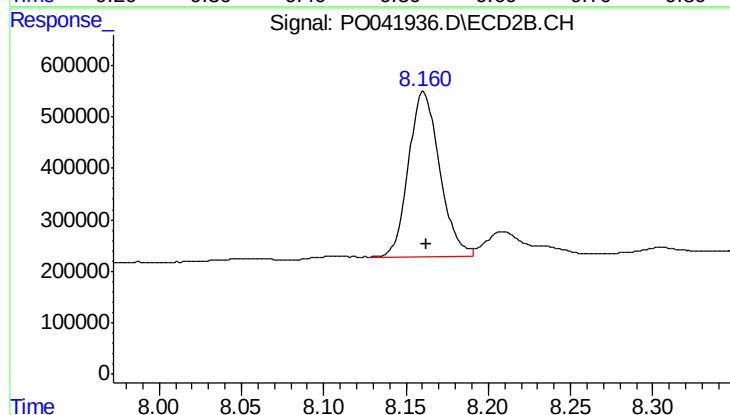

#2 Decachlorobiphenyl

R.T.: 8.160 min
Delta R.T.: -0.002 min
Response: 4198633
Conc: 11.74 ng/ml m