

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013120\
 Data File : P0066158.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jan 2020 15:57
 Operator : DD\AJ
 Sample : L1319-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RAINEY-PARK-BH-06-C

Manual Integrations
 APPROVED

mohammad
 2/4/2020 12:22:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 04:58:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.149	3.424	677734	915756	23.265m	22.388
2) SA Decachlor...	9.636	8.318	862780	1203278	21.893	20.530

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013120\
Data File : P0066158.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jan 2020 15:57
Operator : DD\AJ
Sample : L1319-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RAINEY-PARK-BH-06-C


Manual Integrations
APPROVED

mohammad
2/4/2020 12:22:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 04:58:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

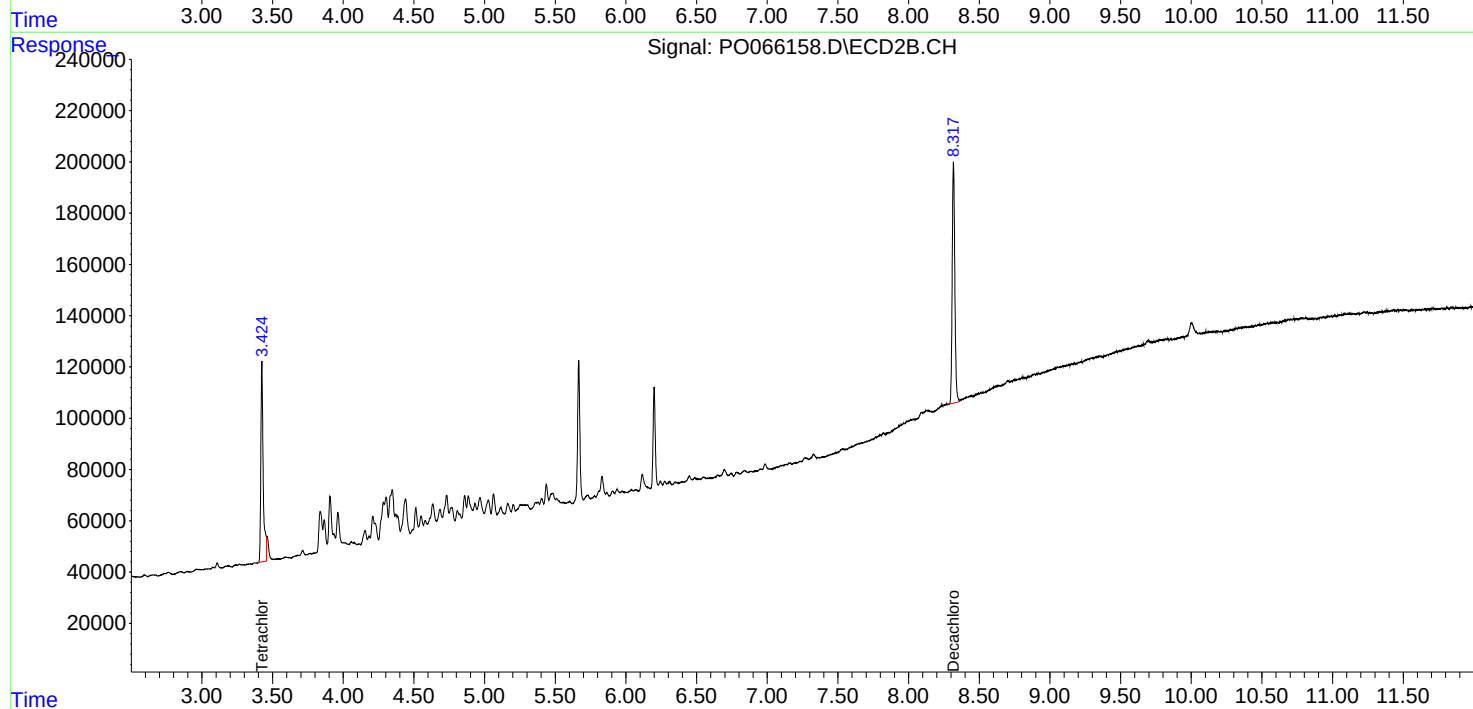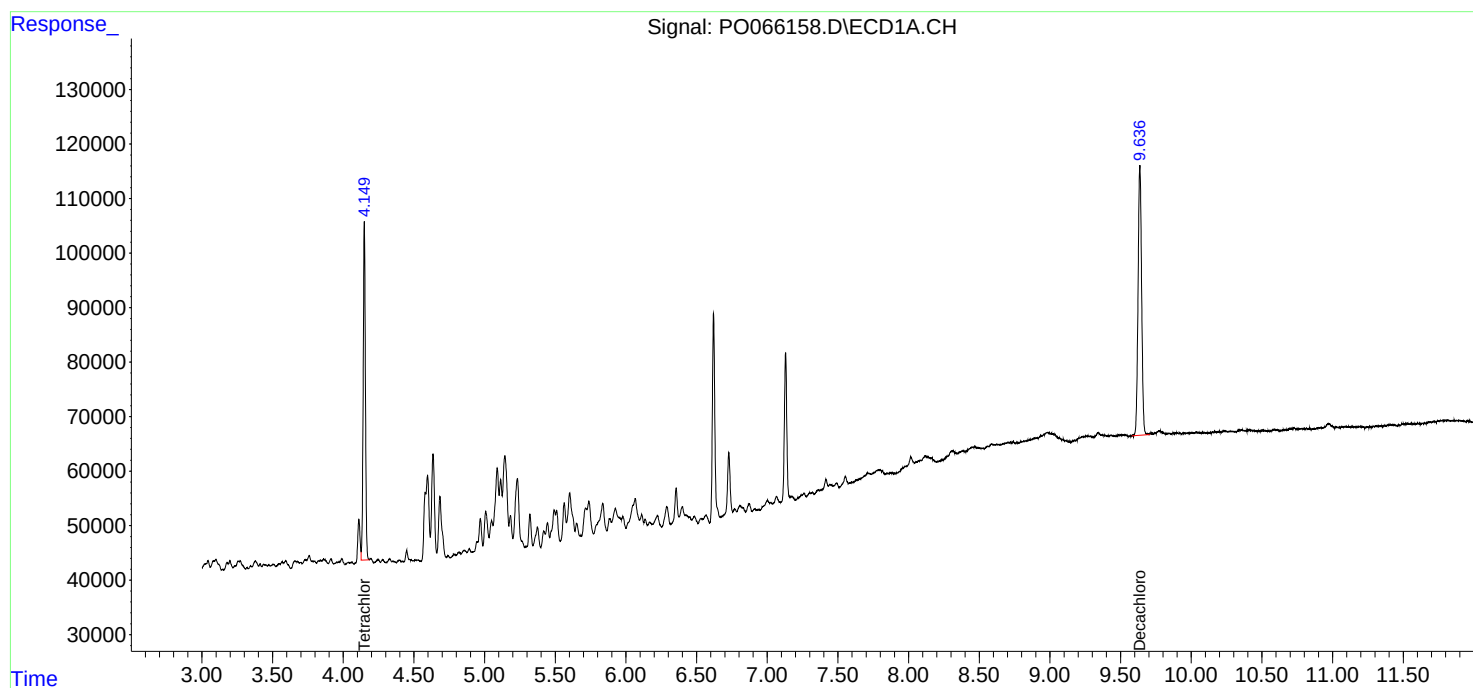

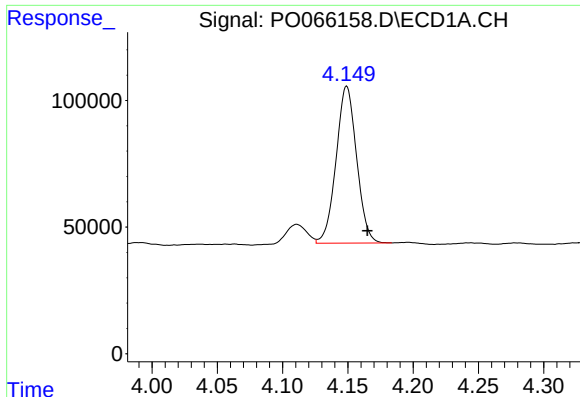


#1 Tetrachloro-m-xylene

R.T.: 4.149 min
Delta R.T.: -0.016 min
Response: 677734
Conc: 23.27 ng/ml m

Instrument :
ECD_O
ClientSampleId :
RAINEY-PARK-BH-06-C


Manual Integrations
APPROVED

mohammad
2/4/2020 12:22:27 PM

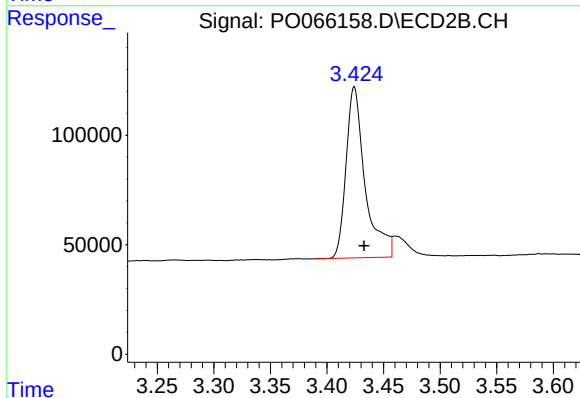


#1 Tetrachloro-m-xylene

R.T.: 3.424 min
Delta R.T.: -0.009 min
Response: 915756
Conc: 22.39 ng/ml

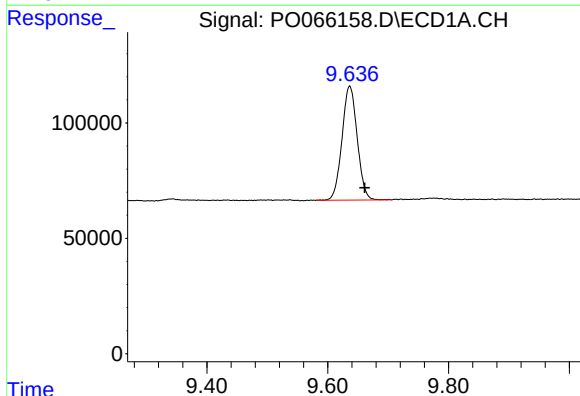

#2 Decachlorobiphenyl

R.T.: 9.636 min
Delta R.T.: -0.025 min
Response: 862780
Conc: 21.89 ng/ml

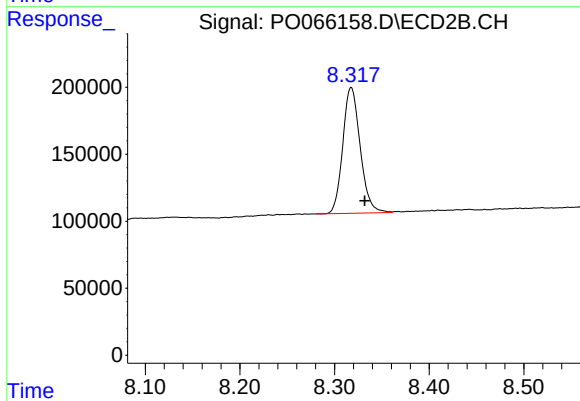

#2 Decachlorobiphenyl

R.T.: 8.318 min
Delta R.T.: -0.014 min
Response: 1203278
Conc: 20.53 ng/ml