

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013120\
 Data File : P0066162.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jan 2020 17:04
 Operator : DD\AJ
 Sample : L1319-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RAINEY-PARK-BH-01-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 04:26:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.145	3.422	678911	1010660	23.306	24.708
2) SA Decachlor...	9.632	8.316	804825	1095556	20.423	18.692

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013120\
Data File : P0066162.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jan 2020 17:04
Operator : DD\AJ
Sample : L1319-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RAINEY-PARK-BH-01-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 04:26:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

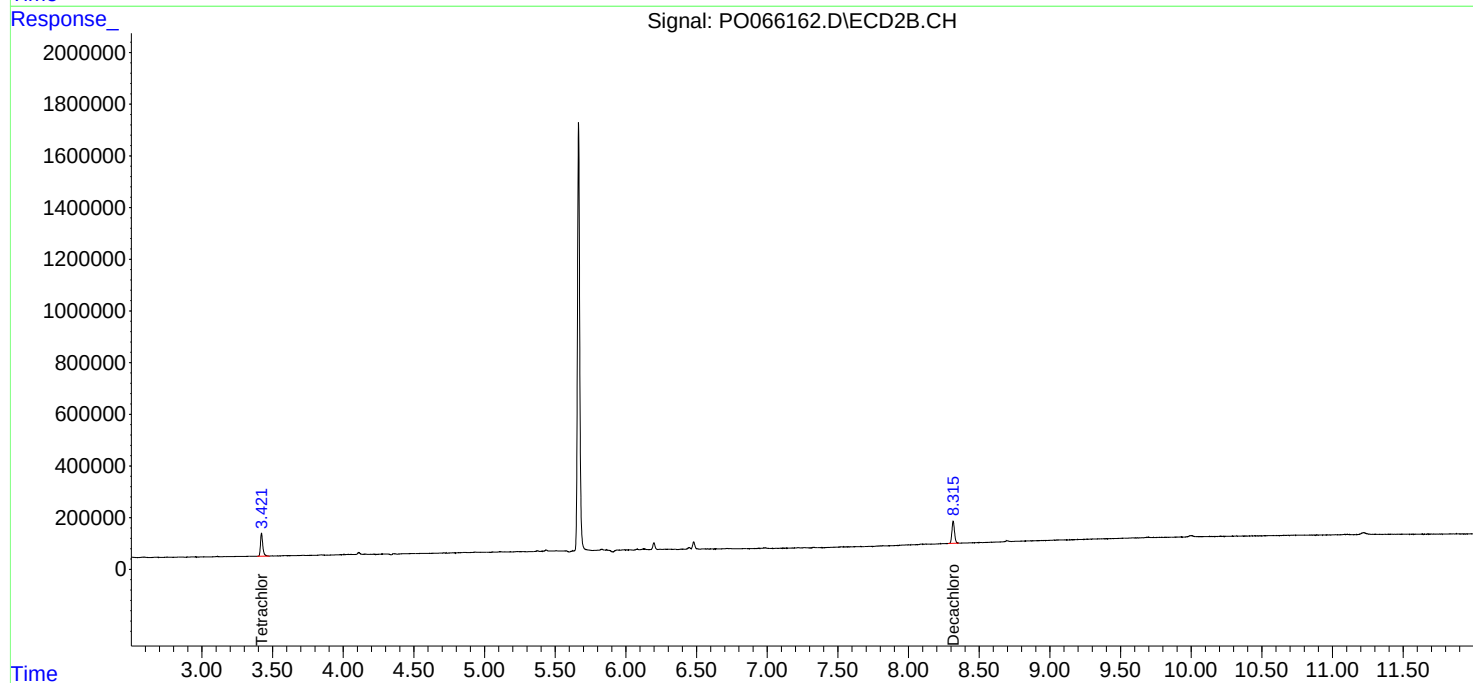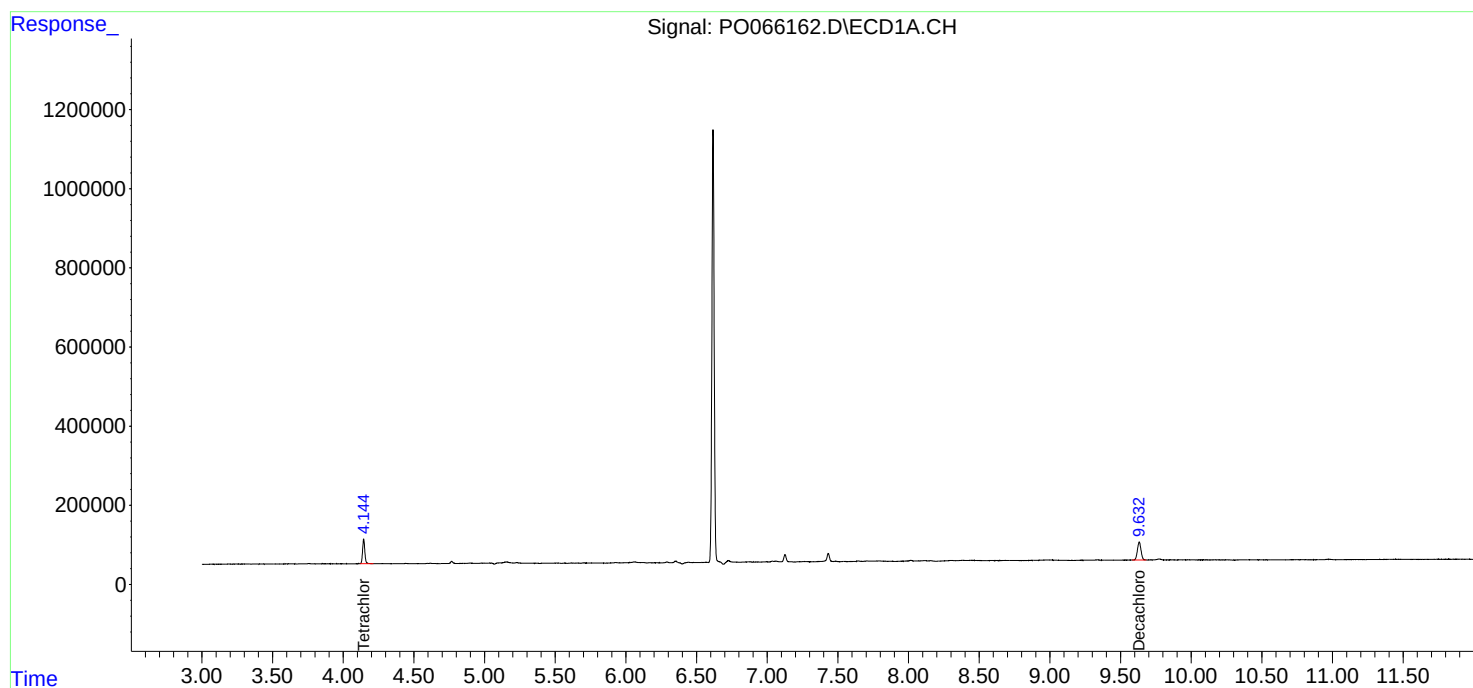


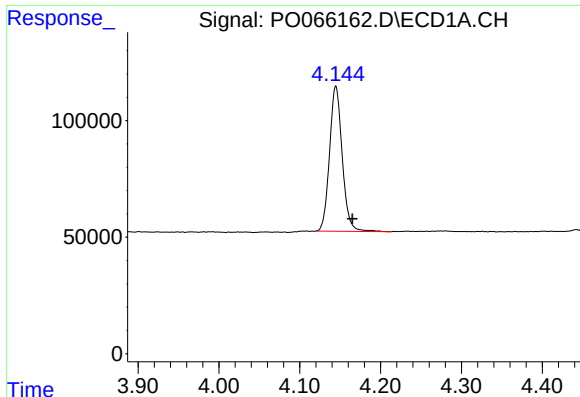

#1 Tetrachloro-m-xylene


R.T.: 4.145 min
Delta R.T.: -0.020 min
Response: 678911
Conc: 23.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
RAINEY-PARK-BH-01-B

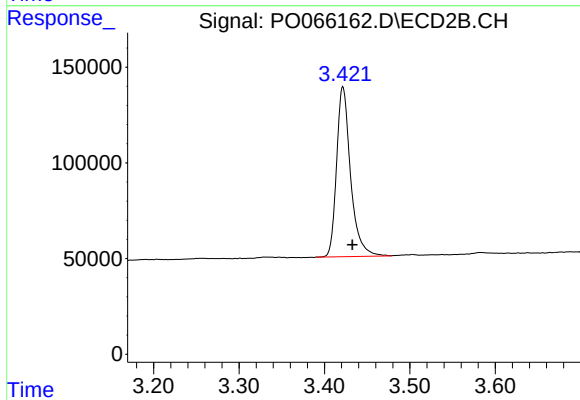


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.011 min
Response: 1010660
Conc: 24.71 ng/ml

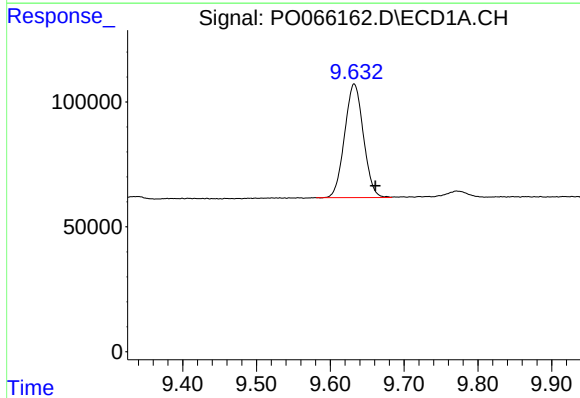

#2 Decachlorobiphenyl

R.T.: 9.632 min
Delta R.T.: -0.029 min
Response: 804825
Conc: 20.42 ng/ml

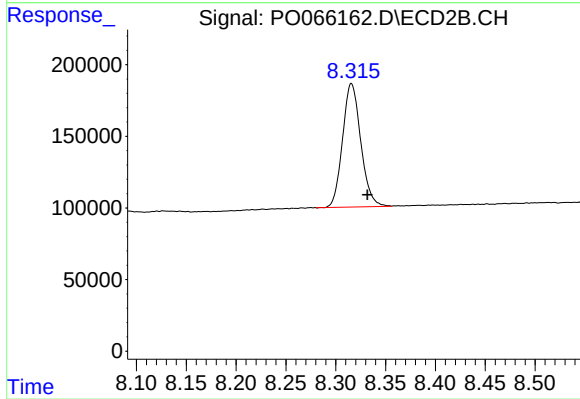

#2 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: -0.016 min
Response: 1095556
Conc: 18.69 ng/ml