

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013120\
 Data File : P0066180.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Jan 2020 22:06
 Operator : DD\AJ
 Sample : L1329-19
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-5

Manual Integrations
 APPROVED

mohammad
 2/4/2020 12:24:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 04:39:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 31 01:14:46 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.146	3.424	311966	359344	10.709	8.785
2)	SA Decachlor...	9.630	8.313	87204	118499	2.213m	2.022m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0013120\
Data File : P0066180.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Jan 2020 22:06
Operator : DD\AJ
Sample : L1329-19
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-5


Manual Integrations
APPROVED

mohammad
2/4/2020 12:24:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 04:39:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013020.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 31 01:14:46 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

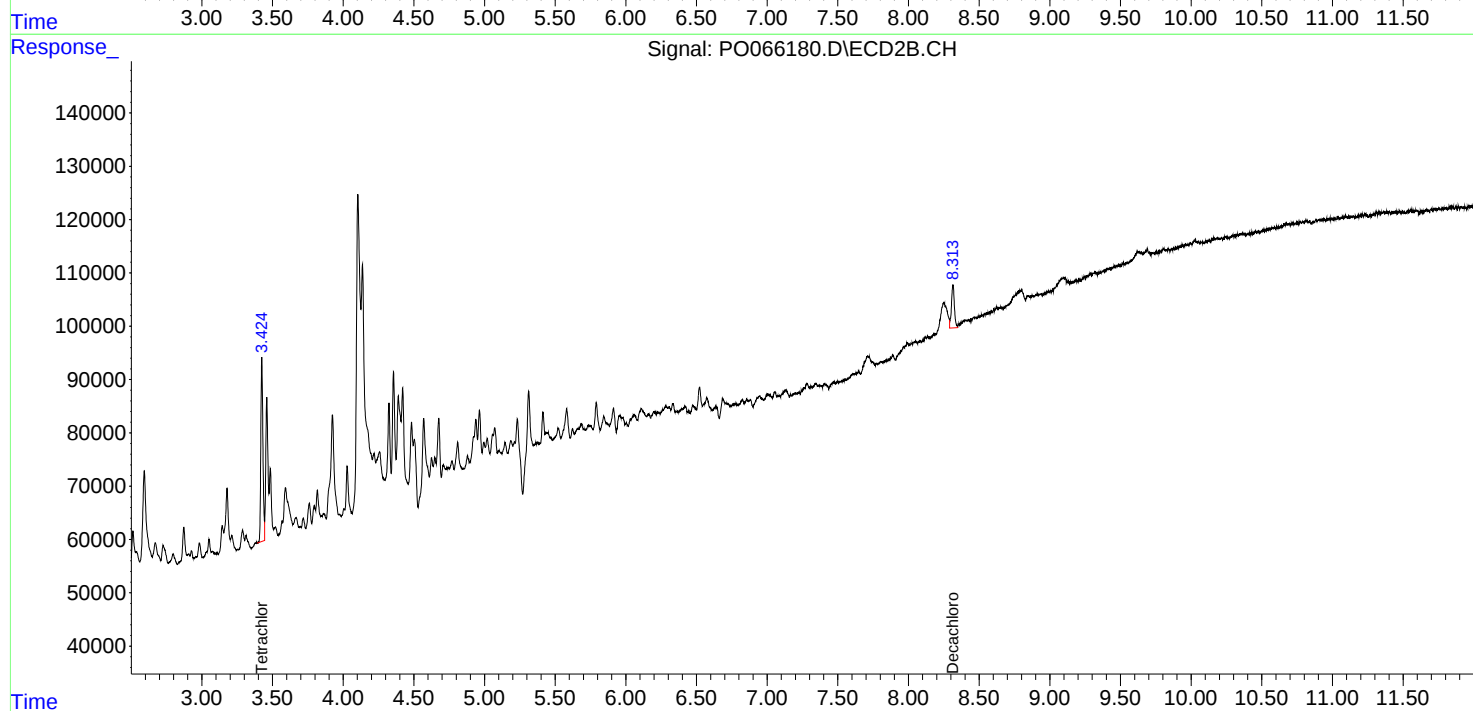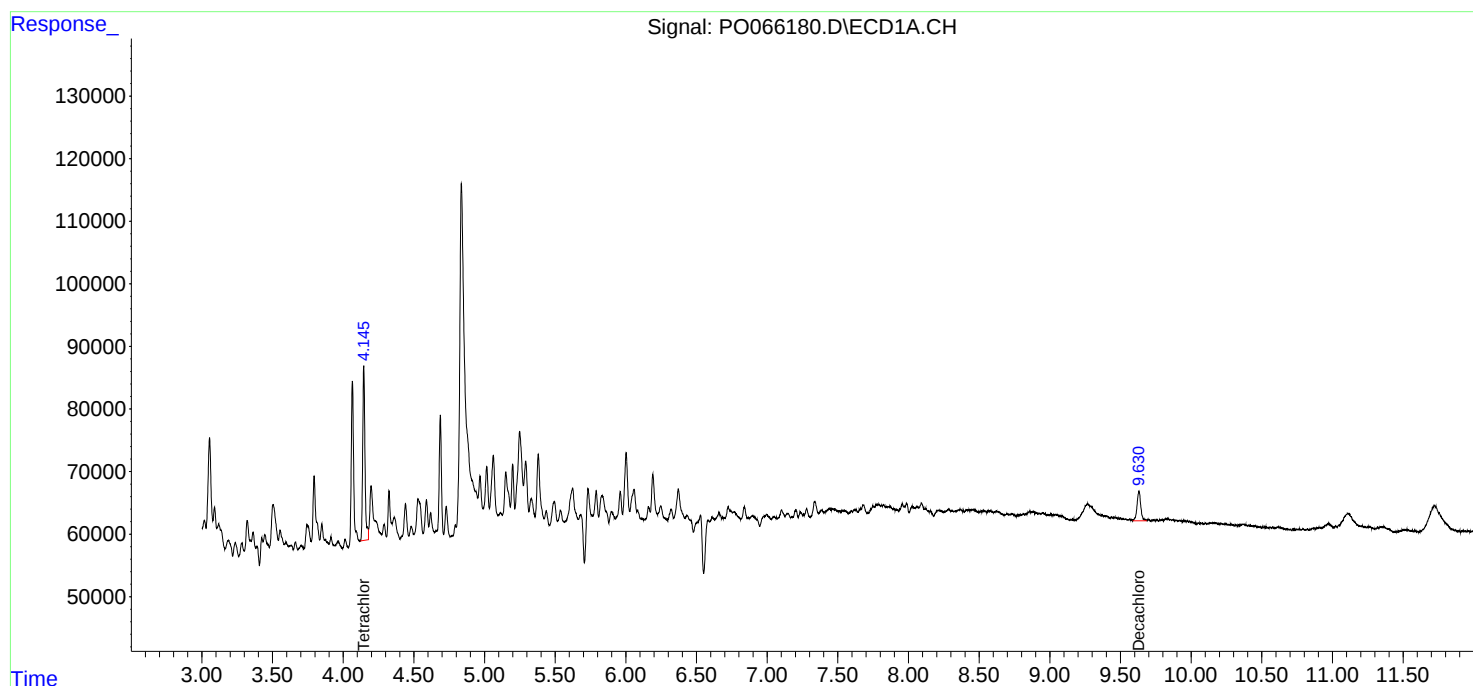

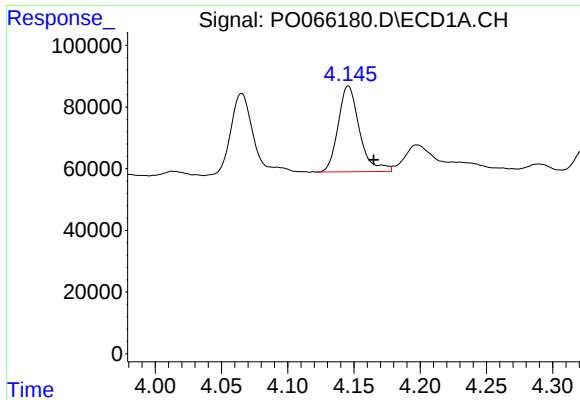


#1 Tetrachloro-m-xylene

R.T.: 4.146 min
Delta R.T.: -0.019 min
Response: 311966
Conc: 10.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-5


Manual Integrations
APPROVED

mohammad
2/4/2020 12:24:02 PM

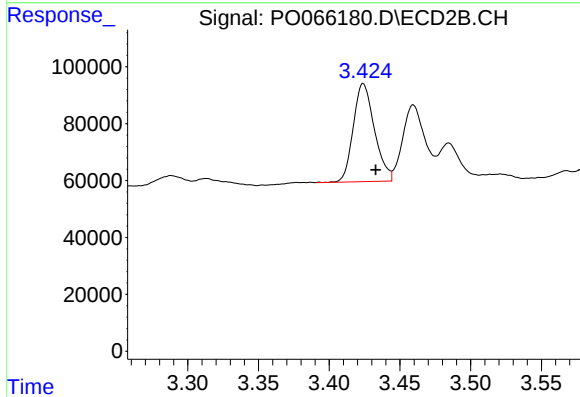


#1 Tetrachloro-m-xylene

R.T.: 3.424 min
Delta R.T.: -0.009 min
Response: 359344
Conc: 8.78 ng/ml

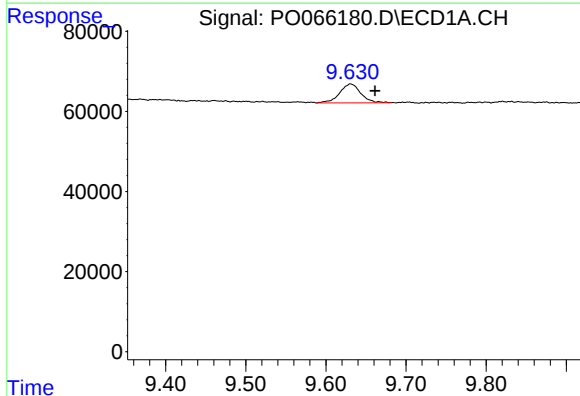

#2 Decachlorobiphenyl

R.T.: 9.630 min
Delta R.T.: -0.031 min
Response: 87204
Conc: 2.21 ng/ml m

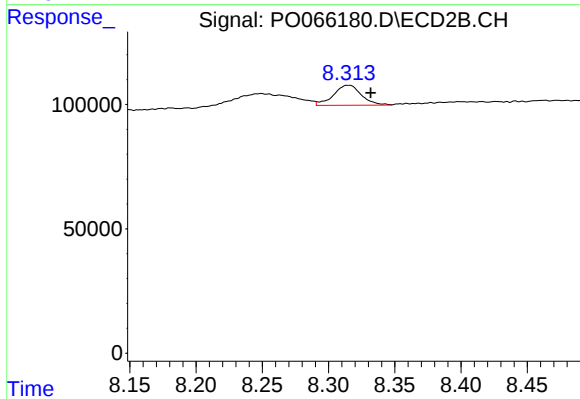

#2 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: -0.019 min
Response: 118499
Conc: 2.02 ng/ml m