

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020119\
 Data File : P0053638.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Feb 2019 13:45
 Operator : SM/SJ
 Sample : K1268-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 012819-SIDI-E-D-M

Manual Integrations
 APPROVED

Sohil
 2/5/2019 12:53:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 21:40:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.100	3.162	27645500	4104151	14.184	17.111
2) SA Decachlor...	9.490	7.771	11554493	3213604	11.855	12.870m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020119\
Data File : PO053638.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Feb 2019 13:45
Operator : SM/SJ
Sample : K1268-06
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
012819-SIDI-E-D-M


Manual Integrations
APPROVED

Sohil
2/5/2019 12:53:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 21:40:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

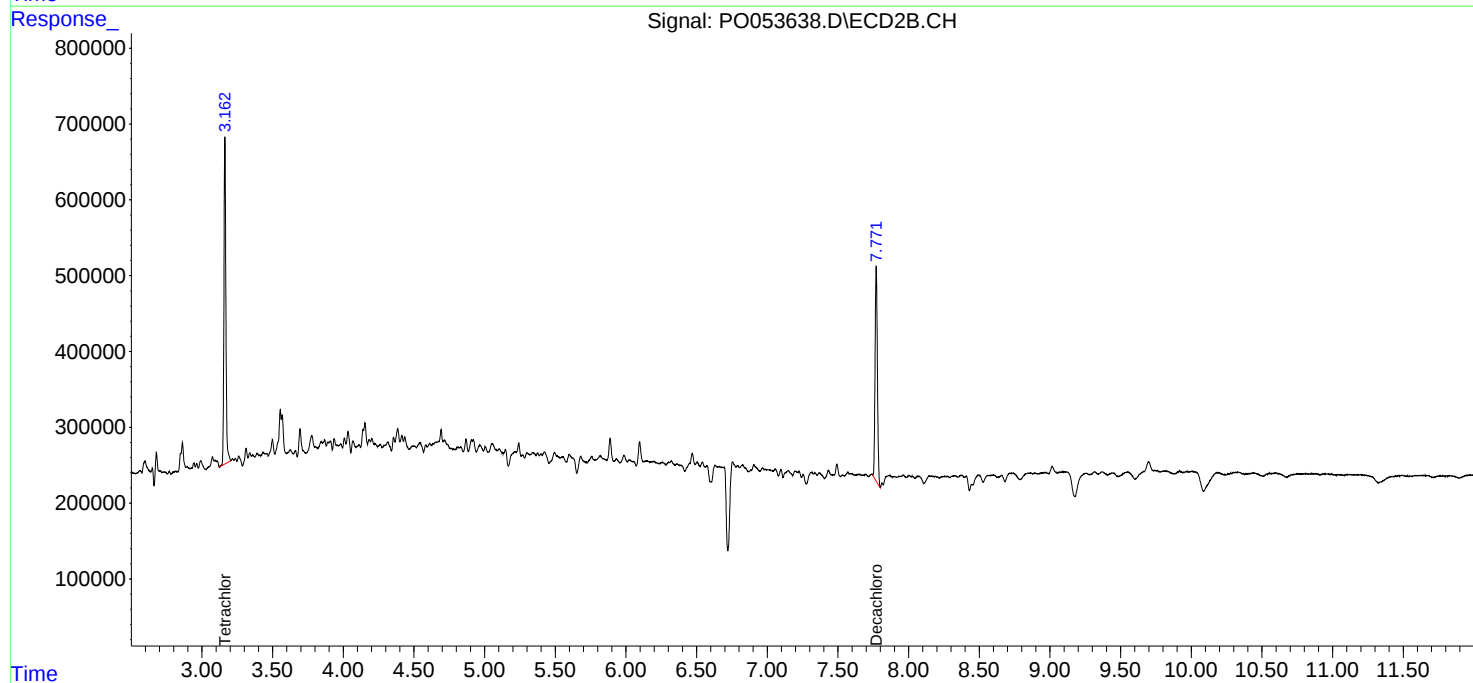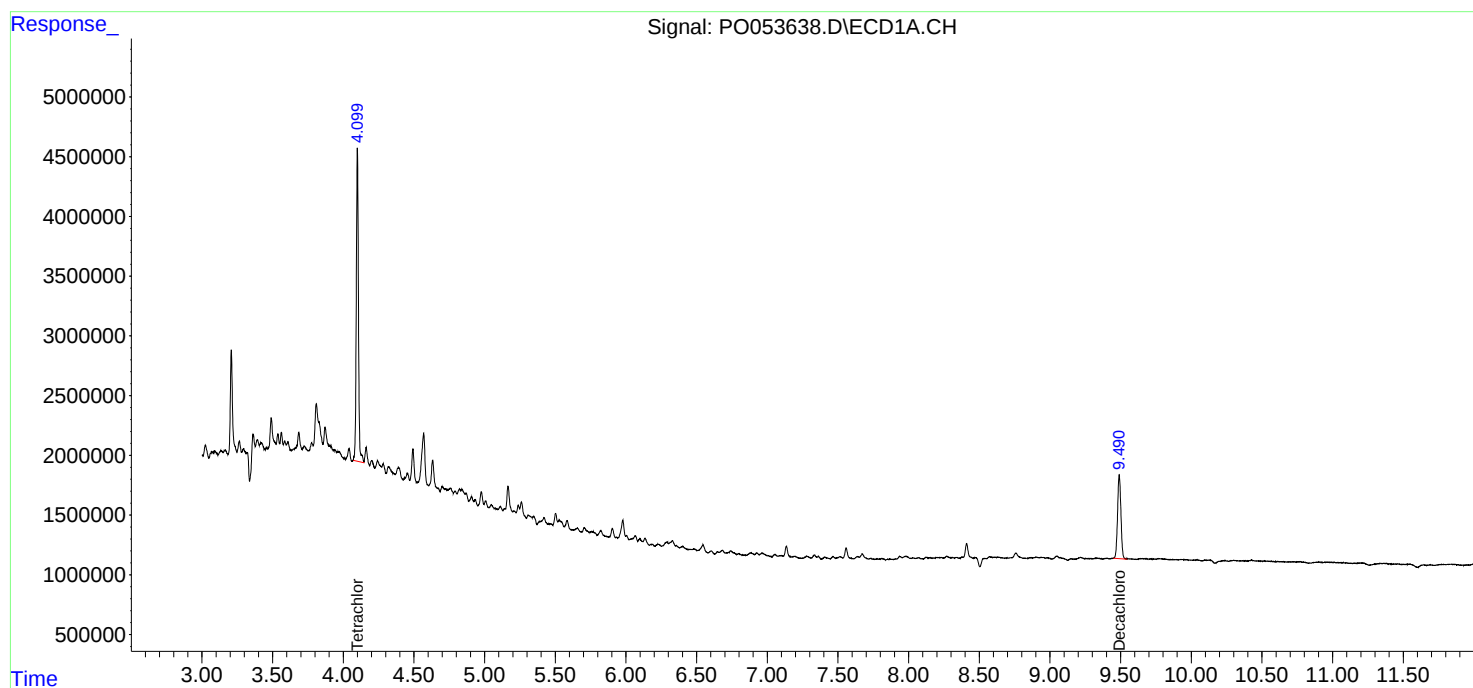

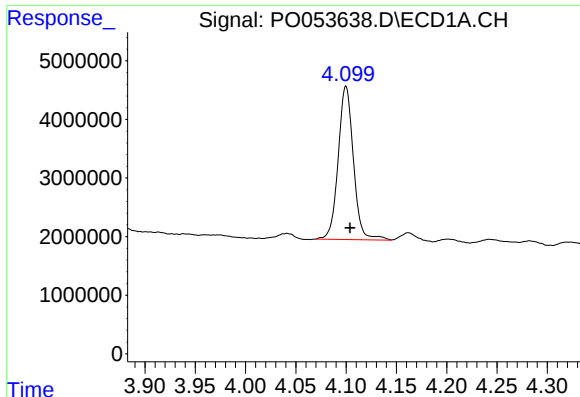


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.004 min
Response: 27645500
Conc: 14.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
012819-SIDI-E-D-M


Manual Integrations
APPROVED

Sohil
2/5/2019 12:53:05 PM

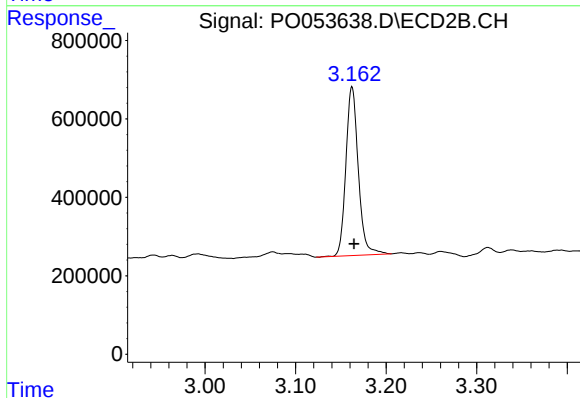


#1 Tetrachloro-m-xylene

R.T.: 3.162 min
Delta R.T.: -0.002 min
Response: 4104151
Conc: 17.11 ng/ml

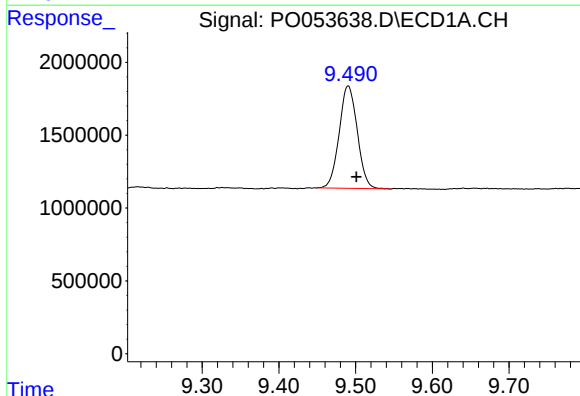

#2 Decachlorobiphenyl

R.T.: 9.490 min
Delta R.T.: -0.011 min
Response: 11554493
Conc: 11.86 ng/ml

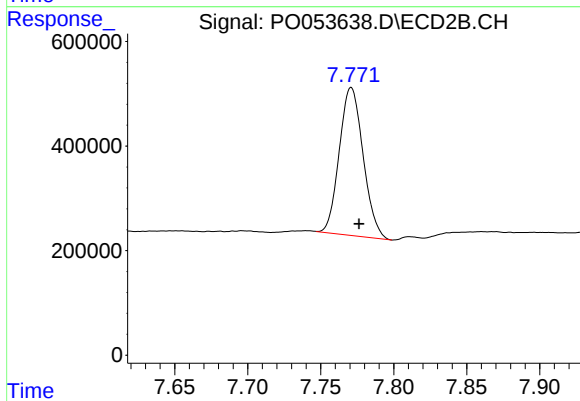

#2 Decachlorobiphenyl

R.T.: 7.771 min
Delta R.T.: -0.006 min
Response: 3213604
Conc: 12.87 ng/ml m