

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020119\
 Data File : P0053658.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Feb 2019 19:26
 Operator : SM/SJ
 Sample : K1307-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 013019-SIDI-E-U-M

Manual Integrations
 APPROVED

Sohil
 2/5/2019 12:53:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 21:44:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.099	3.161	30578117	4087444	15.689	17.042
2) SA Decachlor...	9.488	7.768	13071740	3591838	13.412	14.385m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020119\
Data File : P0053658.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Feb 2019 19:26
Operator : SM/SJ
Sample : K1307-02
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
013019-SIDI-E-U-M


Manual Integrations
APPROVED

Sohil
2/5/2019 12:53:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 21:44:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

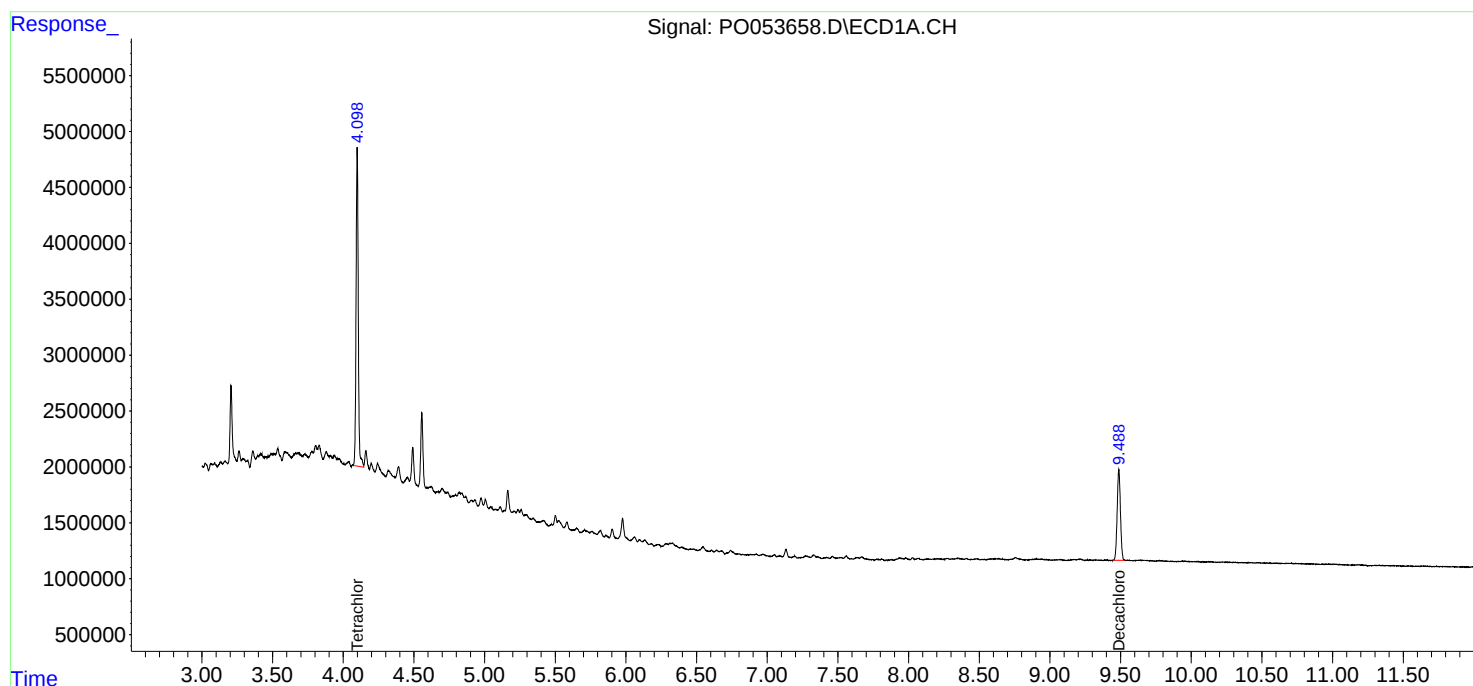

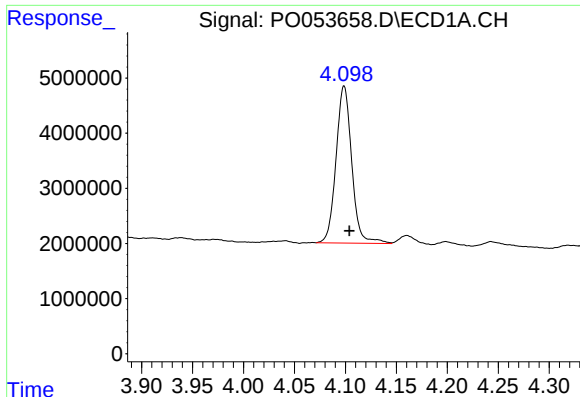


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: -0.005 min
Response: 30578117
Conc: 15.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
013019-SIDI-E-U-M


Manual Integrations
APPROVED

Sohil
2/5/2019 12:53:16 PM

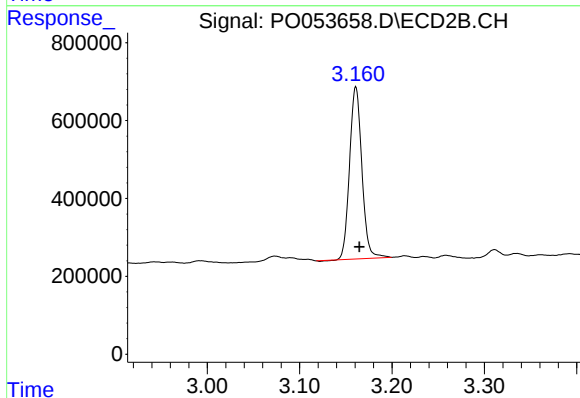


#1 Tetrachloro-m-xylene

R.T.: 3.161 min
Delta R.T.: -0.004 min
Response: 4087444
Conc: 17.04 ng/ml

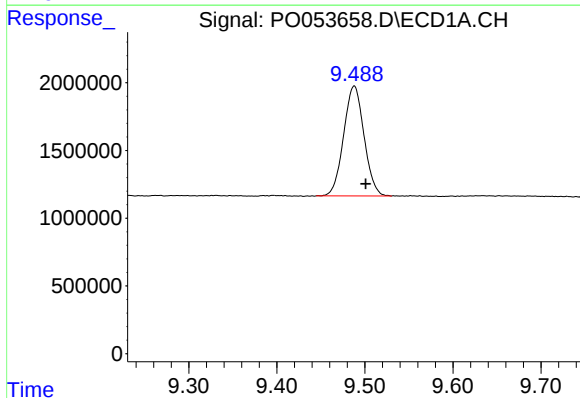

#2 Decachlorobiphenyl

R.T.: 9.488 min
Delta R.T.: -0.013 min
Response: 13071740
Conc: 13.41 ng/ml

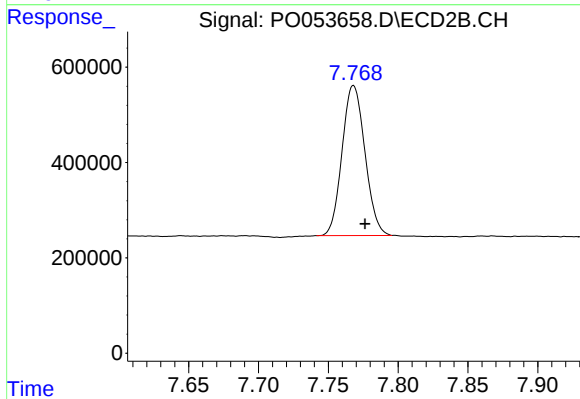

#2 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: -0.009 min
Response: 3591838
Conc: 14.38 ng/ml m