

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020119\
 Data File : P0053662.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Feb 2019 20:33
 Operator : SM/SJ
 Sample : K1307-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 013019-SIDI-E-D-S

Manual Integrations
 APPROVED

Sohil
 2/5/2019 12:53:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 21:45:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.098	3.161	27838268	3951706	14.283m	16.476m
2) SA Decachlor...	9.487	7.768	14306978	3834682	14.679	15.357m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020119\
Data File : PO053662.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Feb 2019 20:33
Operator : SM/SJ
Sample : K1307-06
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
013019-SIDI-E-D-S


Manual Integrations
APPROVED

Sohil
2/5/2019 12:53:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 21:45:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

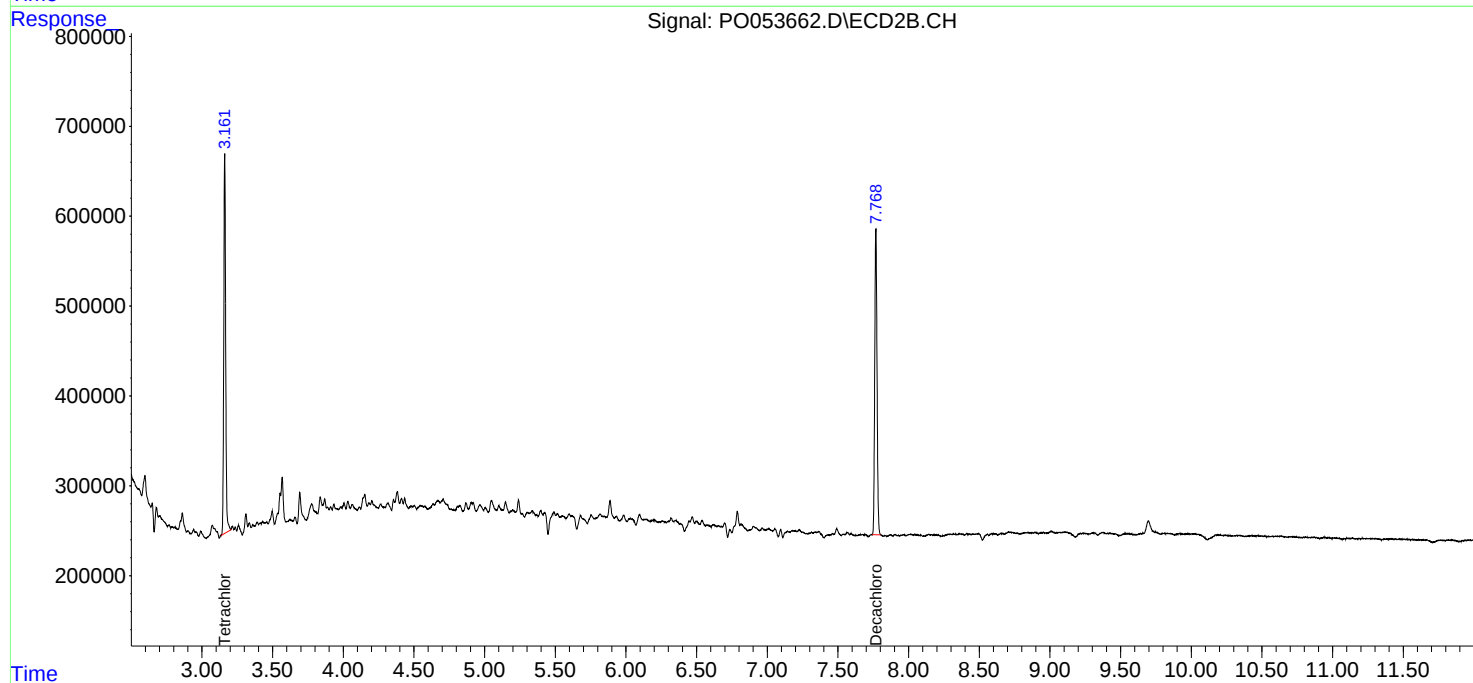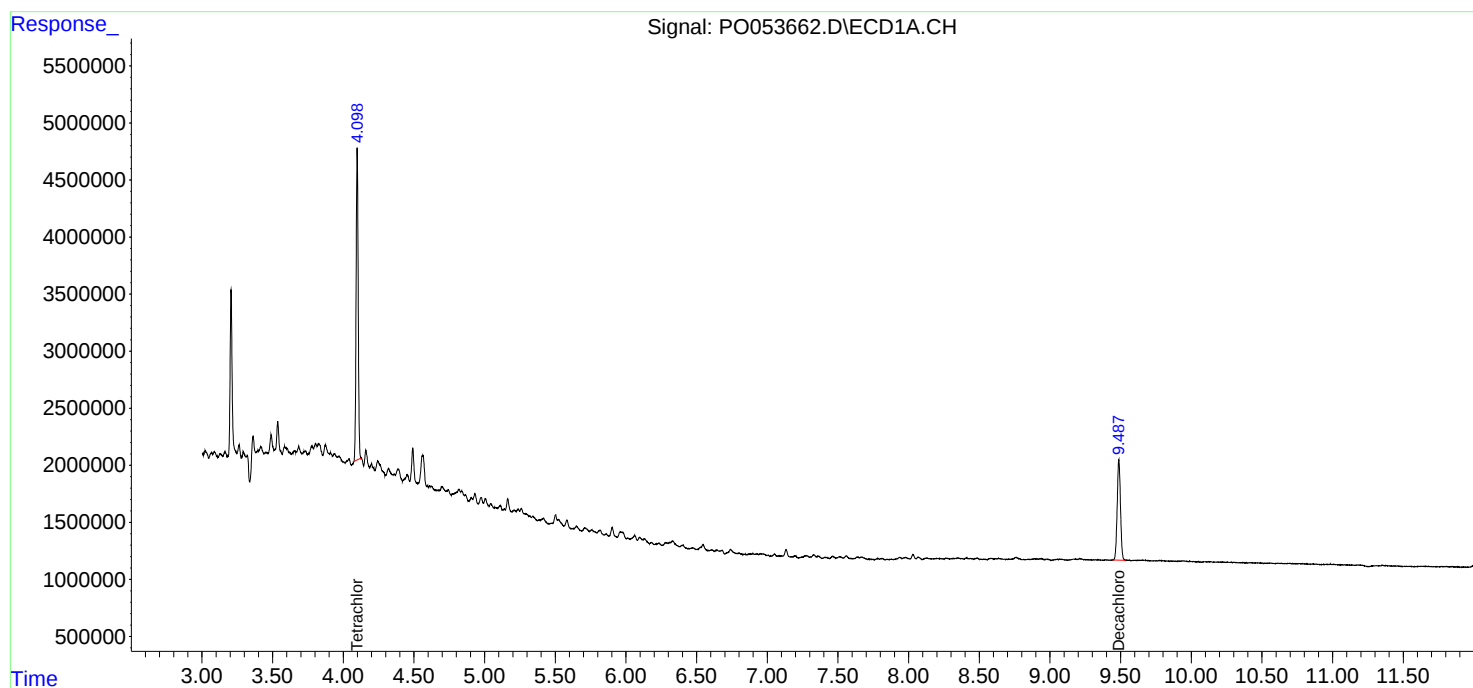

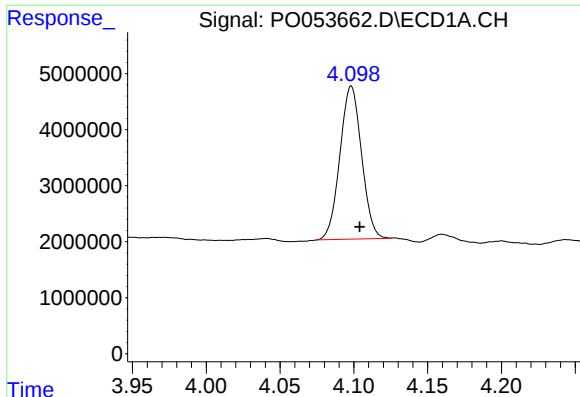


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.006 min
Response: 27838268
Conc: 14.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
013019-SIDI-E-D-S


Manual Integrations
APPROVED

Sohil
2/5/2019 12:53:19 PM

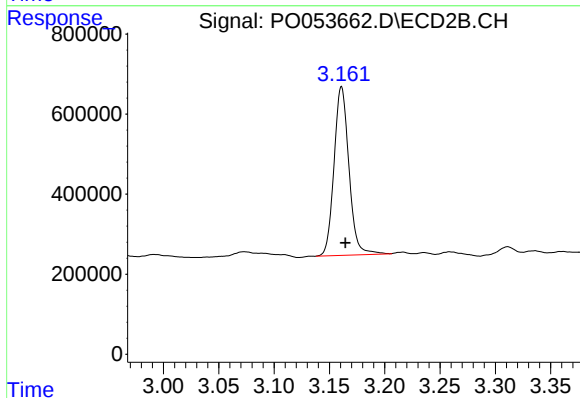


#1 Tetrachloro-m-xylene

R.T.: 3.161 min
Delta R.T.: -0.004 min
Response: 3951706
Conc: 16.48 ng/ml m

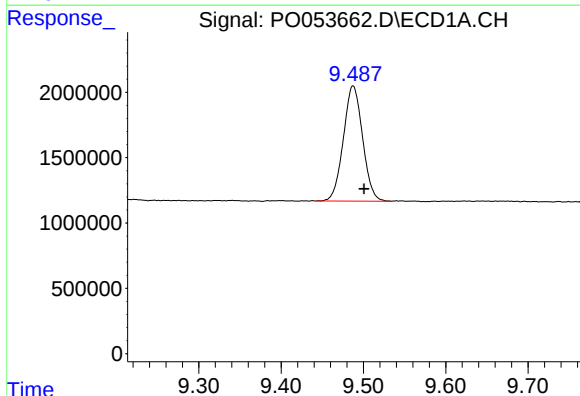

#2 Decachlorobiphenyl

R.T.: 9.487 min
Delta R.T.: -0.014 min
Response: 14306978
Conc: 14.68 ng/ml

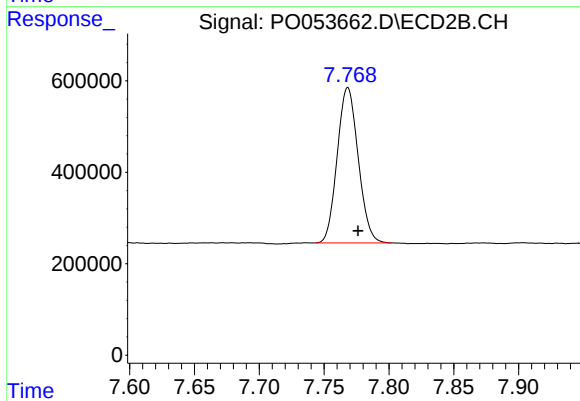

#2 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: -0.008 min
Response: 3834682
Conc: 15.36 ng/ml m