

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020119\
 Data File : P0053668.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Feb 2019 22:15
 Operator : SM/SJ
 Sample : K1299-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SPLP-LEACH-AMND-COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 23:17:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.099	3.162	34058276	4534120	17.474	18.904
2) SA Decachlor...	9.488	7.768	11959585	3455662	12.271	13.839

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020119\
Data File : P0053668.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Feb 2019 22:15
Operator : SM/SJ
Sample : K1299-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SPLP-LEACH-AMND-COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 23:17:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

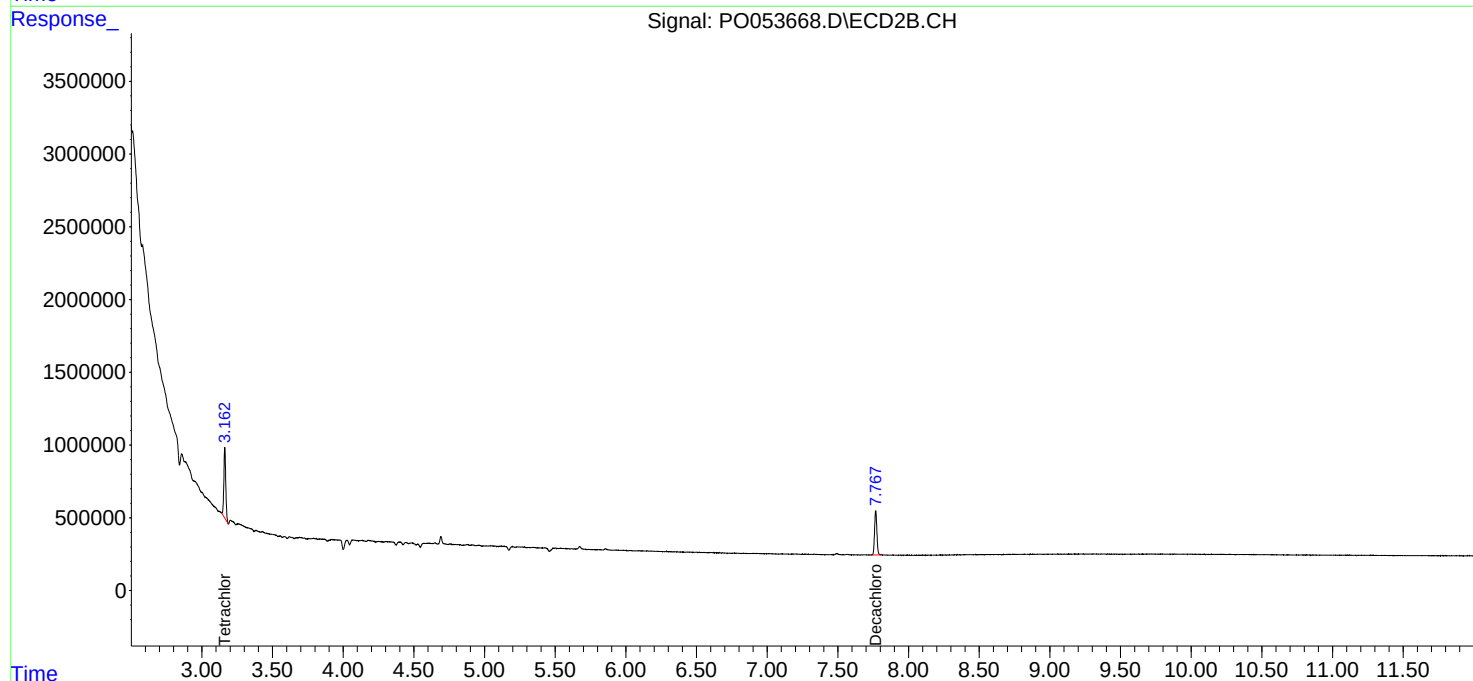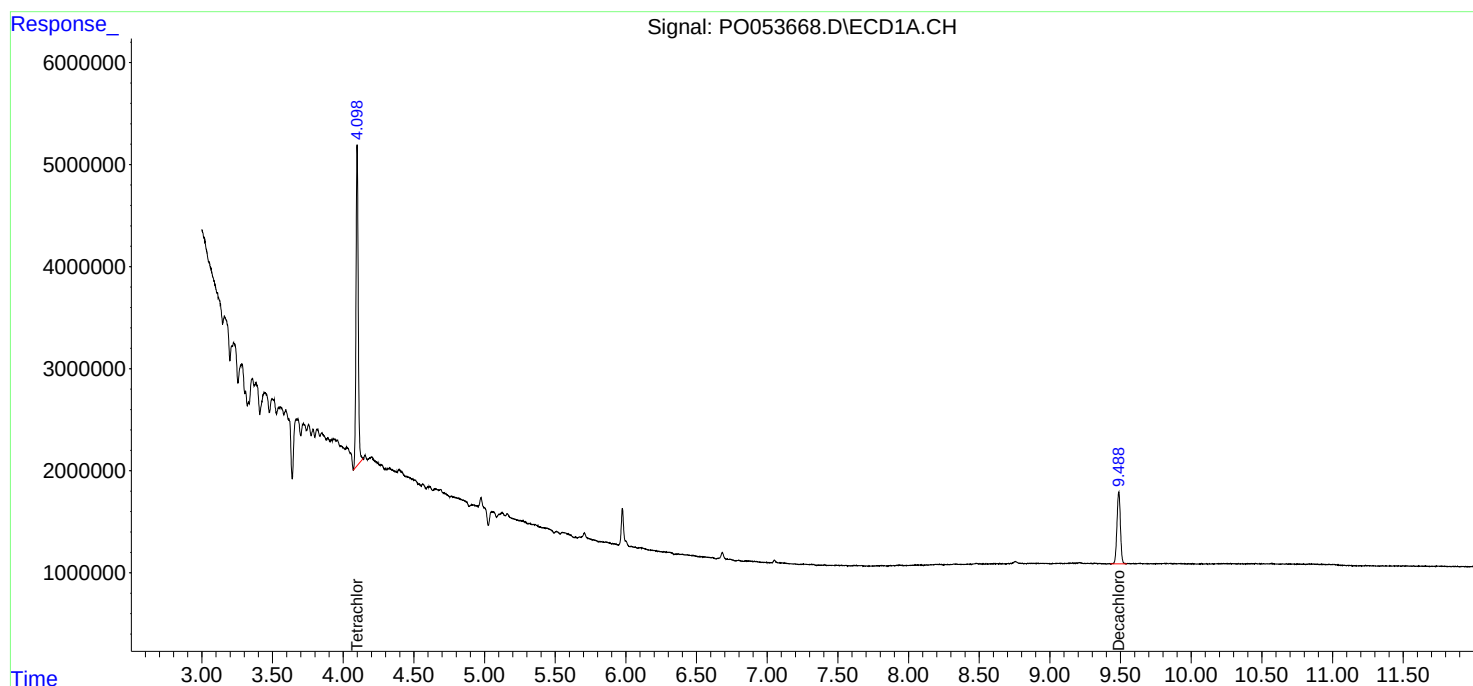


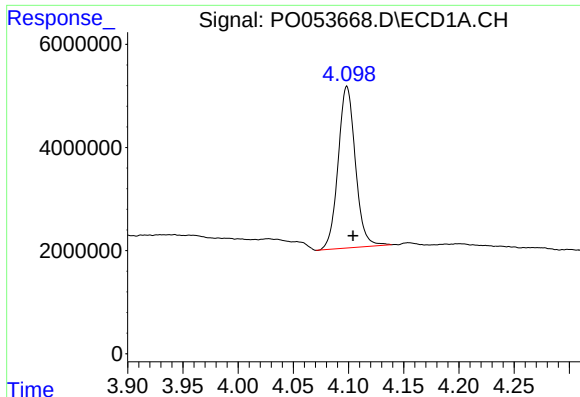

#1 Tetrachloro-m-xylene


R.T.: 4.099 min
Delta R.T.: -0.005 min
Response: 34058276
Conc: 17.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
SPLP-LEACH-AMND-COMP-1

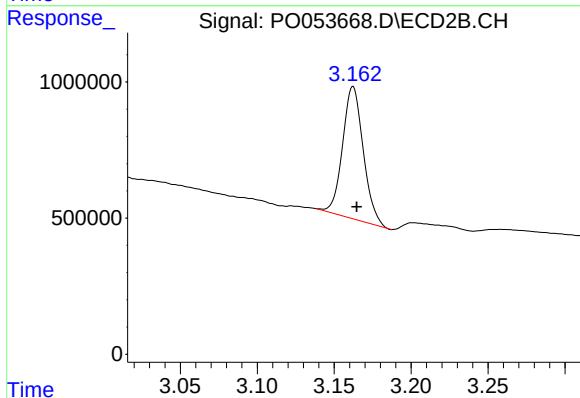


#1 Tetrachloro-m-xylene

R.T.: 3.162 min
Delta R.T.: -0.002 min
Response: 4534120
Conc: 18.90 ng/ml

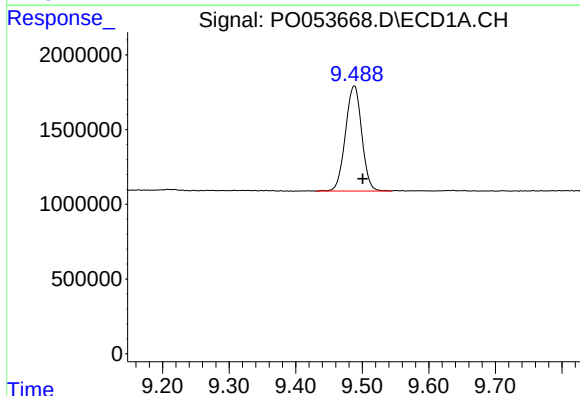

#2 Decachlorobiphenyl

R.T.: 9.488 min
Delta R.T.: -0.013 min
Response: 11959585
Conc: 12.27 ng/ml

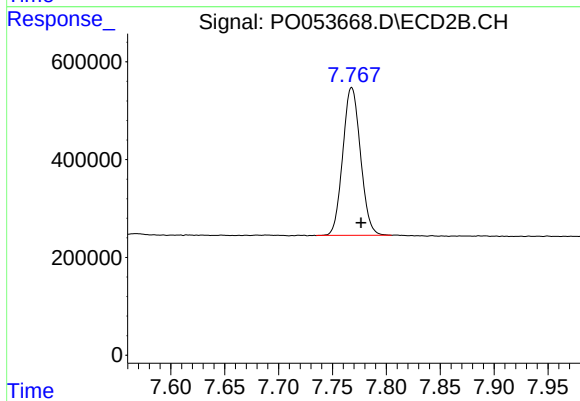

#2 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: -0.008 min
Response: 3455662
Conc: 13.84 ng/ml