

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020119\
 Data File : P0053675.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Feb 2019 00:13
 Operator : SM/SJ
 Sample : K1303-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 131-A-E

Manual Integrations
 APPROVED

Sohil
 2/5/2019 12:54:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 01:24:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.098	3.161	31500988	4161981	16.162	17.352
2) SA Decachlor...	9.484	7.767	15252500	4092512	15.650	16.390m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020119\
Data File : PO053675.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Feb 2019 00:13
Operator : SM/SJ
Sample : K1303-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
131-A-E


Manual Integrations
APPROVED

Sohil
2/5/2019 12:54:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 01:24:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

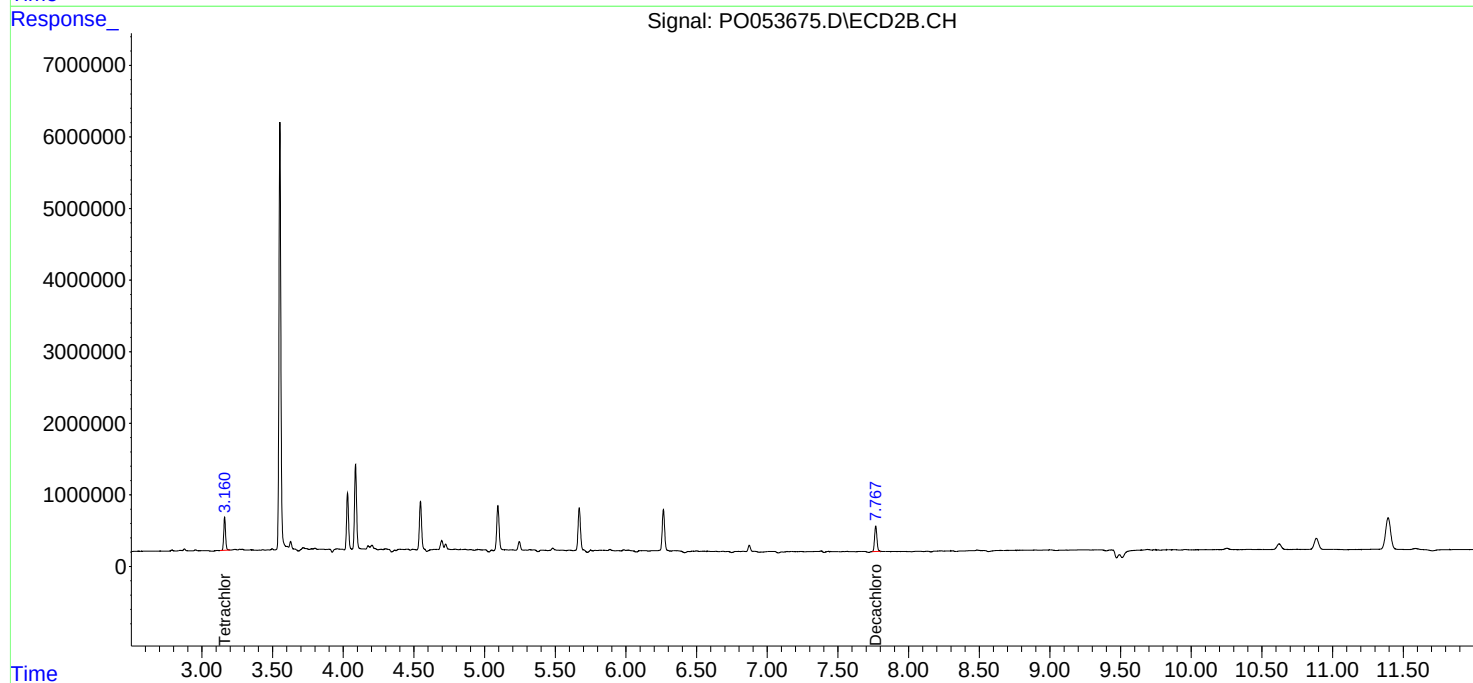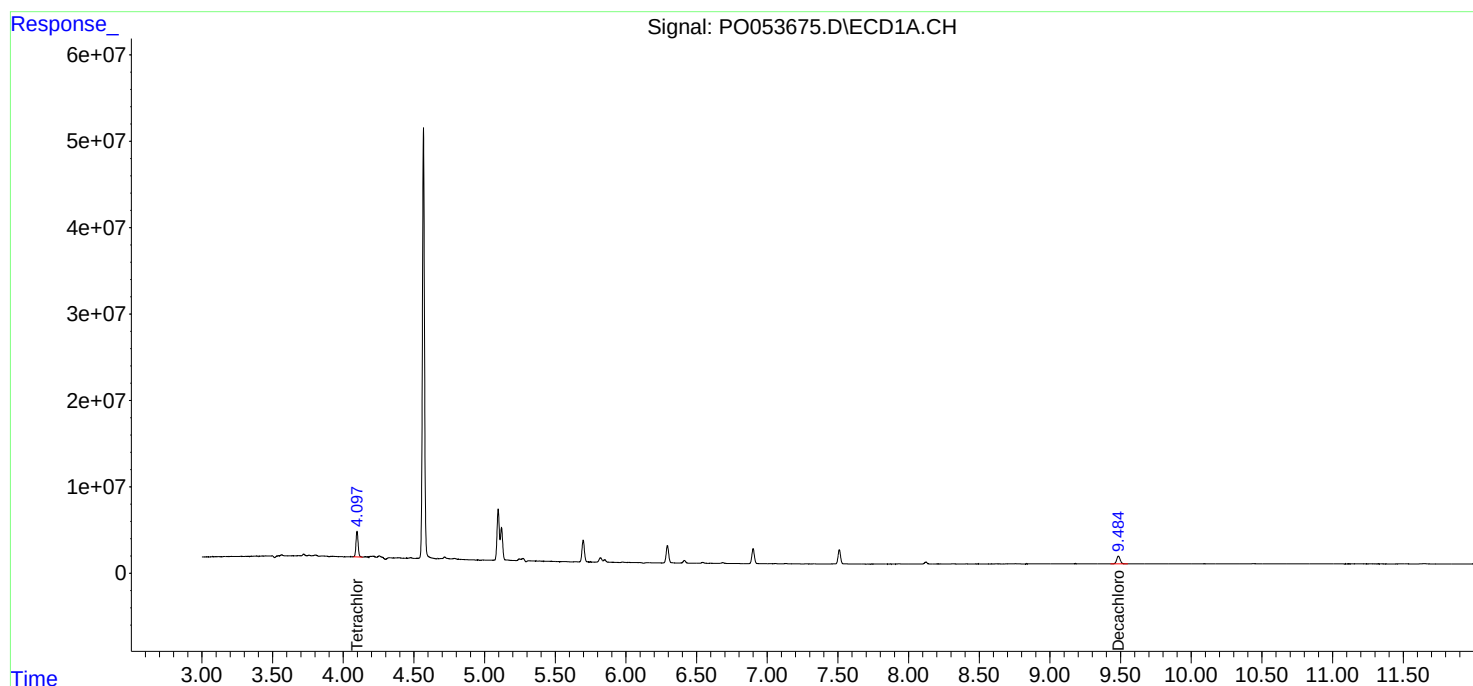

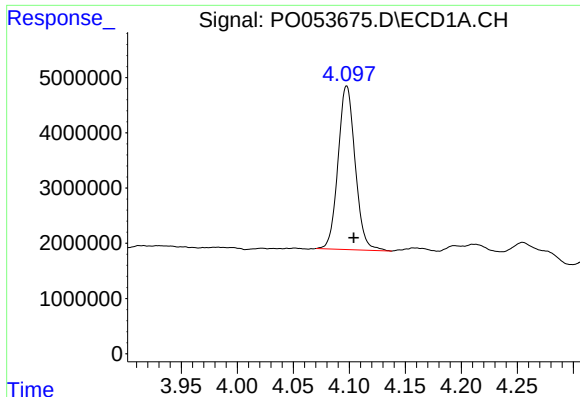


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.006 min
Response: 31500988
Conc: 16.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
131-A-E


Manual Integrations
APPROVED

Sohil
2/5/2019 12:54:10 PM

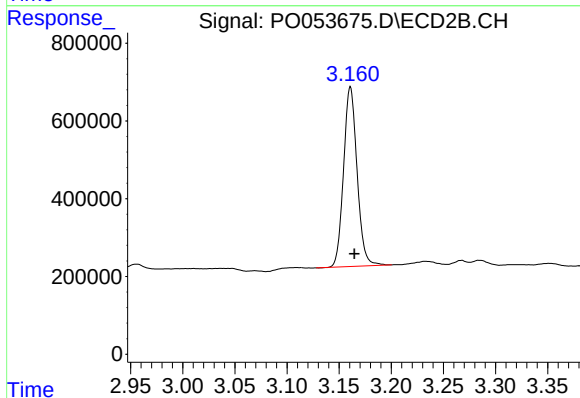


#1 Tetrachloro-m-xylene

R.T.: 3.161 min
Delta R.T.: -0.004 min
Response: 4161981
Conc: 17.35 ng/ml

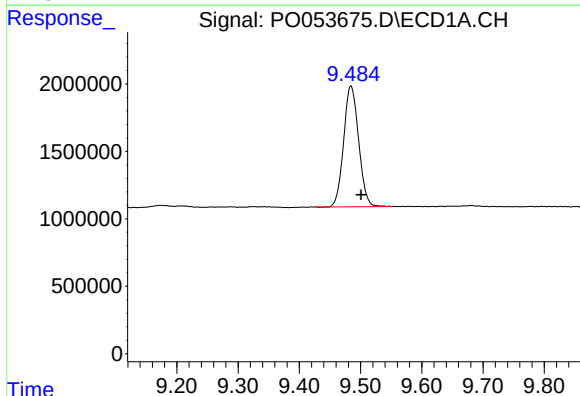

#2 Decachlorobiphenyl

R.T.: 9.484 min
Delta R.T.: -0.017 min
Response: 15252500
Conc: 15.65 ng/ml

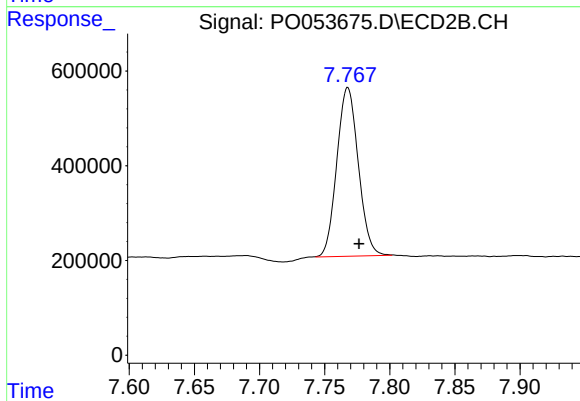

#2 Decachlorobiphenyl

R.T.: 7.767 min
Delta R.T.: -0.009 min
Response: 4092512
Conc: 16.39 ng/ml m