

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020121\
 Data File : P0075384.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Feb 2021 13:09
 Operator : AJ/MA
 Sample : M1246-05DL 100X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 250EM-007-0002DL

Manual Integrations
 APPROVED

Ankita
 2/2/2021 1:19:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 13:28:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.922	3.995	18169	12904	0.180	0.268m#
2) SA Decachlor...	10.939	9.245	806011	451217	8.354	9.295
Target Compounds						
36) L8 AR-1262-1	8.573	7.342	3896226	56978	446.483	26.122 #
37) L8 AR-1262-2	9.131	7.889	4433690	2126842	293.195	277.330
38) L8 AR-1262-3	9.441	8.173	9243718	4262245	884.834	1287.950 #
39) L8 AR-1262-4	9.536	8.239	9217935	4519332	1247.161	787.090 #
40) L8 AR-1262-5	10.198	8.731	5968938	2835012	1150.992	1030.594

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020121\
Data File : PO075384.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Feb 2021 13:09
Operator : AJ/MA
Sample : M1246-05DL 100X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
250EM-007-0002DL


Manual Integrations
APPROVED

Ankita
2/2/2021 1:19:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 13:28:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

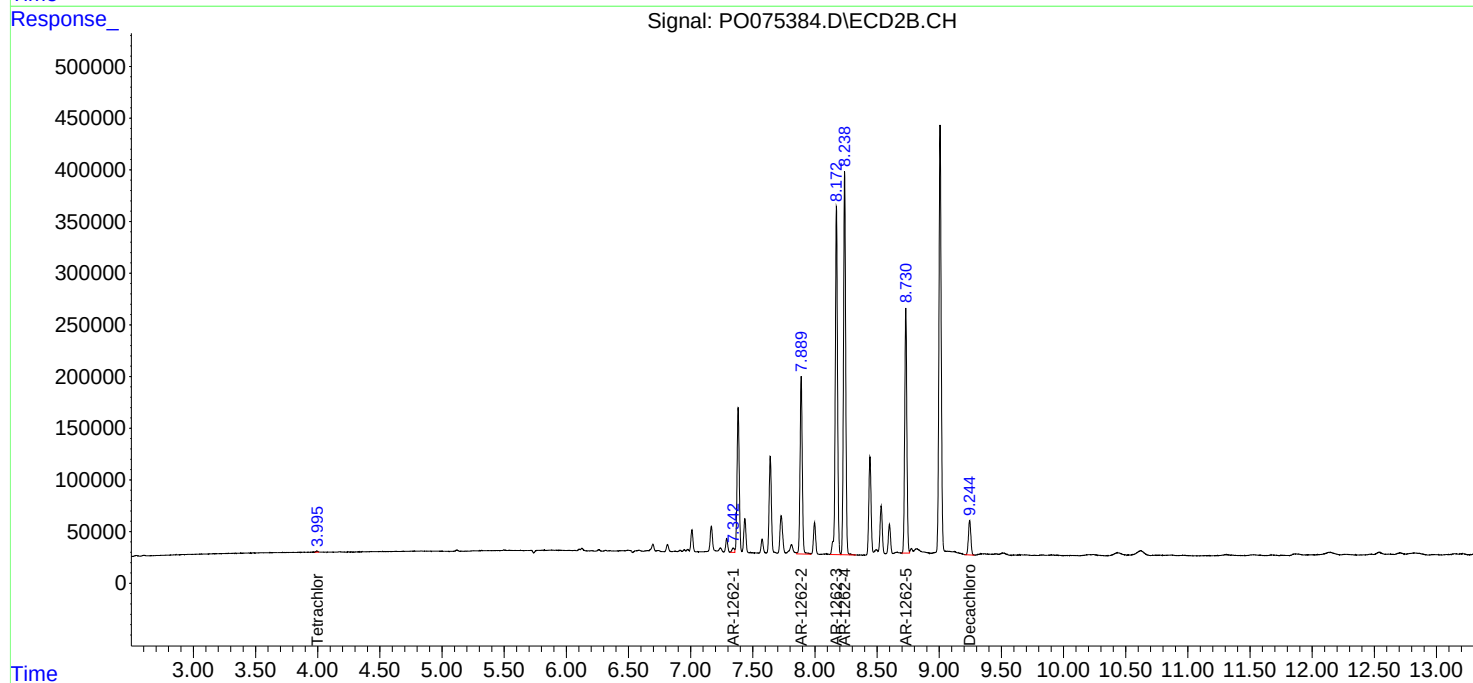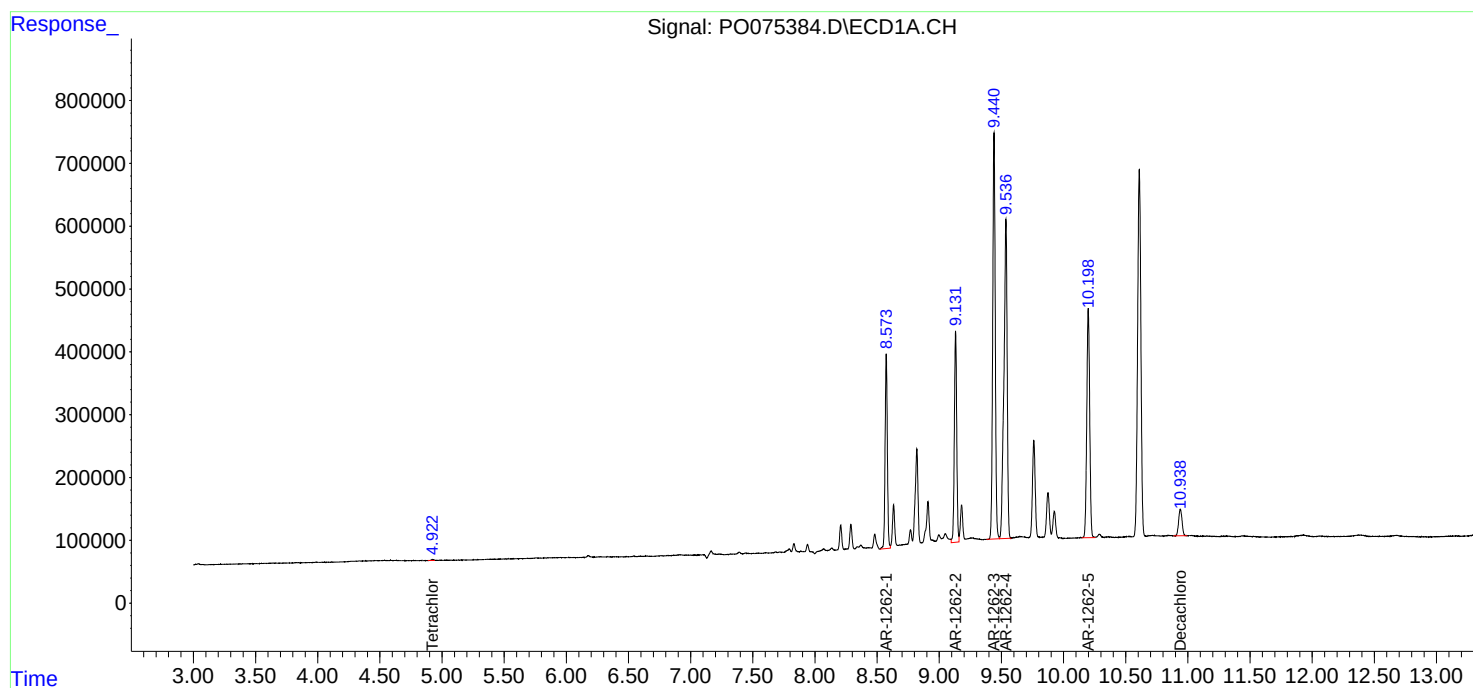

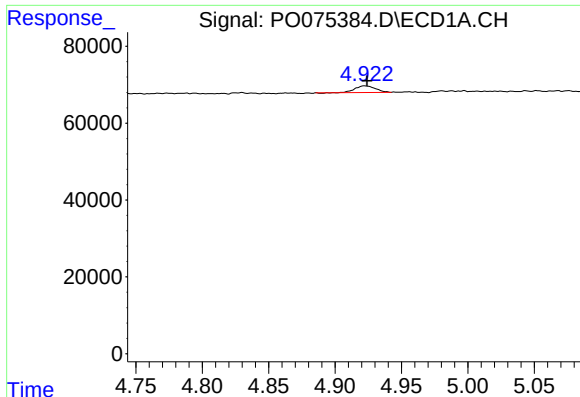


#1 Tetrachloro-m-xylene

R.T.: 4.922 min
Delta R.T.: -0.002 min
Response: 18169
Conc: 0.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-007-0002DL


Manual Integrations
APPROVED

Ankita
2/2/2021 1:19:02 PM

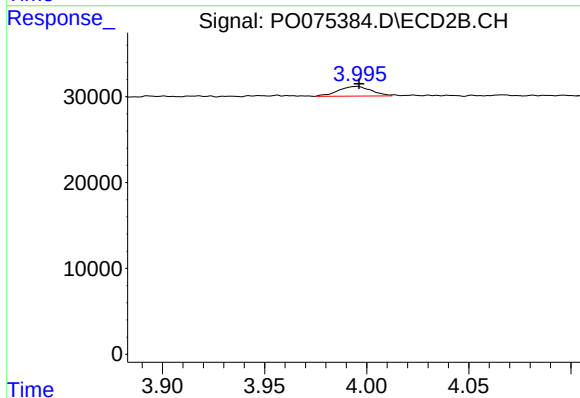


#1 Tetrachloro-m-xylene

R.T.: 3.995 min
Delta R.T.: 0.000 min
Response: 12904
Conc: 0.27 ng/ml m

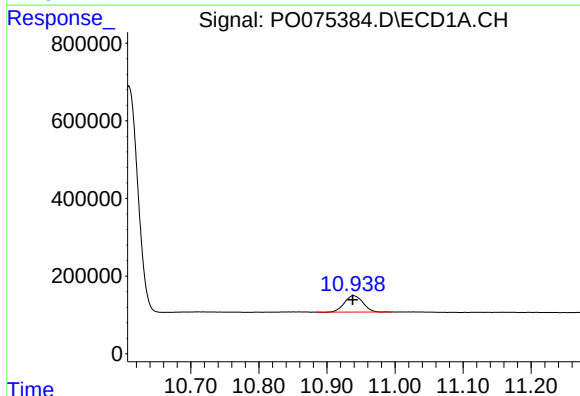


#2 Decachlorobiphenyl

R.T.: 10.939 min
Delta R.T.: 0.001 min
Response: 806011
Conc: 8.35 ng/ml

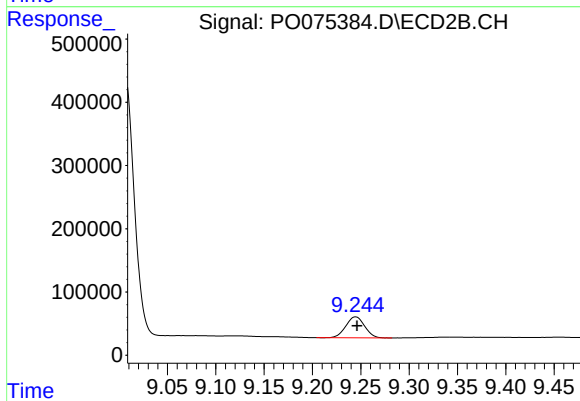

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.002 min
Response: 451217
Conc: 9.30 ng/ml

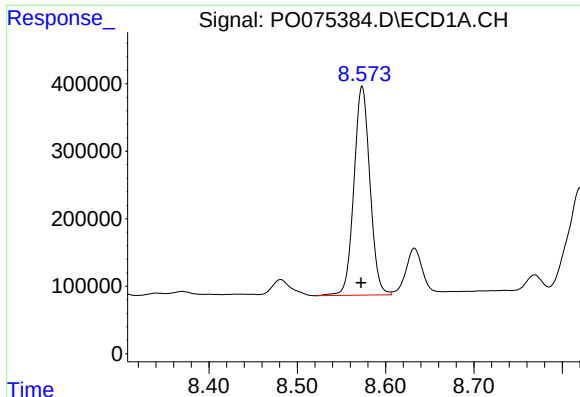


#36 AR-1262-1

R.T.: 8.573 min
Delta R.T.: 0.001 min
Response: 3896226
Conc: 446.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-007-0002DL


Manual Integrations
APPROVED

Ankita
2/2/2021 1:19:02 PM

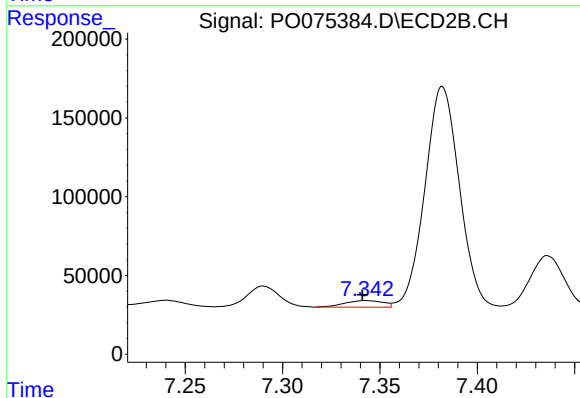


#36 AR-1262-1

R.T.: 7.342 min
Delta R.T.: 0.001 min
Response: 56978
Conc: 26.12 ng/ml

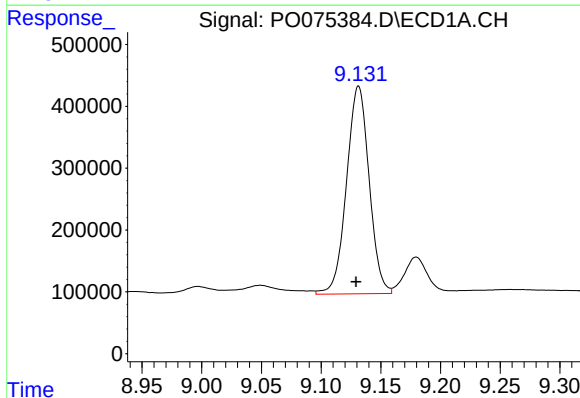


#37 AR-1262-2

R.T.: 9.131 min
Delta R.T.: 0.002 min
Response: 4433690
Conc: 293.20 ng/ml

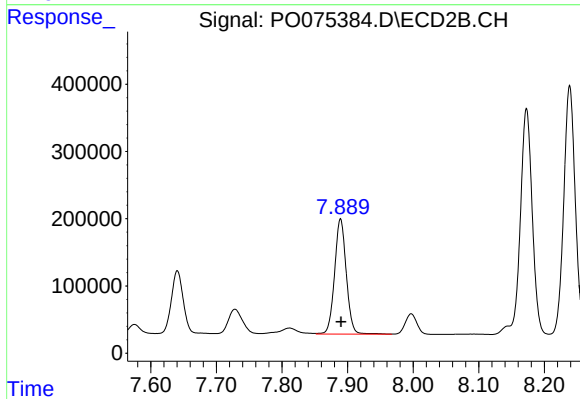

#37 AR-1262-2

R.T.: 7.889 min
Delta R.T.: 0.000 min
Response: 2126842
Conc: 277.33 ng/ml

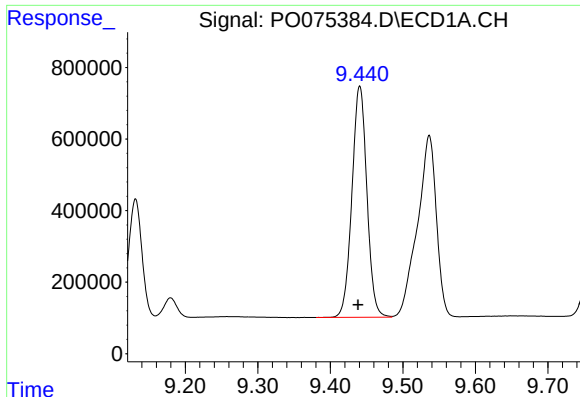


#38 AR-1262-3

R.T.: 9.441 min
Delta R.T.: 0.002 min
Response: 9243718
Conc: 884.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-007-0002DL


Manual Integrations
APPROVED

Ankita
2/2/2021 1:19:02 PM

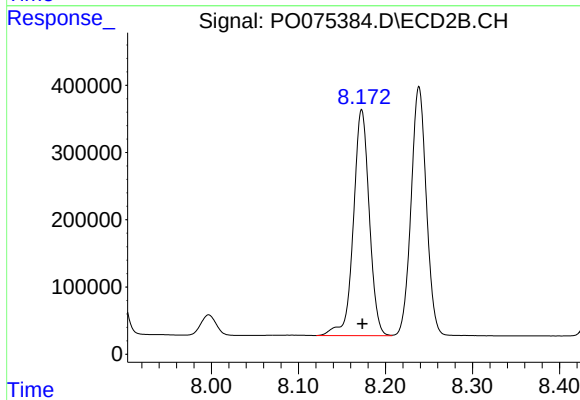


#38 AR-1262-3

R.T.: 8.173 min
Delta R.T.: 0.000 min
Response: 4262245
Conc: 1287.95 ng/ml

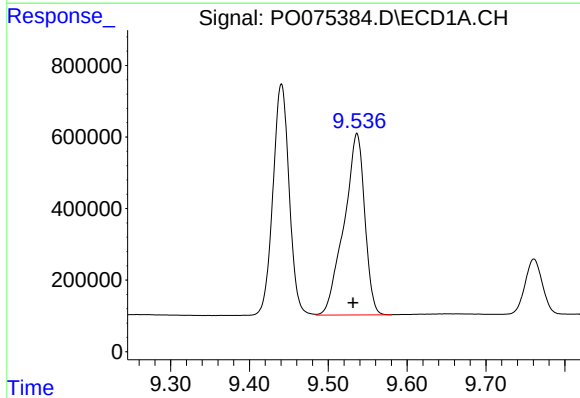


#39 AR-1262-4

R.T.: 9.536 min
Delta R.T.: 0.005 min
Response: 9217935
Conc: 1247.16 ng/ml

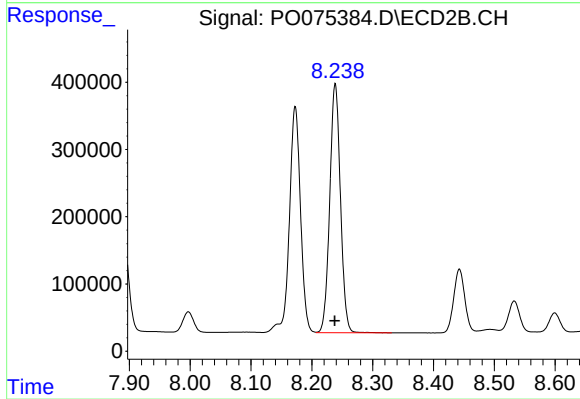

#39 AR-1262-4

R.T.: 8.239 min
Delta R.T.: 0.001 min
Response: 4519332
Conc: 787.09 ng/ml

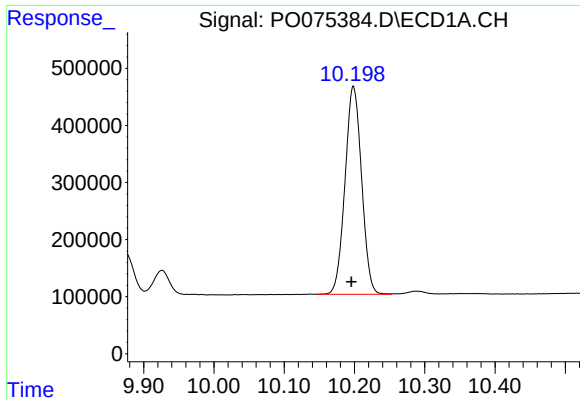


#40 AR-1262-5

R.T.: 10.198 min
Delta R.T.: 0.003 min
Response: 5968938
Conc: 1150.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-007-0002DL

Manual Integrations
APPROVED

Ankita
2/2/2021 1:19:02 PM

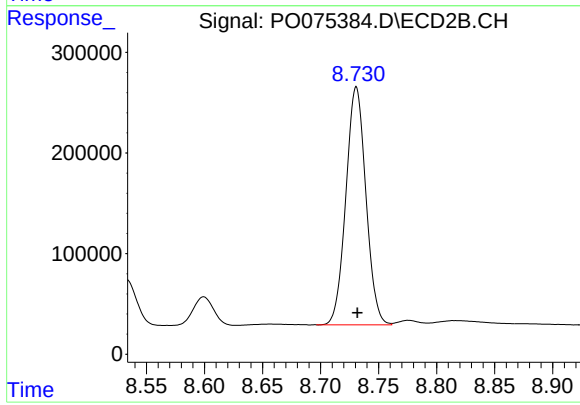

#40 AR-1262-5

R.T.: 8.731 min
Delta R.T.: 0.000 min
Response: 2835012
Conc: 1030.59 ng/ml