

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020121\
 Data File : P0075398.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Feb 2021 17:25
 Operator : AJ/MA
 Sample : M1297-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LLEXSITUTV-025-001-SO

Manual Integrations
 APPROVED

Ankita
 2/2/2021 1:19:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 00:30:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 29 09:09:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.923	3.994	2105274	1033428	20.803	21.498
2) SA Decachlor...	10.940	9.245	2141226	1082639	22.193	22.303
Target Compounds						
26) L6 AR-1254-1	7.160	6.102	673507	390862	156.271	126.199
27) L6 AR-1254-2	7.390	6.262	916373	357796	135.917m	133.240
28) L6 AR-1254-3	7.774	6.678	1049596	603838	152.201	141.613
29) L6 AR-1254-4	8.071	6.916	821968	352842	135.963	121.056
30) L6 AR-1254-5	8.500	7.341	881497	609024	157.695	156.919

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020121\
Data File : PO075398.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Feb 2021 17:25
Operator : AJ/MA
Sample : M1297-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LLEXSITUTV-025-001-SO


Manual Integrations
APPROVED

Ankita
2/2/2021 1:19:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 00:30:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012821.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 29 09:09:46 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

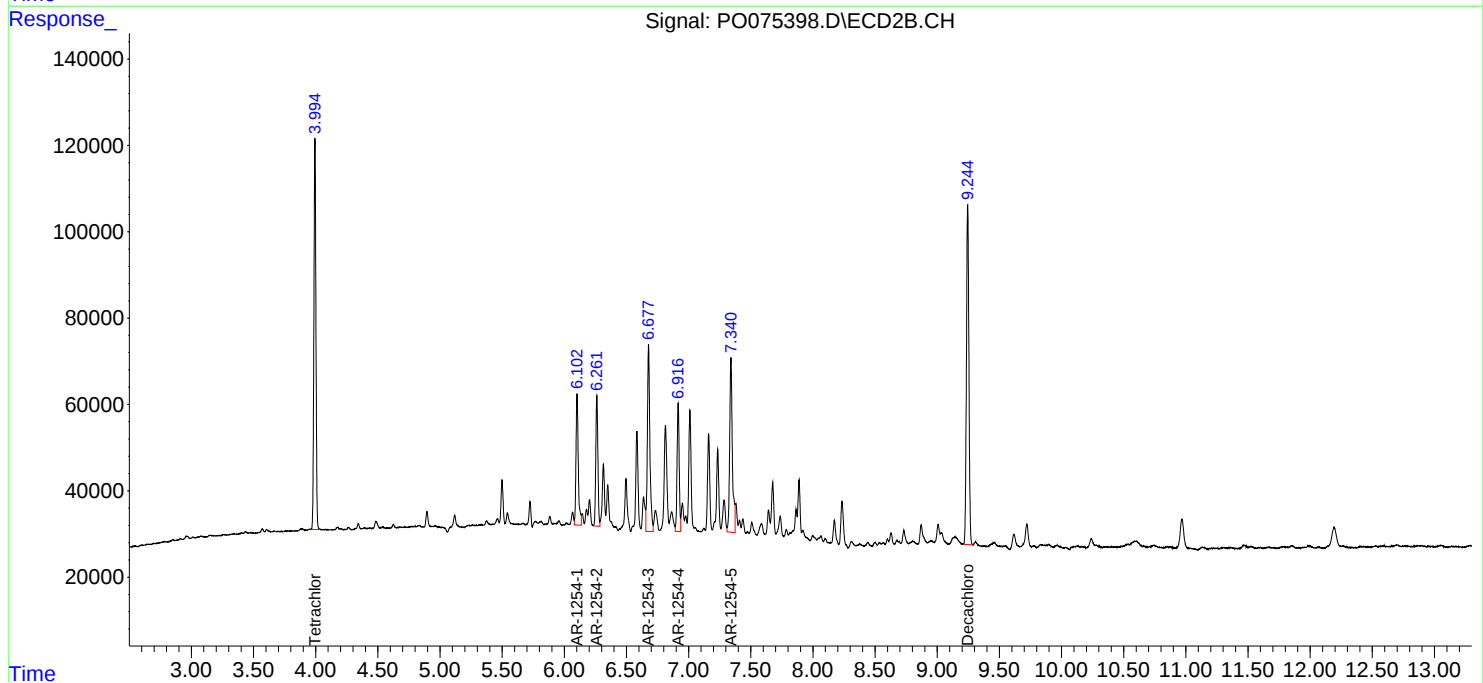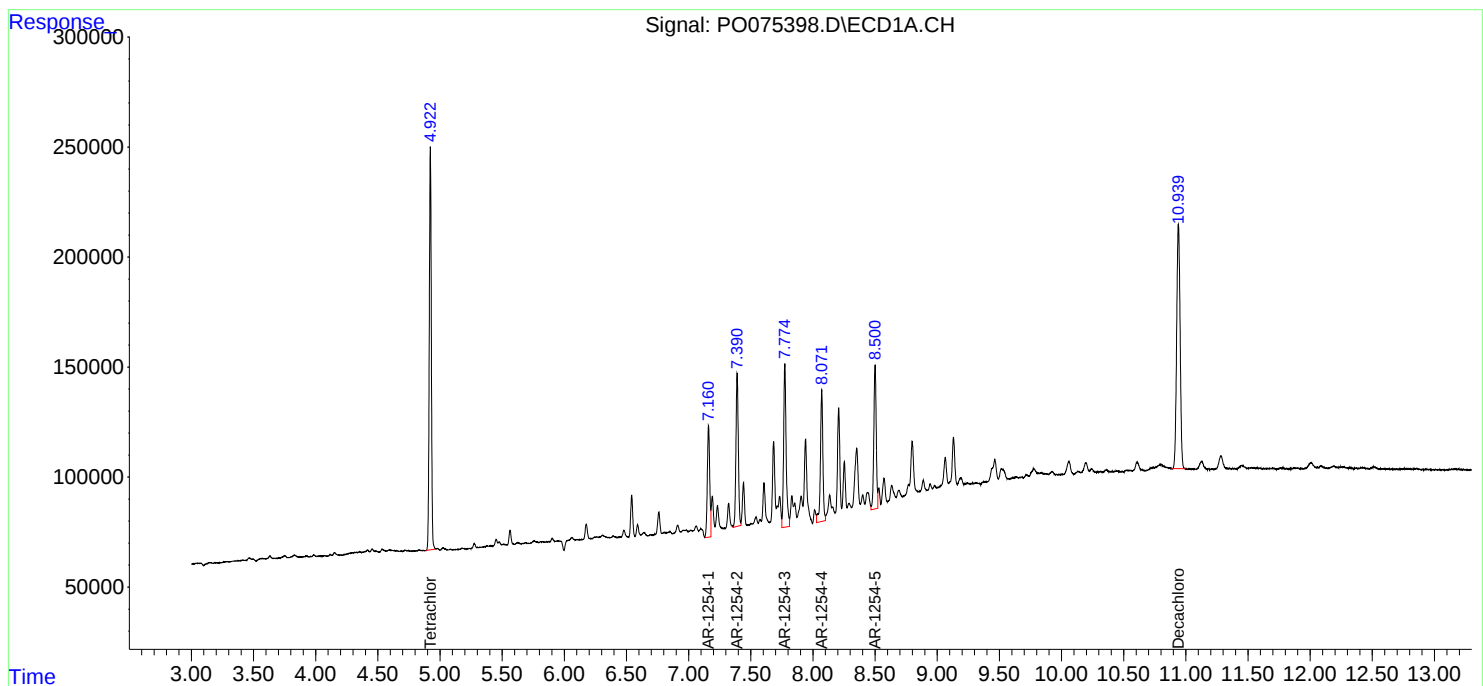

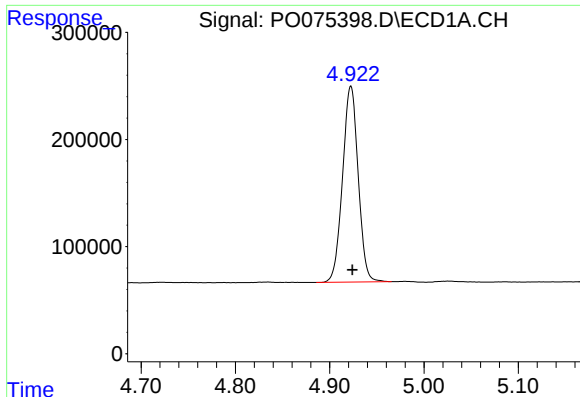


#1 Tetrachloro-m-xylene

R.T.: 4.923 min
Delta R.T.: -0.001 min
Response: 2105274
Conc: 20.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LLEXSITUTV-025-001-SO


Manual Integrations
APPROVED

Ankita
2/2/2021 1:19:28 PM

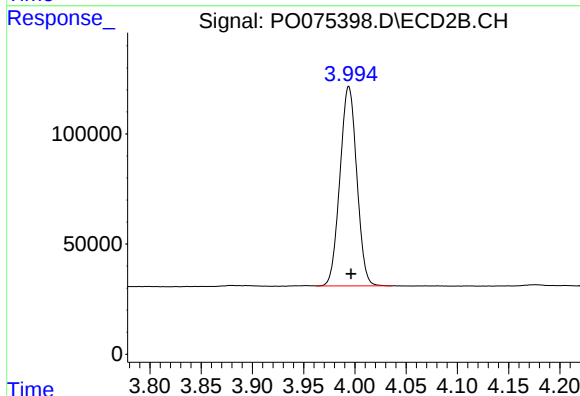


#1 Tetrachloro-m-xylene

R.T.: 3.994 min
Delta R.T.: -0.002 min
Response: 1033428
Conc: 21.50 ng/ml

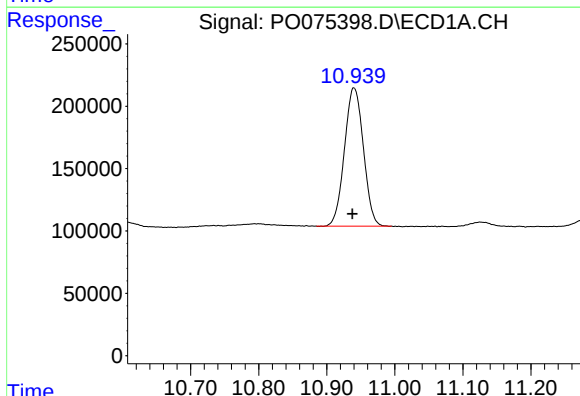


#2 Decachlorobiphenyl

R.T.: 10.940 min
Delta R.T.: 0.002 min
Response: 2141226
Conc: 22.19 ng/ml

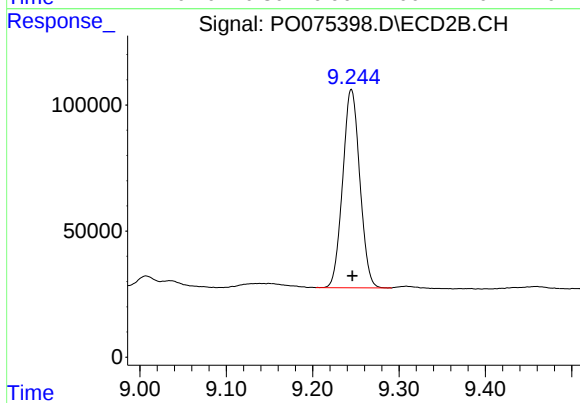

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.001 min
Response: 1082639
Conc: 22.30 ng/ml

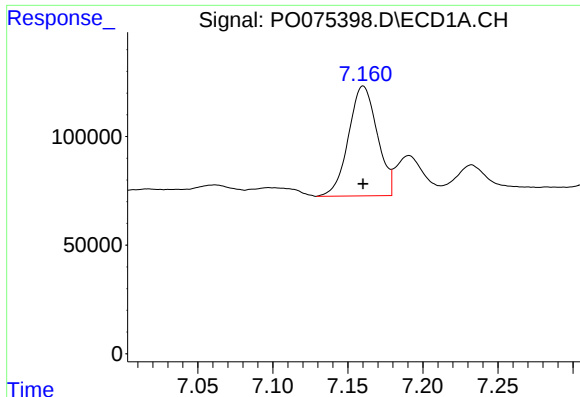


#26 AR-1254-1

R.T.: 7.160 min
Delta R.T.: 0.000 min
Response: 673507
Conc: 156.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
LLEXSITUTV-025-001-SO


Manual Integrations
APPROVED

Ankita
2/2/2021 1:19:28 PM

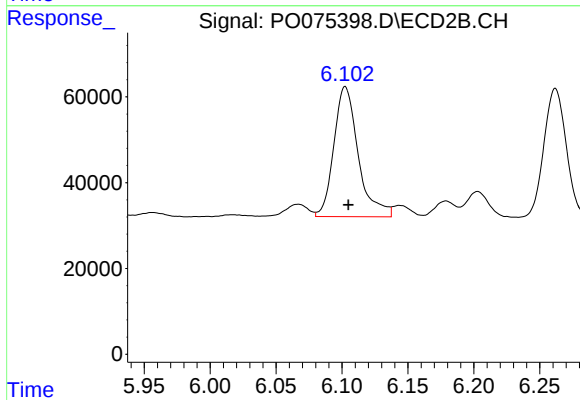


#26 AR-1254-1

R.T.: 6.102 min
Delta R.T.: -0.002 min
Response: 390862
Conc: 126.20 ng/ml

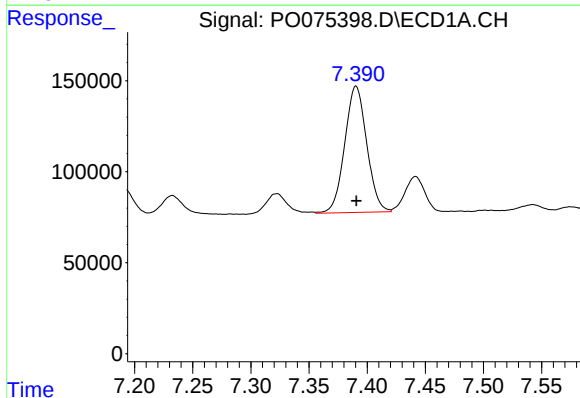


#27 AR-1254-2

R.T.: 7.390 min
Delta R.T.: 0.000 min
Response: 916373
Conc: 135.92 ng/ml m

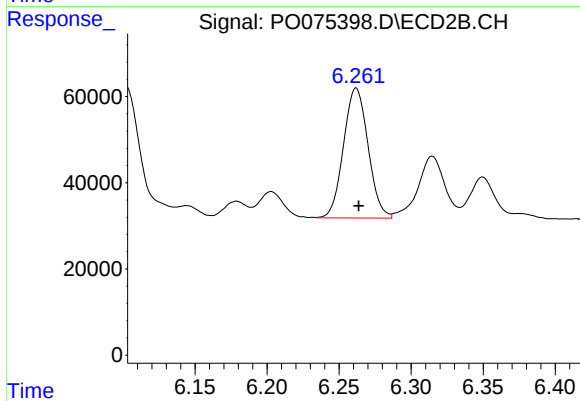

#27 AR-1254-2

R.T.: 6.262 min
Delta R.T.: -0.002 min
Response: 357796
Conc: 133.24 ng/ml

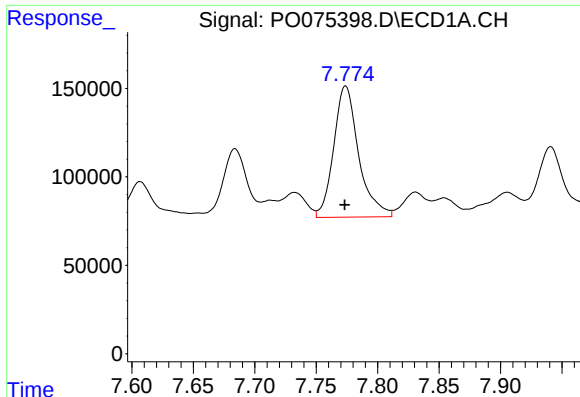


#28 AR-1254-3

R.T.: 7.774 min
Delta R.T.: 0.000 min
Response: 1049596
Conc: 152.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LLEXSITUTV-025-001-SO


Manual Integrations
APPROVED

Ankita
2/2/2021 1:19:28 PM

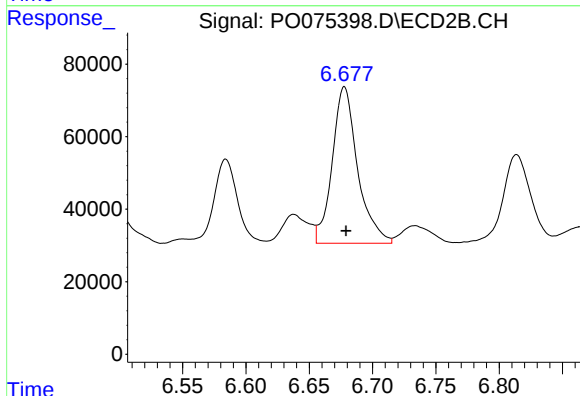


#28 AR-1254-3

R.T.: 6.678 min
Delta R.T.: -0.001 min
Response: 603838
Conc: 141.61 ng/ml

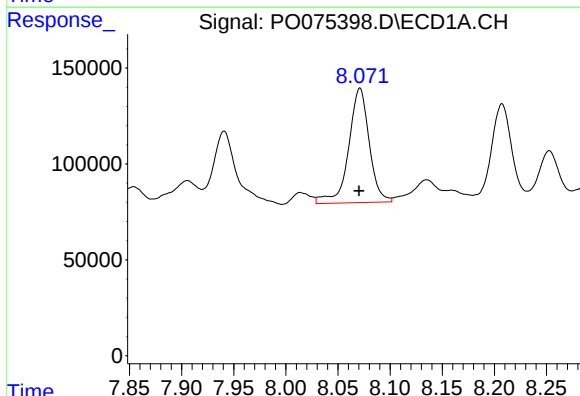


#29 AR-1254-4

R.T.: 8.071 min
Delta R.T.: 0.000 min
Response: 821968
Conc: 135.96 ng/ml

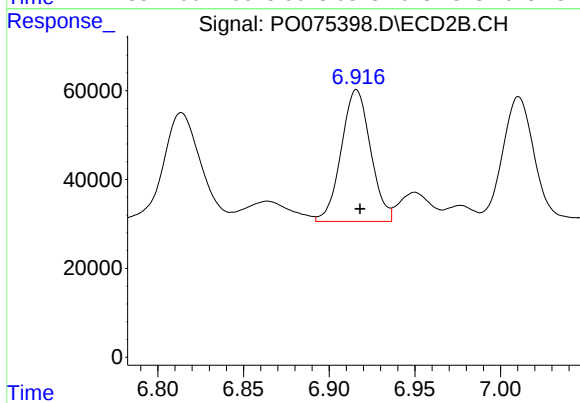

#29 AR-1254-4

R.T.: 6.916 min
Delta R.T.: -0.002 min
Response: 352842
Conc: 121.06 ng/ml

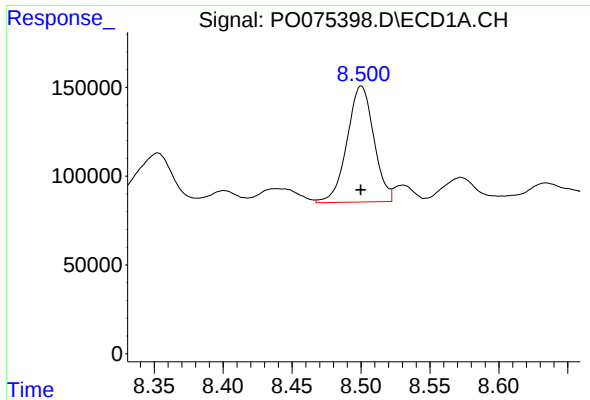


#30 AR-1254-5

R.T.: 8.500 min
Delta R.T.: 0.000 min
Response: 881497
Conc: 157.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
LLEXSITUTV-025-001-SO

Manual Integrations
APPROVED

Ankita
2/2/2021 1:19:28 PM

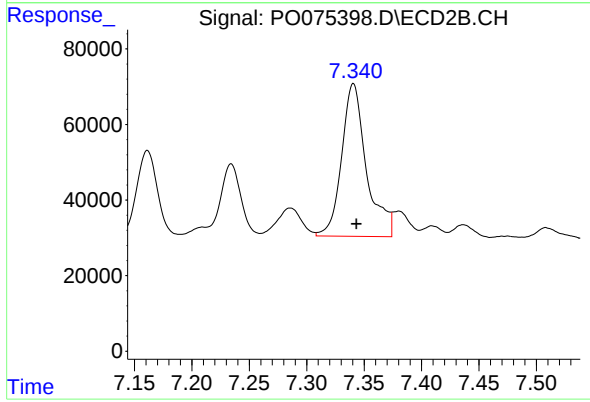

#30 AR-1254-5

R.T.: 7.341 min
Delta R.T.: -0.003 min
Response: 609024
Conc: 156.92 ng/ml