

Data Path : P:\HPCHEM1\ECD\_0\Data\P0020218\  
 Data File : P0041980.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 31 Jan 2018 13:32  
 Operator : SM/UA  
 Sample : J1370-19  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 15K-17A

Manual Integrations  
 APPROVED

ugo  
 1/31/2018 8:39:21 PM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 31 15:24:45 2018  
 Quant Method : P:\HPCHEM1\ECD\_0\P0012318.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Jan 23 01:50:31 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1 | Resp#2 | ng/ml  | ng/ml |
|-----------------------------|-------|-------|--------|--------|--------|-------|
| -----                       |       |       |        |        |        |       |
| System Monitoring Compounds |       |       |        |        |        |       |
| 1) SA Tetrachlo...          | 4.117 | 3.362 | 372564 | 577560 | 1.930  | 1.990 |
| 2) SA Decachlor...          | 9.514 | 8.156 | 290480 | 390615 | 1.236m | 1.092 |

Target Compounds

-----  
 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD\_0\Data\P0020218\  
Data File : P0041980.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 31 Jan 2018 13:32  
Operator : SM/UA  
Sample : J1370-19  
Misc :  
ALS Vial : 15 Sample Multiplier: 1



Instrument :  
ECD\_O  
ClientSampled :  
15K-17A


Manual Integrations  
APPROVED

ugo  
1/31/2018 8:39:21 PM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 31 15:24:45 2018  
Quant Method : P:\HPCHEM1\ECD\_0\P0012318.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Jan 23 01:50:31 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

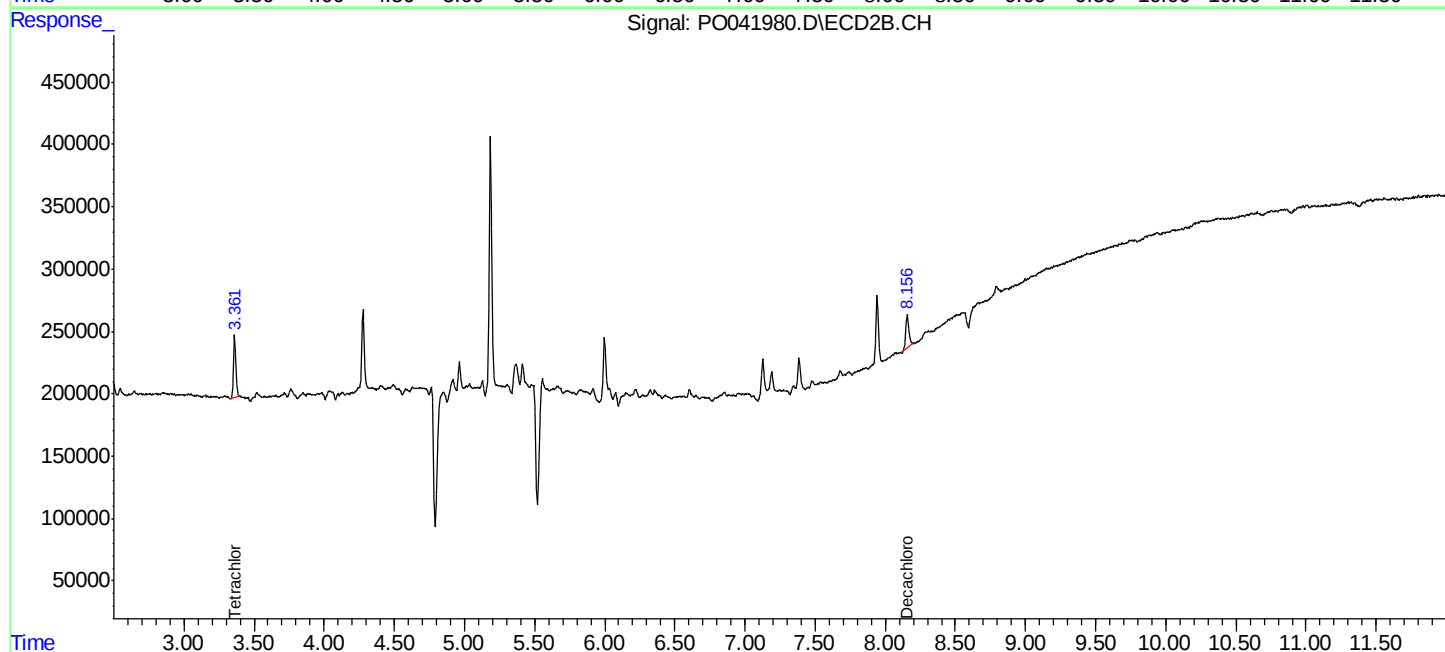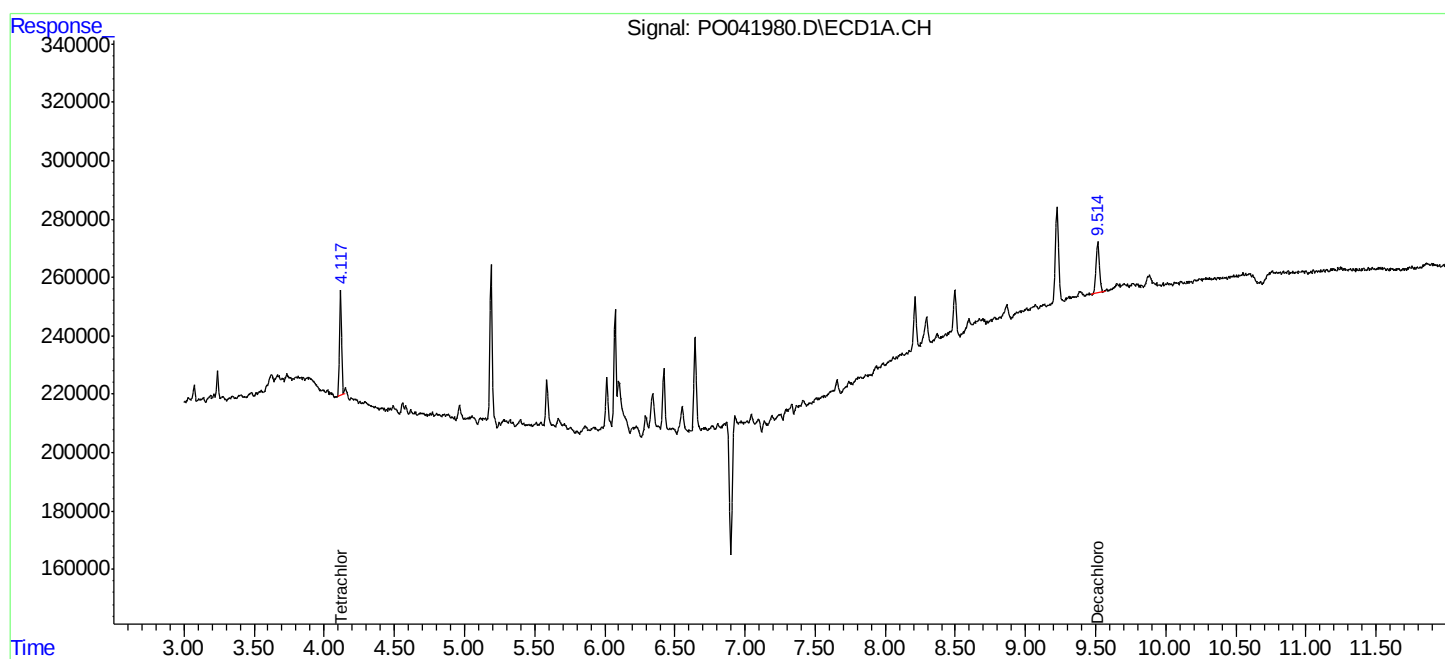

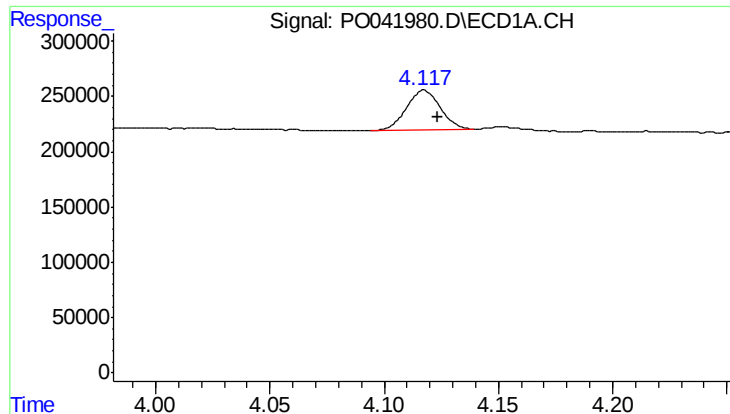


#1 Tetrachloro-m-xylene

R.T.: 4.117 min  
Delta R.T.: -0.006 min  
Response: 372564  
Conc: 1.93 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
15K-17A


Manual Integrations  
APPROVED

ugo  
1/31/2018 8:39:21 PM

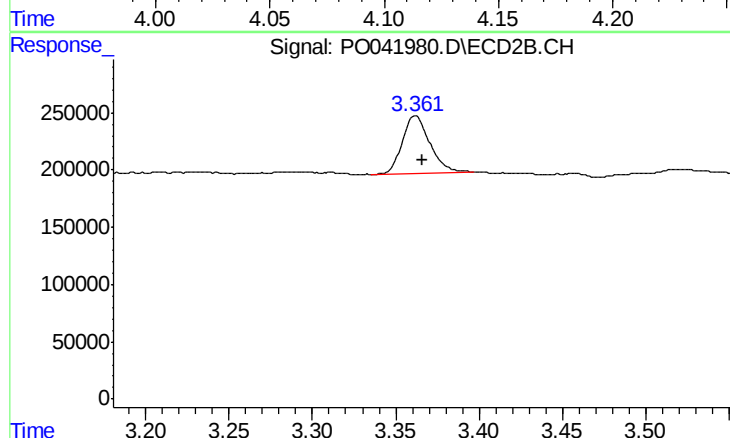


#1 Tetrachloro-m-xylene

R.T.: 3.362 min  
Delta R.T.: -0.004 min  
Response: 577560  
Conc: 1.99 ng/ml

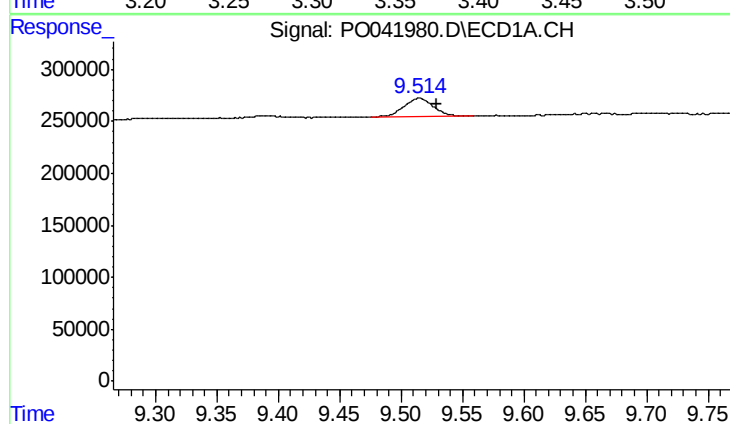

#2 Decachlorobiphenyl

R.T.: 9.514 min  
Delta R.T.: -0.015 min  
Response: 290480  
Conc: 1.24 ng/ml m

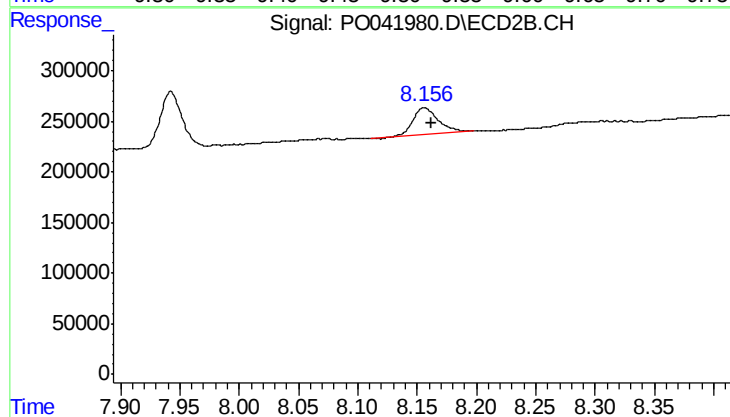

#2 Decachlorobiphenyl

R.T.: 8.156 min  
Delta R.T.: -0.006 min  
Response: 390615  
Conc: 1.09 ng/ml