

Data Path : P:\HPCHEM1\ECD 0\Data\P0020418\  
 Data File : P0042035.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 01 Feb 2018 15:54  
 Operator : SM/UA  
 Sample : J1343-01  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 MH-6

Manual Integrations  
 APPROVED

ugo  
 2/4/2018 10:19:32 AM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 01 16:34:40 2018  
 Quant Method : P:\HPCHEM1\ECD\_0\P0012318.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Jan 23 01:50:31 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1  | RT#2  | Resp#1  | Resp#2  | nq/ml  | nq/ml   |
|-----------------------------|-------|-------|---------|---------|--------|---------|
| -----                       |       |       |         |         |        |         |
| System Monitoring Compounds |       |       |         |         |        |         |
| 1) SA Tetrachlo...          | 4.122 | 3.360 | 3466321 | 5040262 | 17.959 | 17.363m |
| 2) SA Decachlor...          | 9.522 | 8.158 | 1643976 | 3371745 | 6.997  | 9.428m# |

Target Compounds

-----

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\PO020418\  
Data File : PO042035.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 01 Feb 2018 15:54  
Operator : SM/UA  
Sample : J1343-01  
Misc :  
ALS Vial : 4 Sample Multiplier: 1



Instrument :  
ECD\_O  
ClientSampleId :  
MH-6


Manual Integrations  
APPROVED

ugo  
2/4/2018 10:19:32 AM

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 01 16:34:40 2018  
Quant Method : P:\HPCHEM1\ECD\_0\PO012318.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Jan 23 01:50:31 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

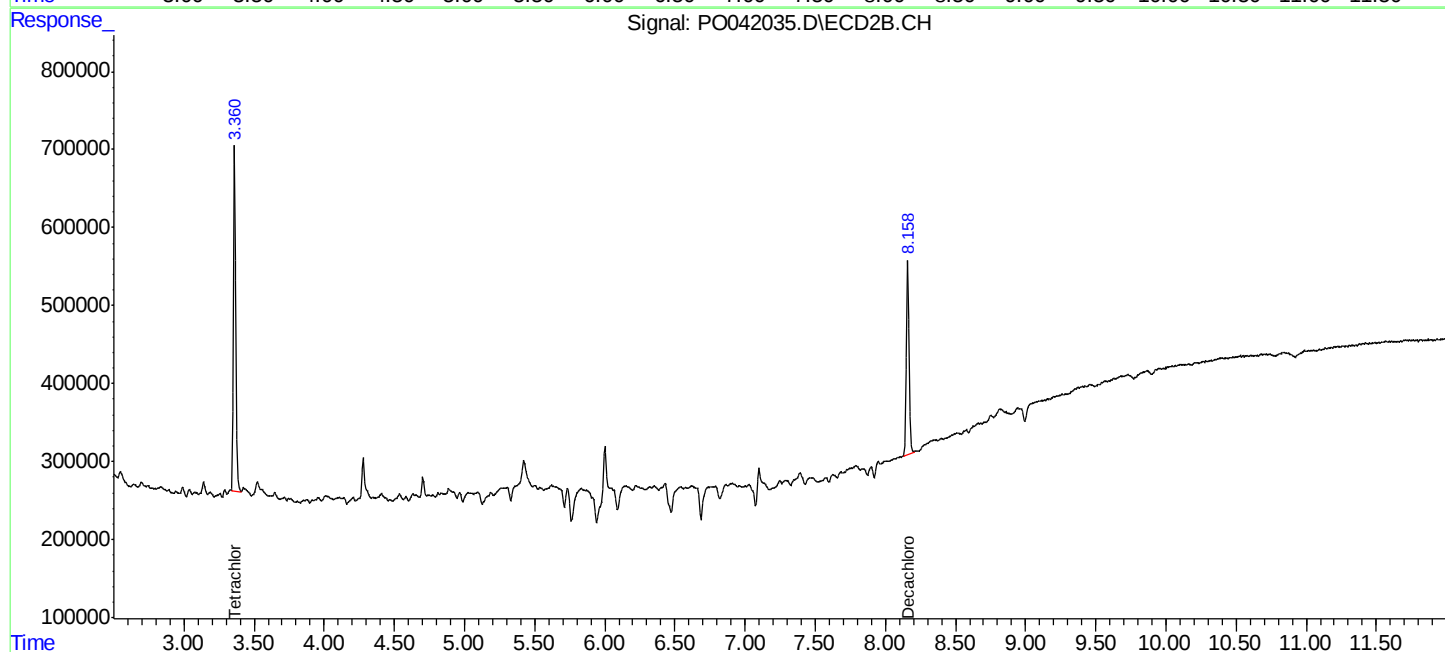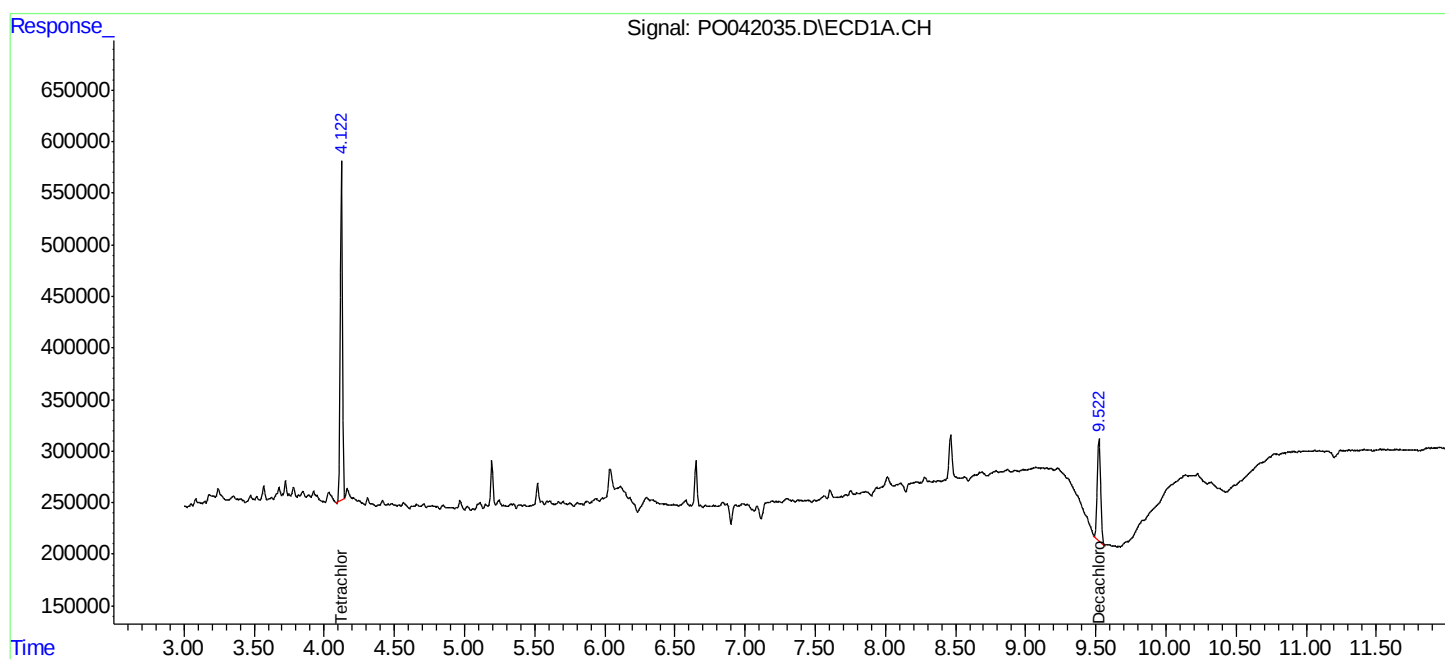

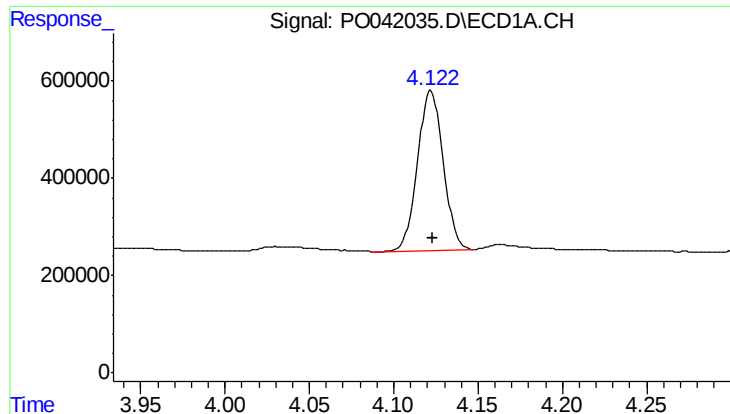


#1 Tetrachloro-m-xylene

R.T.: 4.122 min  
Delta R.T.: -0.001 min  
Response: 3466321  
Conc: 17.96 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
MH-6


Manual Integrations  
APPROVED

ugo  
2/4/2018 10:19:32 AM

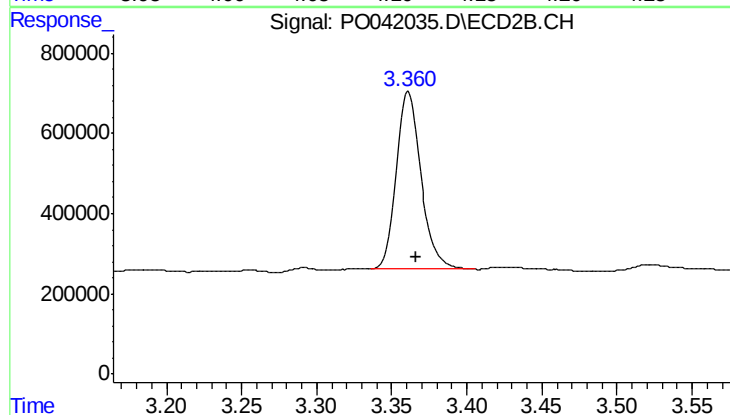


#1 Tetrachloro-m-xylene

R.T.: 3.360 min  
Delta R.T.: -0.006 min  
Response: 5040262  
Conc: 17.36 ng/ml m

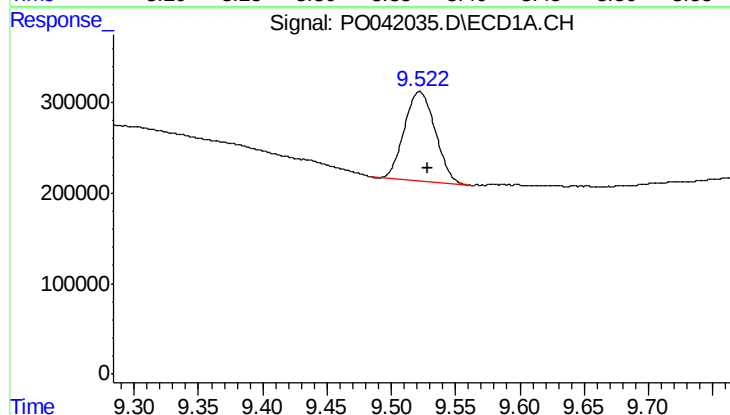

#2 Decachlorobiphenyl

R.T.: 9.522 min  
Delta R.T.: -0.007 min  
Response: 1643976  
Conc: 7.00 ng/ml

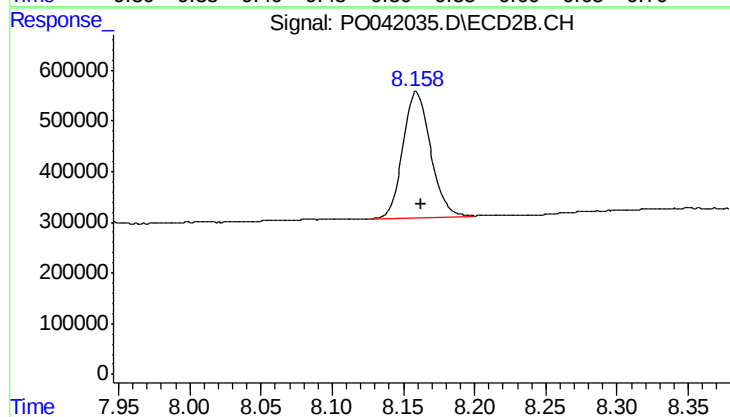

#2 Decachlorobiphenyl

R.T.: 8.158 min  
Delta R.T.: -0.004 min  
Response: 3371745  
Conc: 9.43 ng/ml m