

Data Path : P:\HPCHEM1\ECD 0\Data\P0020418\
 Data File : P0042041.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Feb 2018 17:23
 Operator : SM/UA
 Sample : J1364-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EQUIPMENT-BLANK

Manual Integrations
 APPROVED

ugo
 2/4/2018 10:19:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 02:31:26 2018
 Quant Method : P:\HPCHEM1\ECD_0\P0012318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 23 01:50:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.117	3.362	3391008	5320367	17.569	18.328
2) SA Decachlor...	9.516	8.155	3431526	4701149	14.605	13.146m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD 0\Data\PO020418\
Data File : PO042041.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Feb 2018 17:23
Operator : SM/UA
Sample : J1364-06
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EQUIPMENT-BLANK


Manual Integrations
APPROVED

ugo
2/4/2018 10:19:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 02:31:26 2018
Quant Method : P:\HPCHEM1\ECD_0\PO012318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 23 01:50:31 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

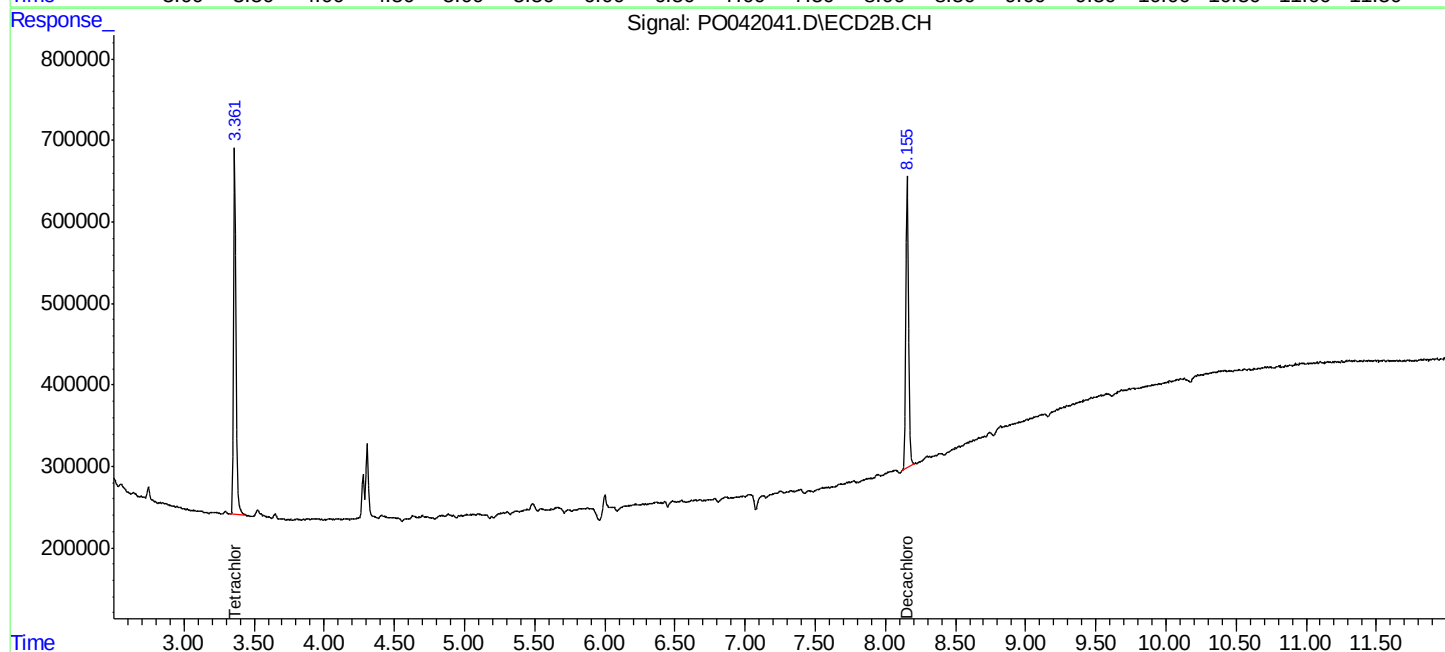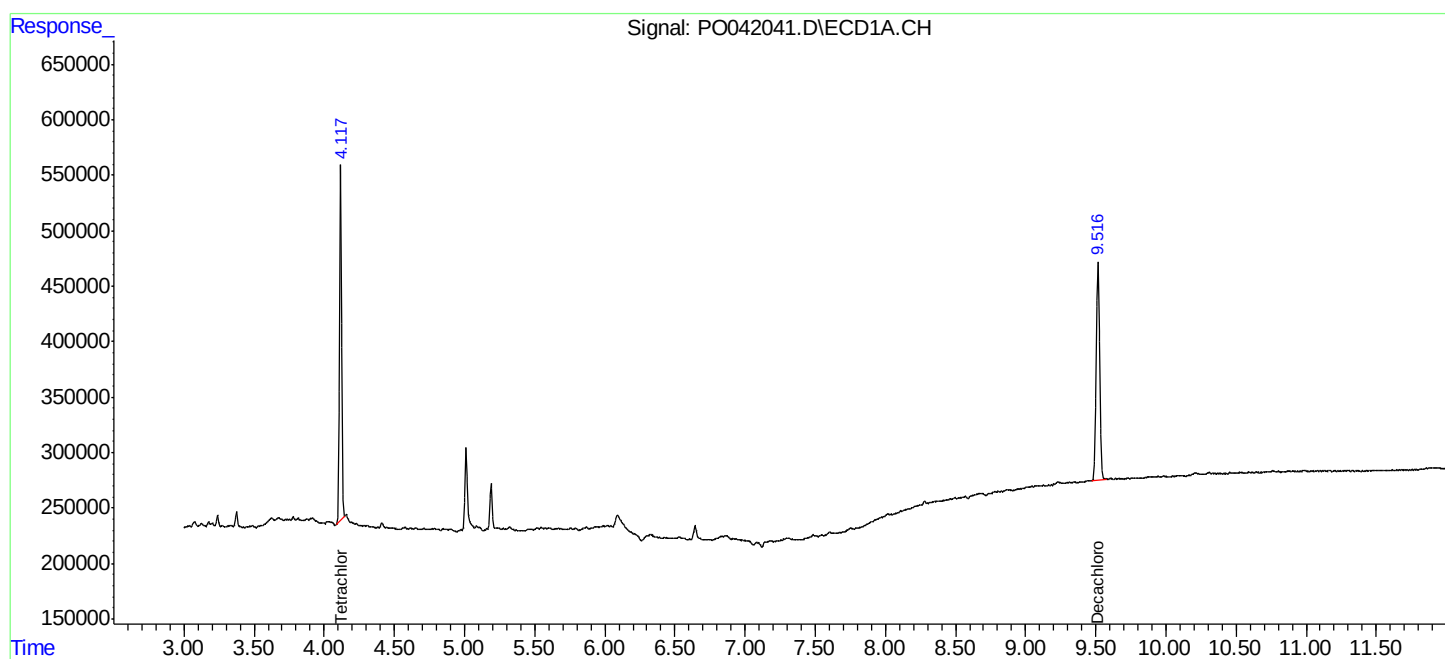

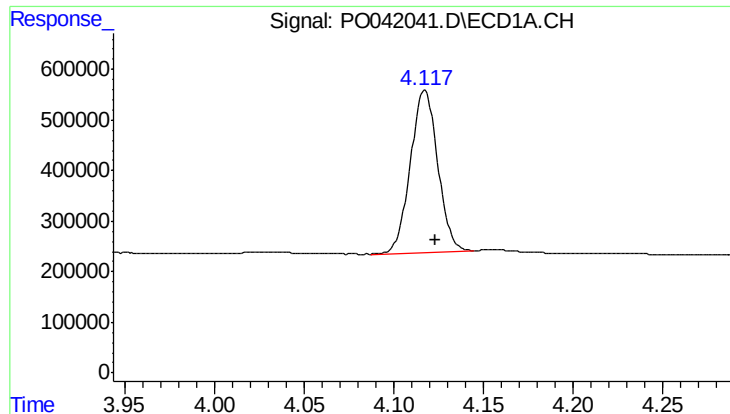


#1 Tetrachloro-m-xylene

R.T.: 4.117 min
Delta R.T.: -0.006 min
Response: 3391008
Conc: 17.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
EQUIPMENT-BLANK


Manual Integrations
APPROVED

ugo
2/4/2018 10:19:42 AM

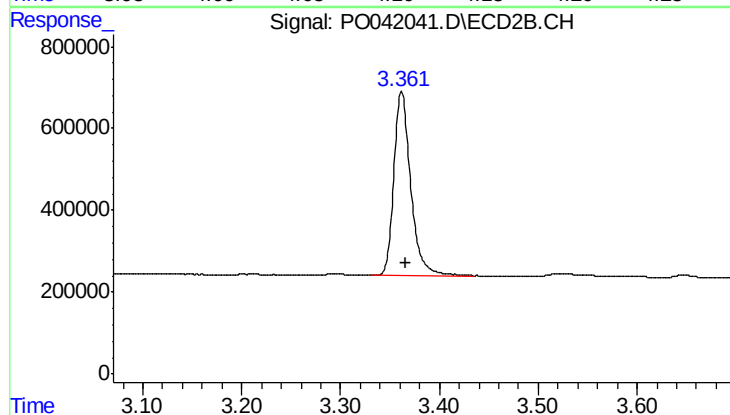


#1 Tetrachloro-m-xylene

R.T.: 3.362 min
Delta R.T.: -0.004 min
Response: 5320367
Conc: 18.33 ng/ml

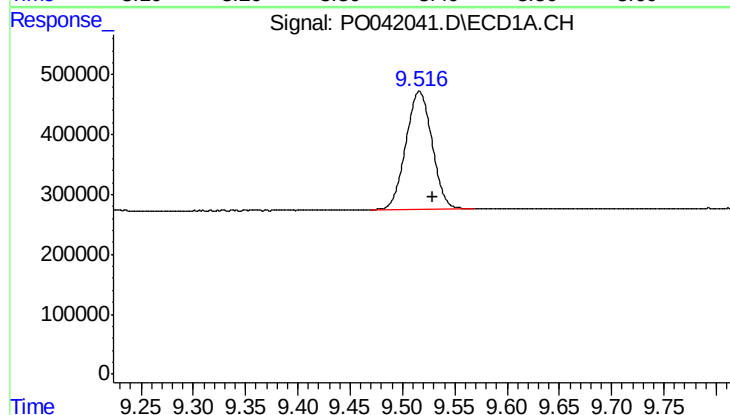

#2 Decachlorobiphenyl

R.T.: 9.516 min
Delta R.T.: -0.013 min
Response: 3431526
Conc: 14.61 ng/ml

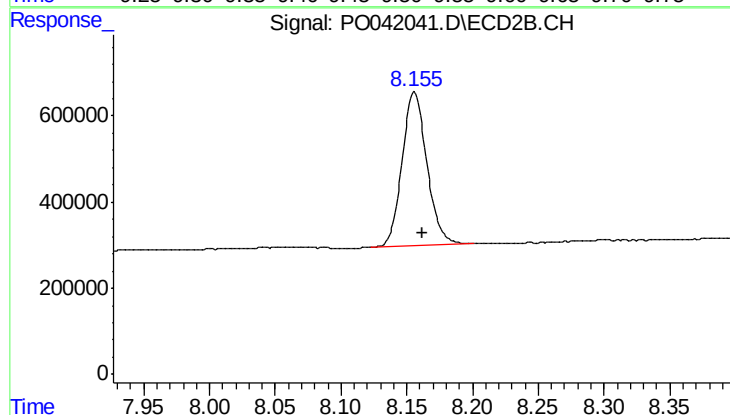

#2 Decachlorobiphenyl

R.T.: 8.155 min
Delta R.T.: -0.007 min
Response: 4701149
Conc: 13.15 ng/ml m