

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020419\
 Data File : P0053710.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2019 18:45
 Operator : SM/SJ
 Sample : K1362-01MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-005-ABCDMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 23:44:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.095	3.159	48042133	5122535	24.649	21.357
2)	SA Decachlor...	9.483	7.765	20932119	5438335	21.477	21.779
Target Compounds							
3)	L1 AR-1016-1	5.235	4.150	10874874	3721254	241.519	422.968 #
4)	L1 AR-1016-2	5.256	4.150	18019264	3721254	267.393	263.595
5)	L1 AR-1016-3	5.316	4.307	11456210	1991848	288.660	252.377
6)	L1 AR-1016-4	5.414	4.350	9419832	1504283	295.990	287.662
7)	L1 AR-1016-5	5.697	4.540	8361206	1963142	298.014	270.043
9)	L2 AR-1221-2	4.391	3.429	2058474	272189	171.996	152.566
10)	L2 AR-1221-3	4.466	3.496	7267404	1113355	184.513	176.802
11)	L3 AR-1232-1	4.466	3.496	7267404	1113355	226.290	207.915
12)	L3 AR-1232-2	4.974	4.150	9776748	3721254	642.624	585.953
13)	L3 AR-1232-3	5.256	4.307	18019264	1991848	615.021	564.455
14)	L3 AR-1232-4	5.414	4.385	9419832	1856691	665.451	725.491
15)	L3 AR-1232-5	5.498	4.540	7278220	1963142	908.322	624.378 #
16)	L4 AR-1242-1	5.235	4.136	10874874	2425635	300.806	326.704
17)	L4 AR-1242-2	5.256	4.150	18019264	3721254	341.086	324.742
18)	L4 AR-1242-3	5.316	4.307	11456210	1991848	358.687	323.164
19)	L4 AR-1242-4	5.414	4.385	9419832	1856691	364.158	348.319
20)	L4 AR-1242-5	0.000	4.862	0	1518152	N.D.	206.627 #
21)	L5 AR-1248-1	5.235	4.136	10874874	2425635	397.401	423.284
22)	L5 AR-1248-2	5.498	4.350	7278220	1504283	220.910	198.304
23)	L5 AR-1248-3	5.697	4.385	8361206	1856691	218.393	236.974
24)	L5 AR-1248-4	6.063	4.540	4635883	1963142	110.456	197.726 #
25)	L5 AR-1248-5	0.000	4.862	0	1518152	N.D.	146.617 #
26)	L6 AR-1254-1	6.063	4.862	4635883	1518152	110.259	93.216
27)	L6 AR-1254-2	6.276	5.001	5960631	1472792	91.321	106.783
28)	L6 AR-1254-3	6.640	5.385	3001656	2636686	43.843	120.625 #
29)	L6 AR-1254-4	6.918	5.593	1843090	309523	36.162	21.806 #
30)	L6 AR-1254-5	7.331	5.980	17233551	4877829	360.045	261.132 #
31)	L7 AR-1260-1	6.794	5.492	12271013	3722839	251.745	244.491
32)	L7 AR-1260-2	7.048	5.676	14974780	4499517	240.966	242.671
33)	L7 AR-1260-3	7.398	5.812	9715103	4067402	248.360	237.933
34)	L7 AR-1260-4	7.623	6.257	10072112	2785980	233.088	252.987
35)	L7 AR-1260-5	7.929	6.499	21068811	6380970	231.450	234.327
36)	L8 AR-1262-1	7.398	6.015	9715103	3205274	141.593	161.845
37)	L8 AR-1262-2	7.929	6.499	21068811	6380970	174.865	187.890
38)	L8 AR-1262-3	8.225	6.762	8401198	1377336	340.669	105.947 #
39)	L8 AR-1262-4	8.269	6.825	7948096	4704302	128.220	192.199 #
40)	L8 AR-1262-5	8.862	7.309	5261553	1449108	124.575	129.633
41)	L9 AR-1268-1	8.199	6.762	4413426	1377336	29.787	35.670
42)	L9 AR-1268-2	8.269	6.825	7948096	4704302	56.631	128.645 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020419\
 Data File : P0053710.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2019 18:45
 Operator : SM/SJ
 Sample : K1362-01MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-005-ABCDMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 23:44:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	8.862	7.309	5261553	1449108	110.677	116.358
45) L9	AR-1268-5	9.208	7.566	1779911	509577	4.747	5.432



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO020419\
Data File : PO053710.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2019 18:45
Operator : SM/SJ
Sample : K1362-01MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 23:44:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

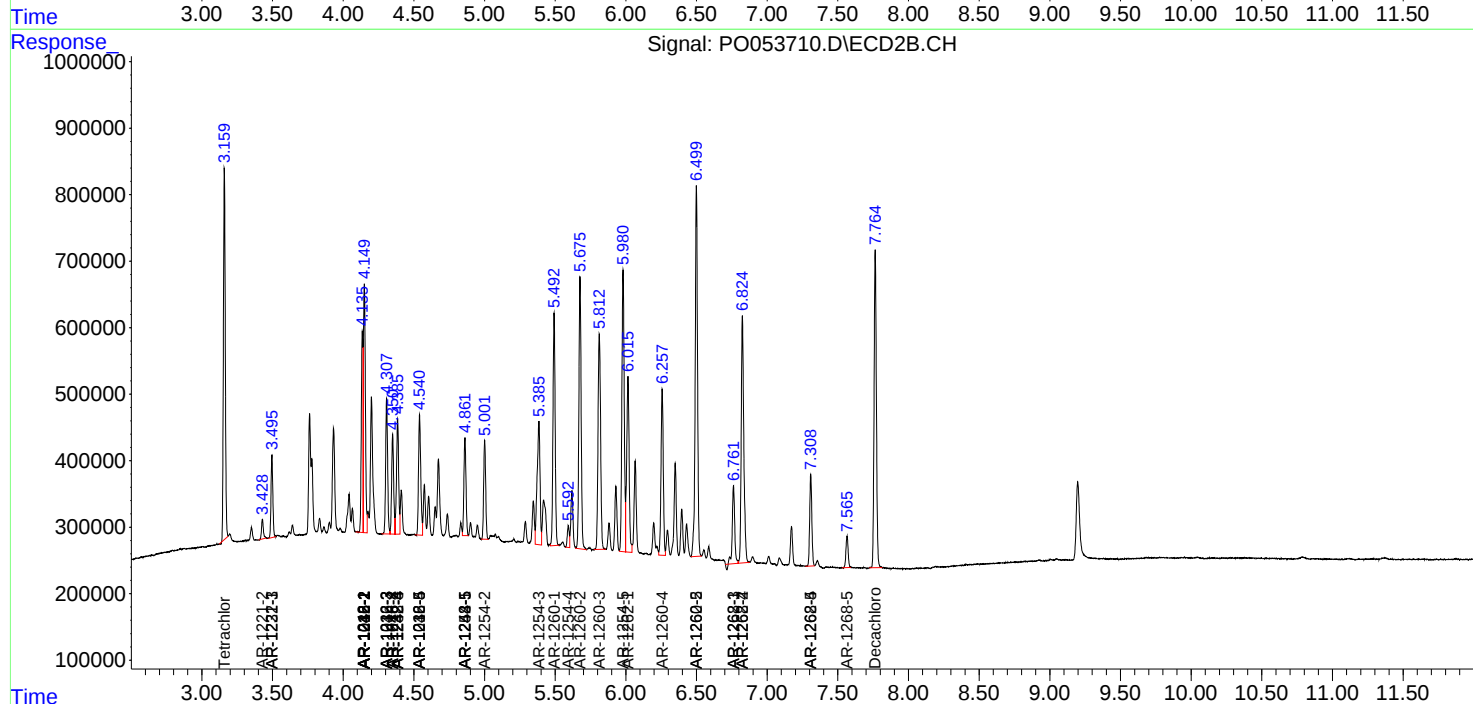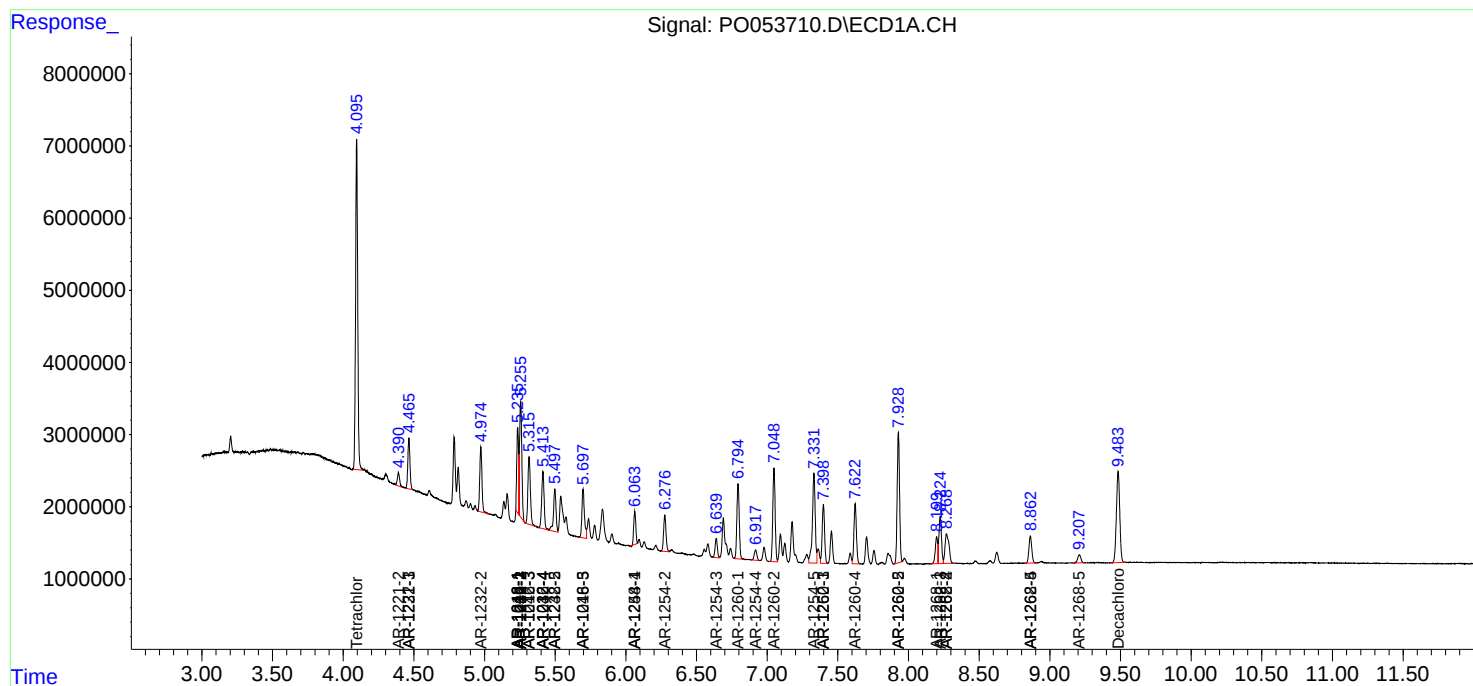


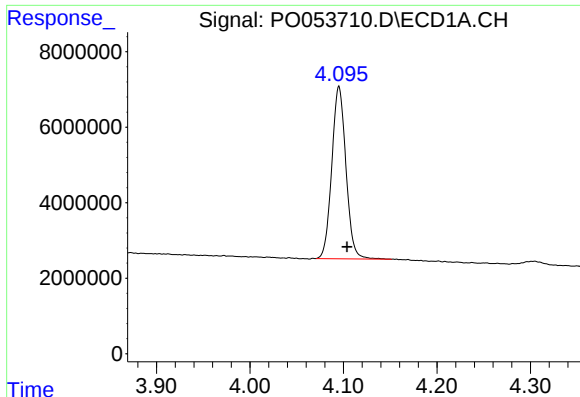

#1 Tetrachloro-m-xylene


R.T.: 4.095 min
Delta R.T.: -0.009 min
Response: 48042133
Conc: 24.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

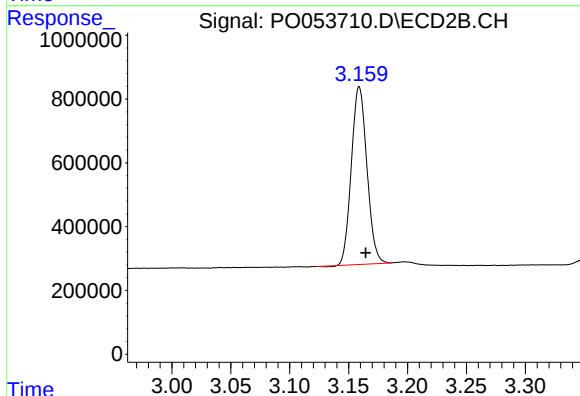


#1 Tetrachloro-m-xylene

R.T.: 3.159 min
Delta R.T.: -0.006 min
Response: 5122535
Conc: 21.36 ng/ml

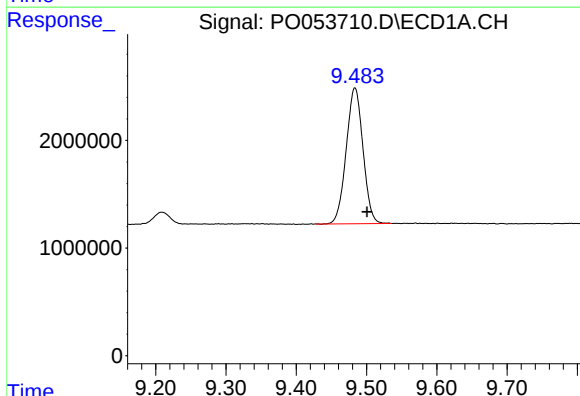


#2 Decachlorobiphenyl

R.T.: 9.483 min
Delta R.T.: -0.017 min
Response: 20932119
Conc: 21.48 ng/ml

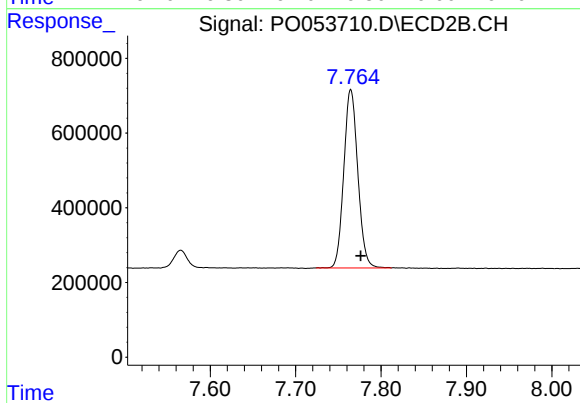

#2 Decachlorobiphenyl


R.T.: 7.765 min
Delta R.T.: -0.012 min
Response: 5438335
Conc: 21.78 ng/ml

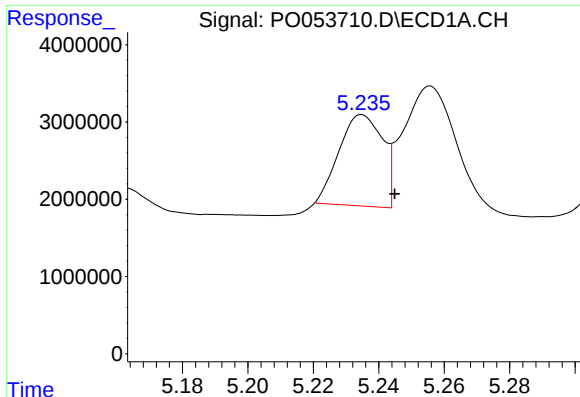

#3 AR-1016-1


R.T.: 5.235 min
Delta R.T.: -0.010 min
Response: 10874874
Conc: 241.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

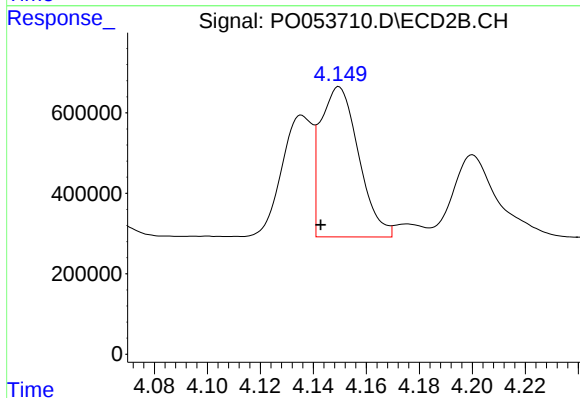


#3 AR-1016-1

R.T.: 4.150 min
Delta R.T.: 0.007 min
Response: 3721254
Conc: 422.97 ng/ml

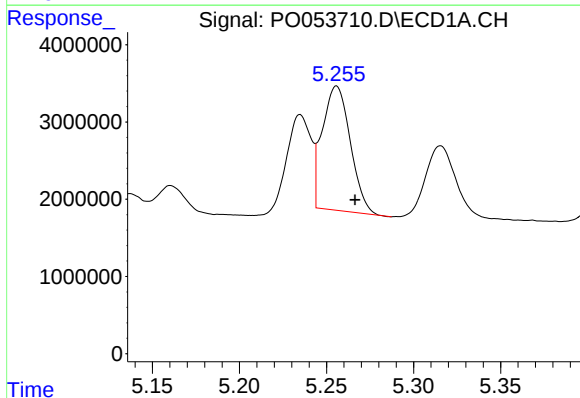


#4 AR-1016-2

R.T.: 5.256 min
Delta R.T.: -0.011 min
Response: 18019264
Conc: 267.39 ng/ml

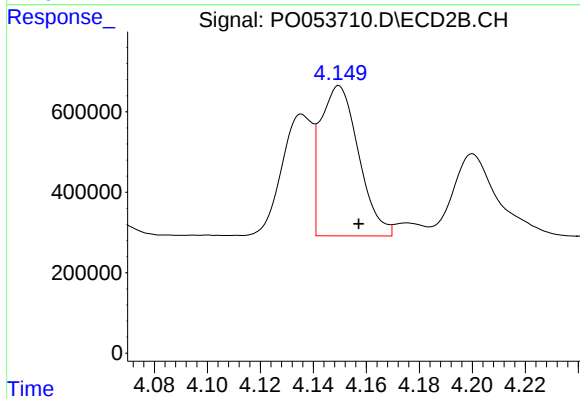

#4 AR-1016-2


R.T.: 4.150 min
Delta R.T.: -0.007 min
Response: 3721254
Conc: 263.60 ng/ml

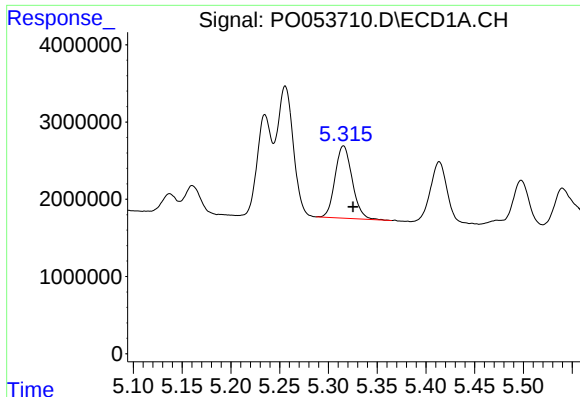

#5 AR-1016-3


R.T.: 5.316 min
Delta R.T.: -0.010 min
Response: 11456210
Conc: 288.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

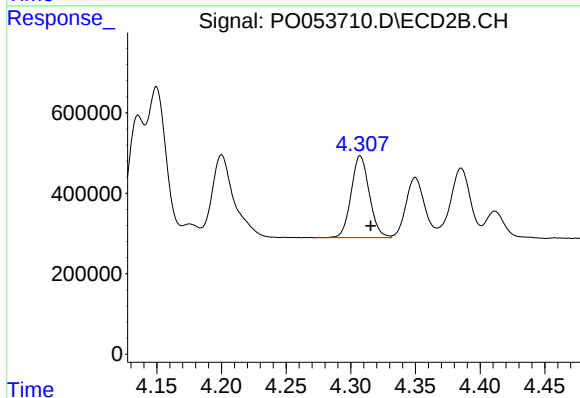


#5 AR-1016-3

R.T.: 4.307 min
Delta R.T.: -0.008 min
Response: 1991848
Conc: 252.38 ng/ml

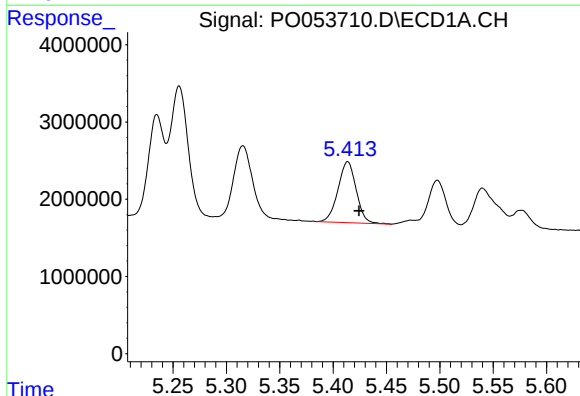


#6 AR-1016-4

R.T.: 5.414 min
Delta R.T.: -0.011 min
Response: 9419832
Conc: 295.99 ng/ml

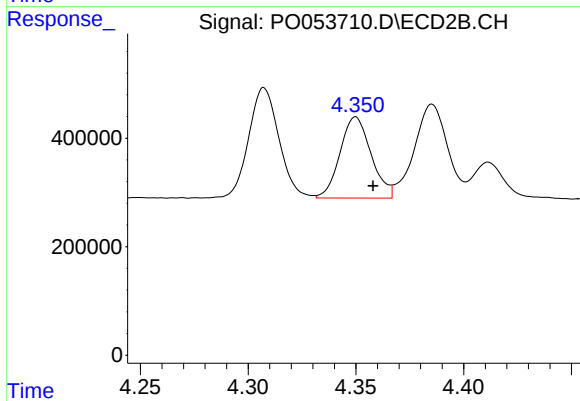

#6 AR-1016-4


R.T.: 4.350 min
Delta R.T.: -0.008 min
Response: 1504283
Conc: 287.66 ng/ml

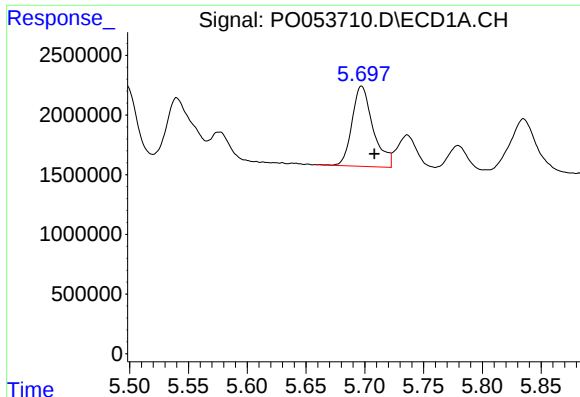

#7 AR-1016-5


R.T.: 5.697 min
Delta R.T.: -0.011 min
Response: 8361206
Conc: 298.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

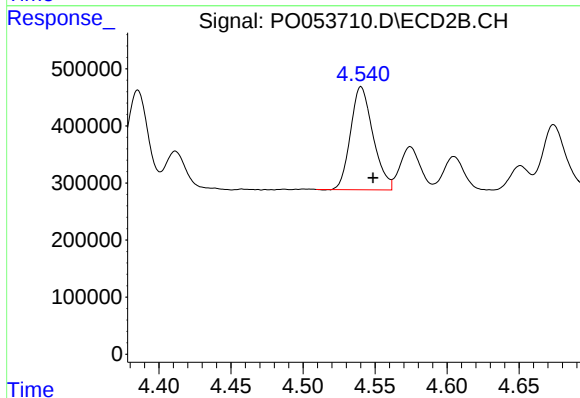


#7 AR-1016-5

R.T.: 4.540 min
Delta R.T.: -0.008 min
Response: 1963142
Conc: 270.04 ng/ml

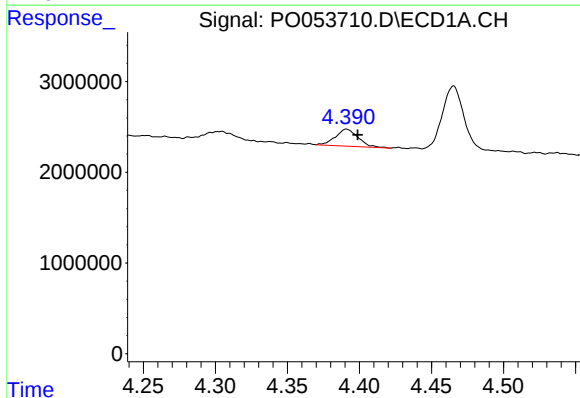


#9 AR-1221-2

R.T.: 4.391 min
Delta R.T.: -0.008 min
Response: 2058474
Conc: 172.00 ng/ml

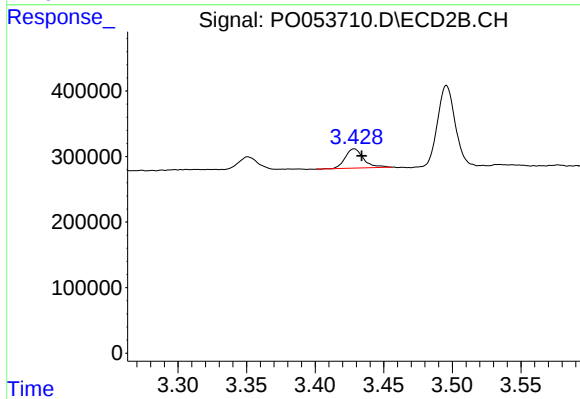

#9 AR-1221-2


R.T.: 3.429 min
Delta R.T.: -0.006 min
Response: 272189
Conc: 152.57 ng/ml

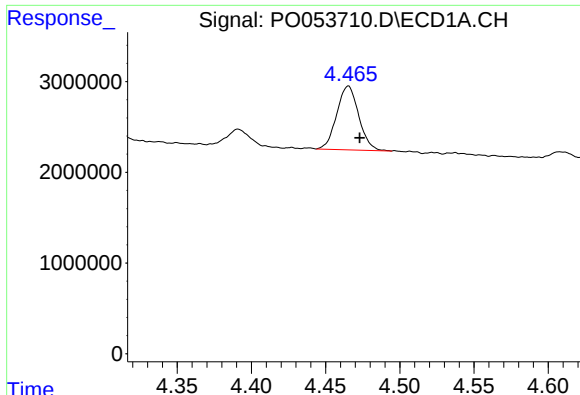

#10 AR-1221-3


R.T.: 4.466 min
Delta R.T.: -0.007 min
Response: 7267404
Conc: 184.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

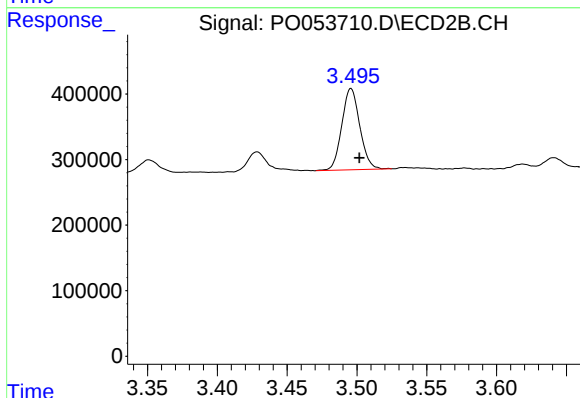


#10 AR-1221-3

R.T.: 3.496 min
Delta R.T.: -0.006 min
Response: 1113355
Conc: 176.80 ng/ml

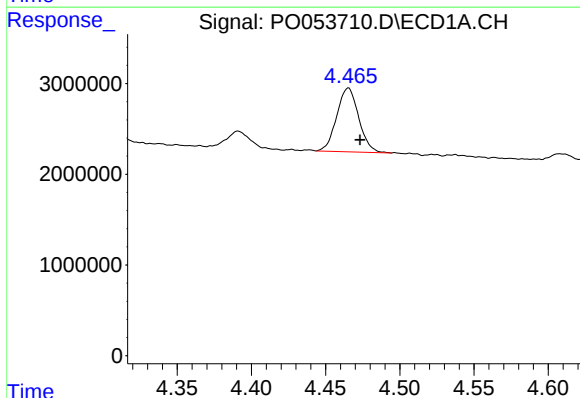


#11 AR-1232-1

R.T.: 4.466 min
Delta R.T.: -0.008 min
Response: 7267404
Conc: 226.29 ng/ml

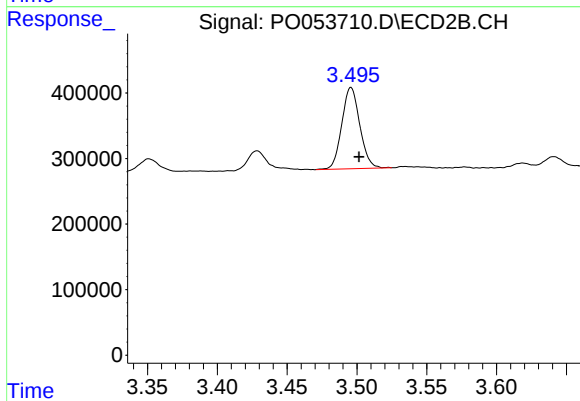

#11 AR-1232-1


R.T.: 3.496 min
Delta R.T.: -0.006 min
Response: 1113355
Conc: 207.92 ng/ml

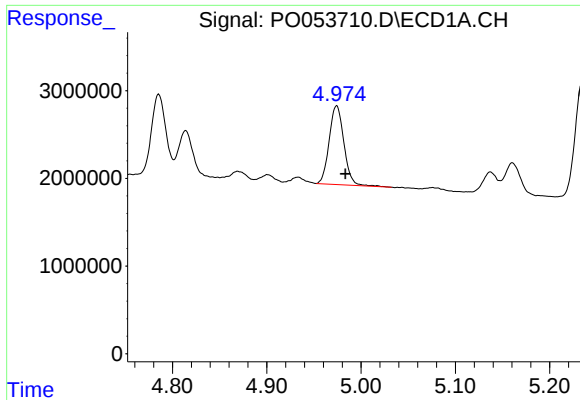

#12 AR-1232-2


R.T.: 4.974 min
Delta R.T.: -0.009 min
Response: 9776748
Conc: 642.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

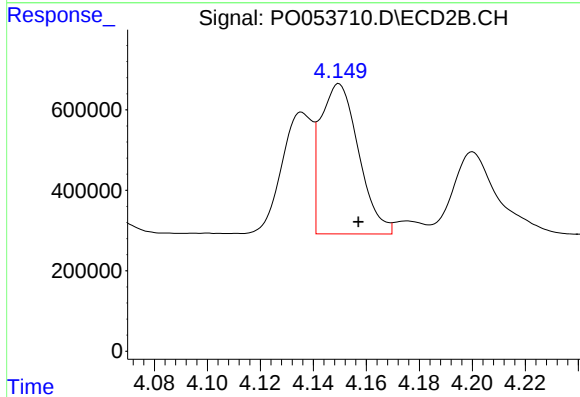


#12 AR-1232-2

R.T.: 4.150 min
Delta R.T.: -0.007 min
Response: 3721254
Conc: 585.95 ng/ml

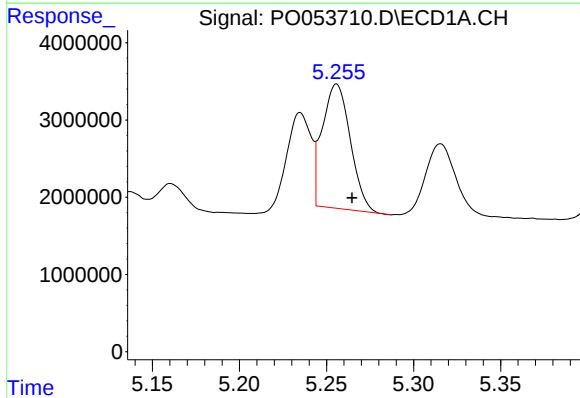


#13 AR-1232-3

R.T.: 5.256 min
Delta R.T.: -0.009 min
Response: 18019264
Conc: 615.02 ng/ml

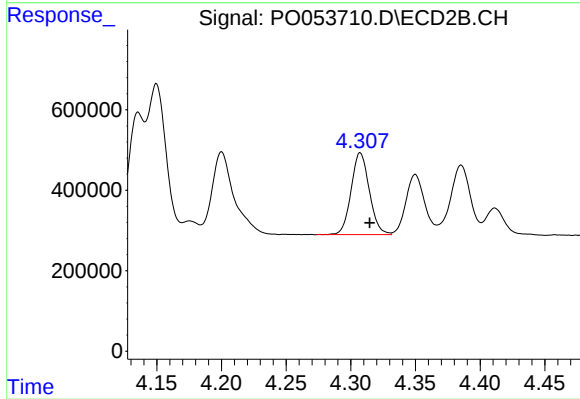

#13 AR-1232-3


R.T.: 4.307 min
Delta R.T.: -0.007 min
Response: 1991848
Conc: 564.45 ng/ml

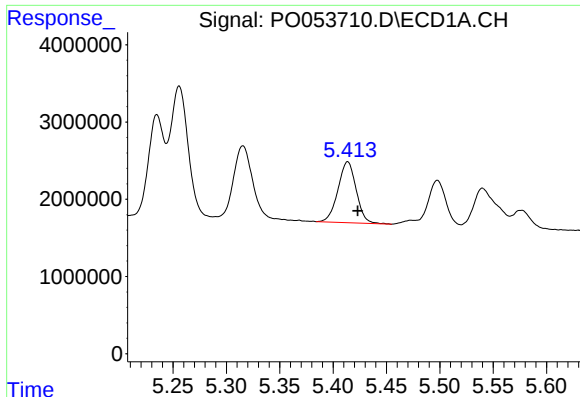

#14 AR-1232-4


R.T.: 5.414 min
Delta R.T.: -0.009 min
Response: 9419832
Conc: 665.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

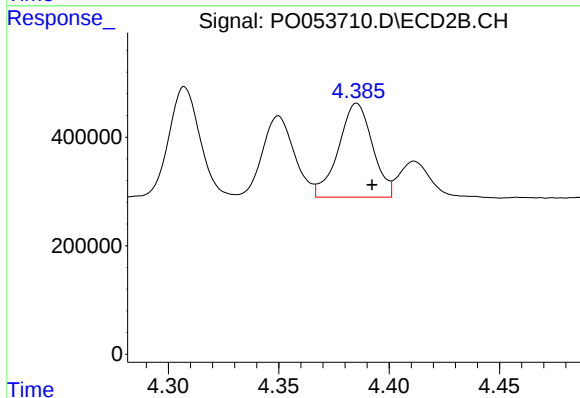


#14 AR-1232-4

R.T.: 4.385 min
Delta R.T.: -0.007 min
Response: 1856691
Conc: 725.49 ng/ml

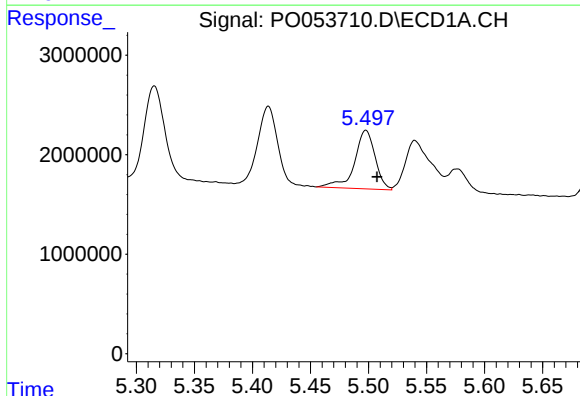


#15 AR-1232-5

R.T.: 5.498 min
Delta R.T.: -0.010 min
Response: 7278220
Conc: 908.32 ng/ml

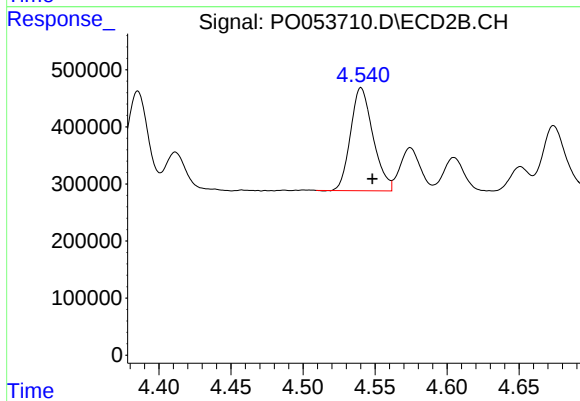

#15 AR-1232-5


R.T.: 4.540 min
Delta R.T.: -0.008 min
Response: 1963142
Conc: 624.38 ng/ml

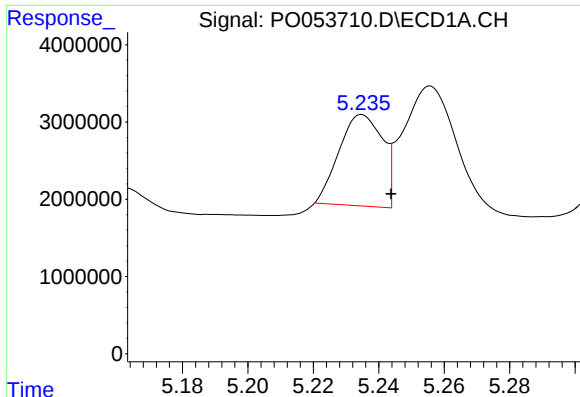

#16 AR-1242-1


R.T.: 5.235 min
Delta R.T.: -0.009 min
Response: 10874874
Conc: 300.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

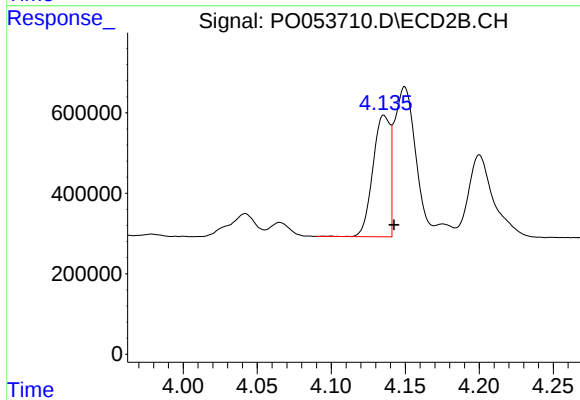


#16 AR-1242-1

R.T.: 4.136 min
Delta R.T.: -0.007 min
Response: 2425635
Conc: 326.70 ng/ml

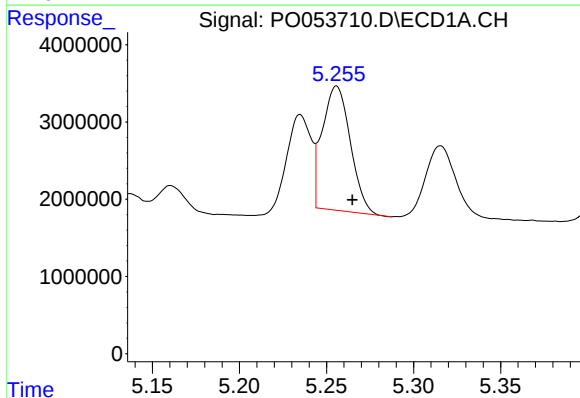


#17 AR-1242-2

R.T.: 5.256 min
Delta R.T.: -0.009 min
Response: 18019264
Conc: 341.09 ng/ml

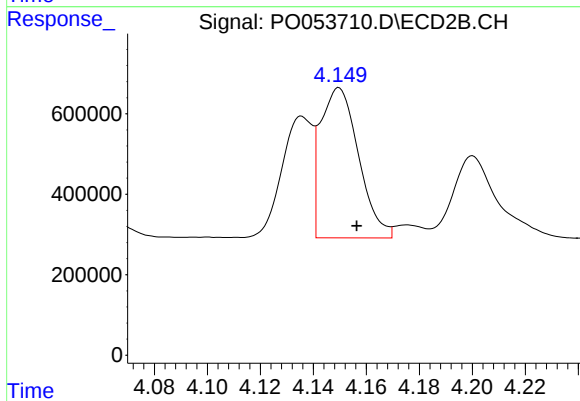

#17 AR-1242-2


R.T.: 4.150 min
Delta R.T.: -0.007 min
Response: 3721254
Conc: 324.74 ng/ml

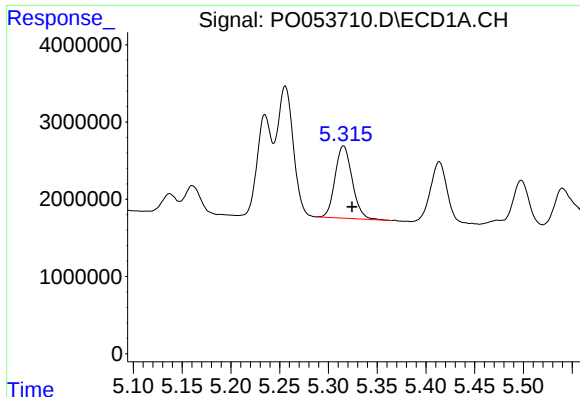

#18 AR-1242-3


R.T.: 5.316 min
Delta R.T.: -0.009 min
Response: 11456210
Conc: 358.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

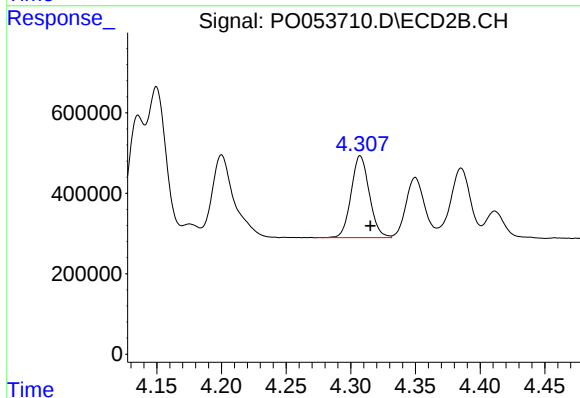


#18 AR-1242-3

R.T.: 4.307 min
Delta R.T.: -0.008 min
Response: 1991848
Conc: 323.16 ng/ml

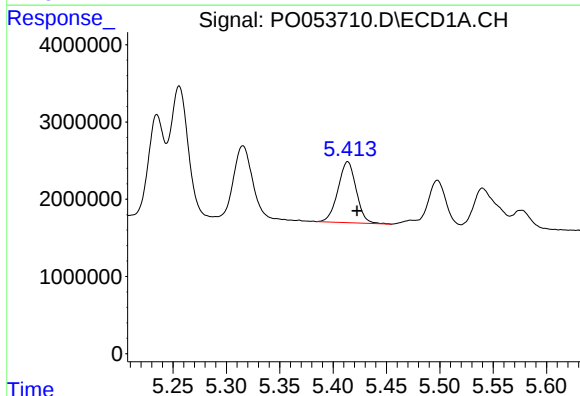


#19 AR-1242-4

R.T.: 5.414 min
Delta R.T.: -0.009 min
Response: 9419832
Conc: 364.16 ng/ml

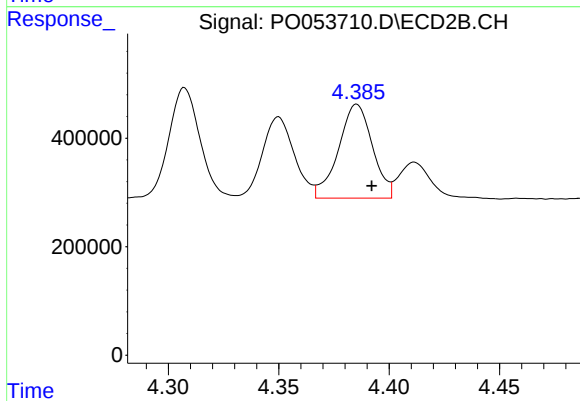

#19 AR-1242-4


R.T.: 4.385 min
Delta R.T.: -0.007 min
Response: 1856691
Conc: 348.32 ng/ml

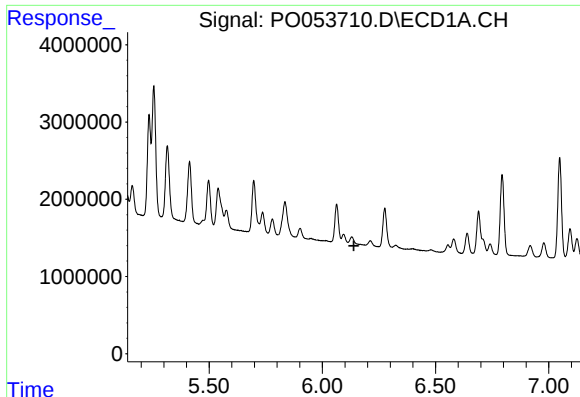

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.140 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

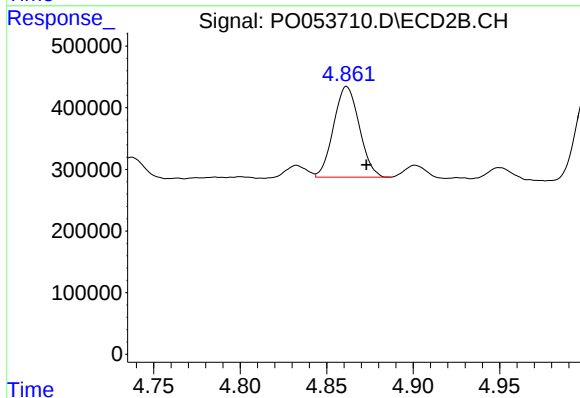


#20 AR-1242-5

R.T.: 4.862 min
Delta R.T.: -0.011 min
Response: 1518152
Conc: 206.63 ng/ml

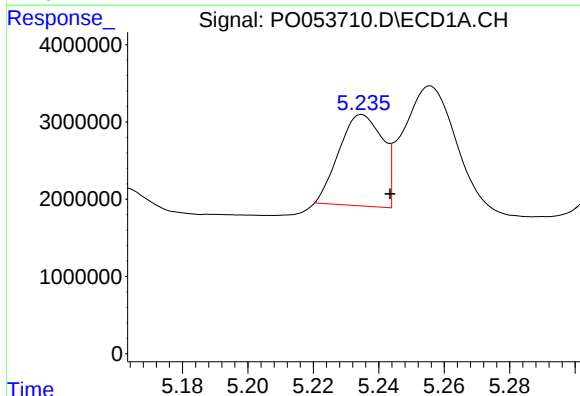


#21 AR-1248-1

R.T.: 5.235 min
Delta R.T.: -0.009 min
Response: 10874874
Conc: 397.40 ng/ml

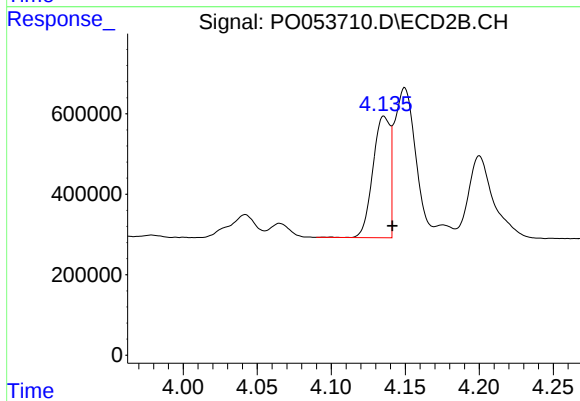

#21 AR-1248-1


R.T.: 4.136 min
Delta R.T.: -0.006 min
Response: 2425635
Conc: 423.28 ng/ml

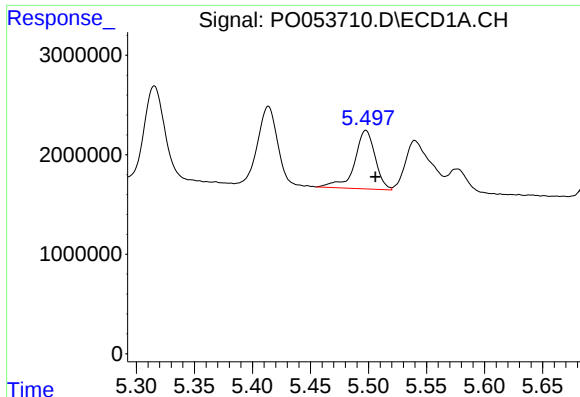

#22 AR-1248-2


R.T.: 5.498 min
Delta R.T.: -0.008 min
Response: 7278220
Conc: 220.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

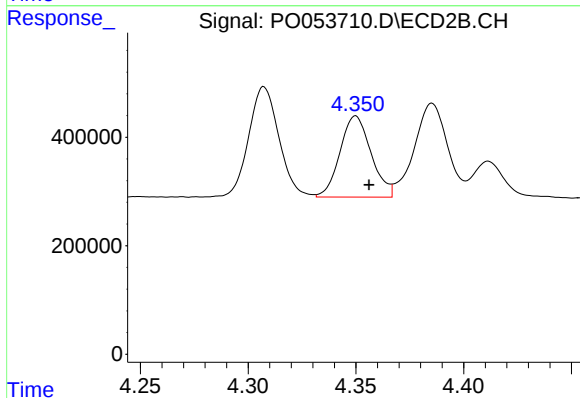


#22 AR-1248-2

R.T.: 4.350 min
Delta R.T.: -0.006 min
Response: 1504283
Conc: 198.30 ng/ml

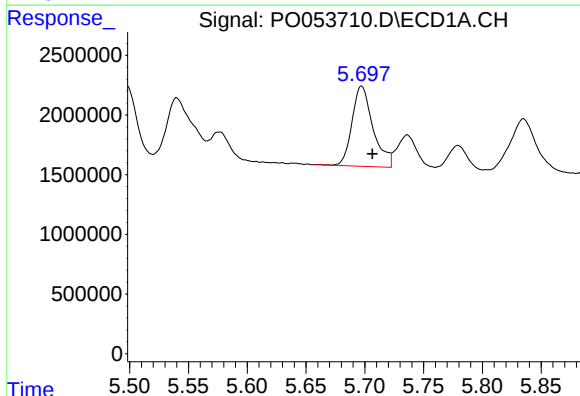


#23 AR-1248-3

R.T.: 5.697 min
Delta R.T.: -0.009 min
Response: 8361206
Conc: 218.39 ng/ml

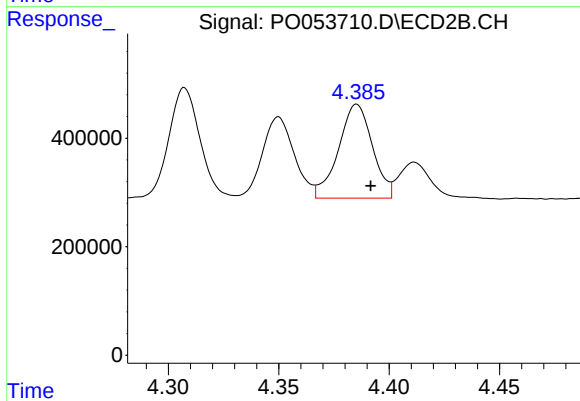

#23 AR-1248-3


R.T.: 4.385 min
Delta R.T.: -0.006 min
Response: 1856691
Conc: 236.97 ng/ml

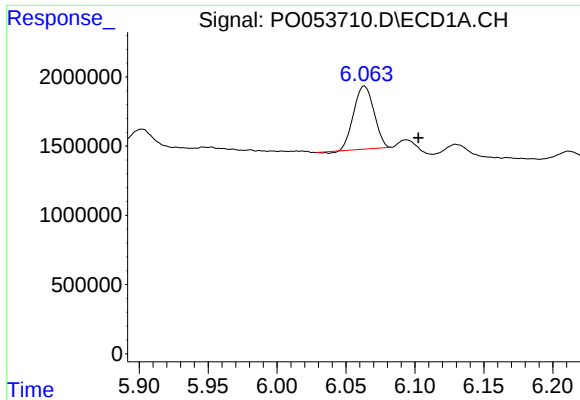

#24 AR-1248-4


R.T.: 6.063 min
Delta R.T.: -0.039 min
Response: 4635883
Conc: 110.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

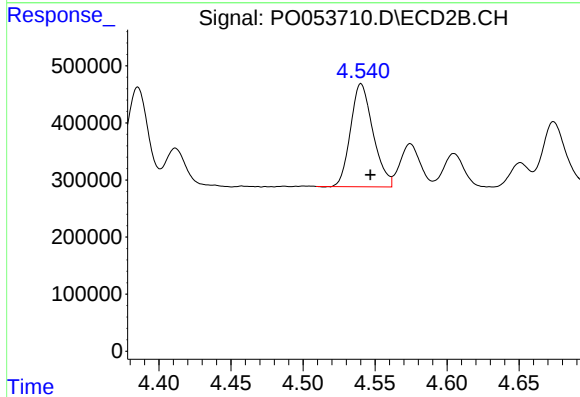


#24 AR-1248-4

R.T.: 4.540 min
Delta R.T.: -0.007 min
Response: 1963142
Conc: 197.73 ng/ml

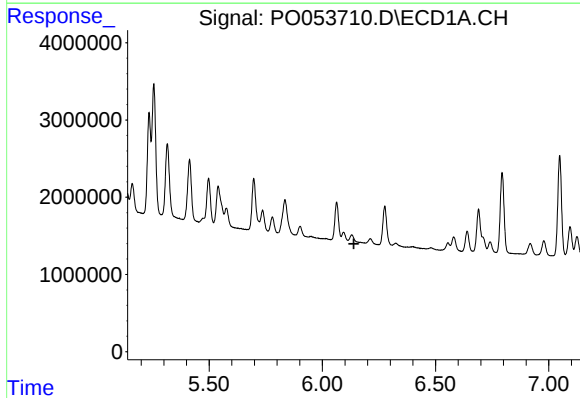


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.140 min
Response: 0
Conc: N.D.

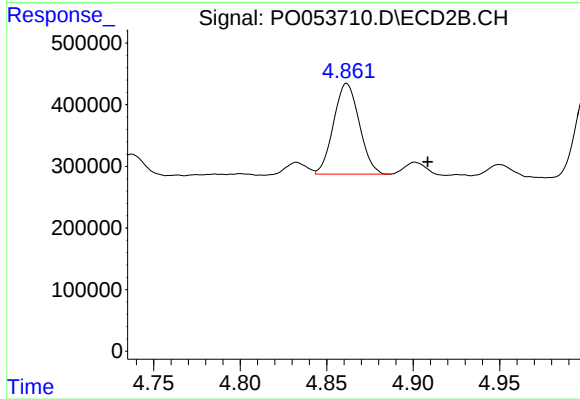

#25 AR-1248-5


R.T.: 4.862 min
Delta R.T.: -0.047 min
Response: 1518152
Conc: 146.62 ng/ml

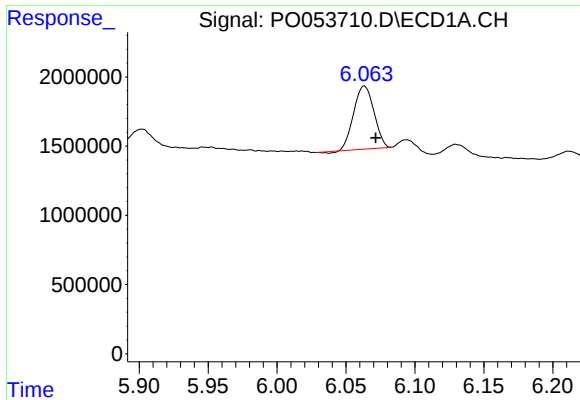

#26 AR-1254-1


R.T.: 6.063 min
Delta R.T.: -0.008 min
Response: 4635883
Conc: 110.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

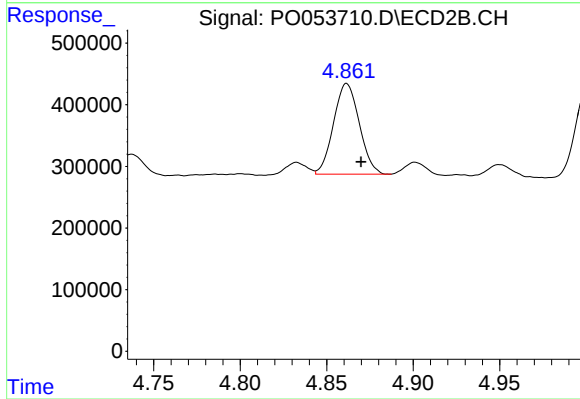


#26 AR-1254-1

R.T.: 4.862 min
Delta R.T.: -0.008 min
Response: 1518152
Conc: 93.22 ng/ml

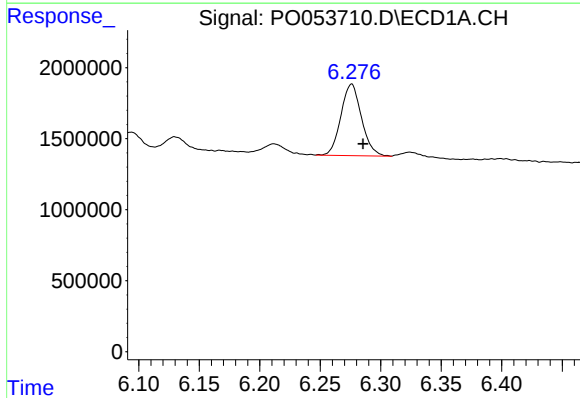


#27 AR-1254-2

R.T.: 6.276 min
Delta R.T.: -0.009 min
Response: 5960631
Conc: 91.32 ng/ml

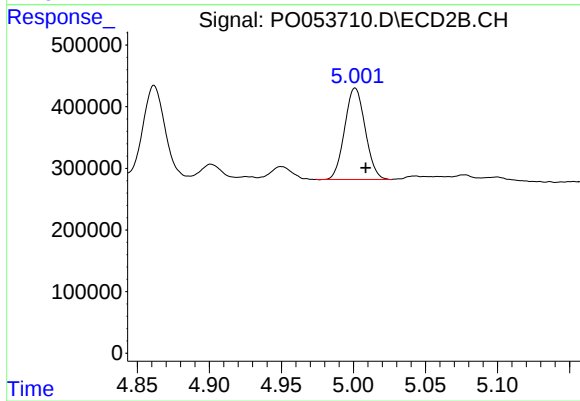

#27 AR-1254-2


R.T.: 5.001 min
Delta R.T.: -0.007 min
Response: 1472792
Conc: 106.78 ng/ml

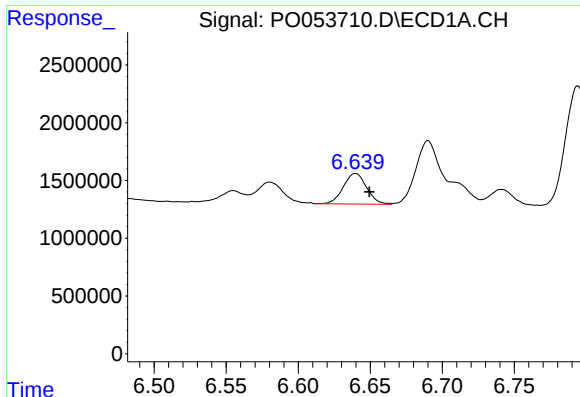

#28 AR-1254-3


R.T.: 6.640 min
Delta R.T.: -0.010 min
Response: 3001656
Conc: 43.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

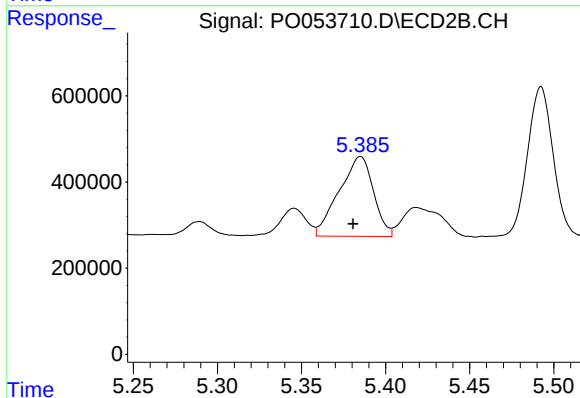


#28 AR-1254-3

R.T.: 5.385 min
Delta R.T.: 0.004 min
Response: 2636686
Conc: 120.63 ng/ml

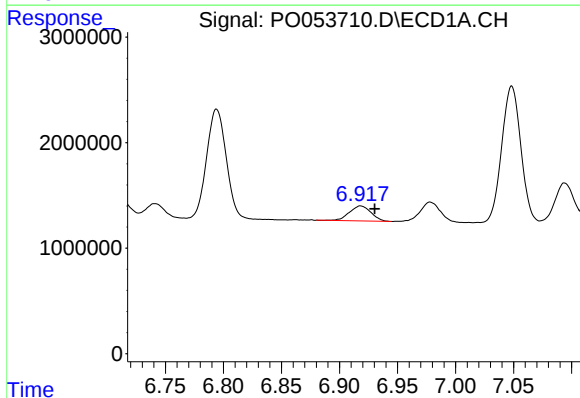


#29 AR-1254-4

R.T.: 6.918 min
Delta R.T.: -0.012 min
Response: 1843090
Conc: 36.16 ng/ml

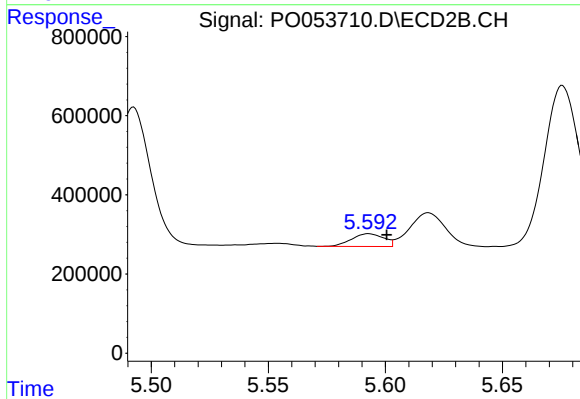

#29 AR-1254-4


R.T.: 5.593 min
Delta R.T.: -0.008 min
Response: 309523
Conc: 21.81 ng/ml

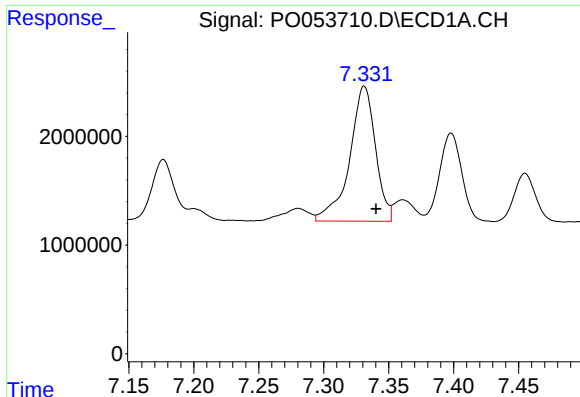

#30 AR-1254-5


R.T.: 7.331 min
Delta R.T.: -0.009 min
Response: 17233551
Conc: 360.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

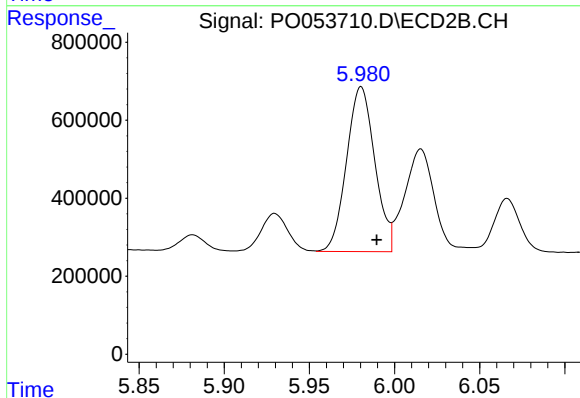


#30 AR-1254-5

R.T.: 5.980 min
Delta R.T.: -0.009 min
Response: 4877829
Conc: 261.13 ng/ml

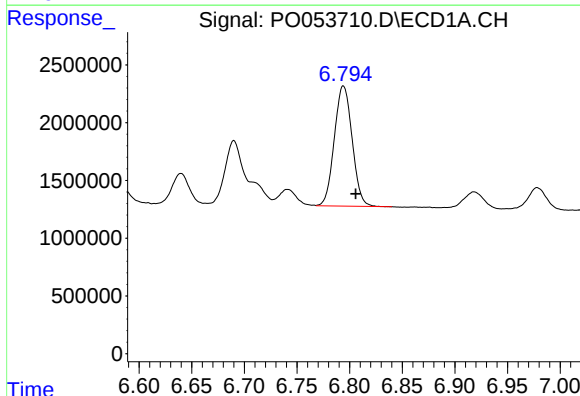


#31 AR-1260-1

R.T.: 6.794 min
Delta R.T.: -0.012 min
Response: 12271013
Conc: 251.74 ng/ml

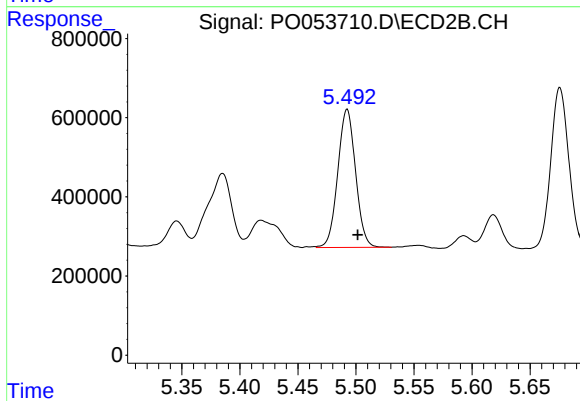

#31 AR-1260-1


R.T.: 5.492 min
Delta R.T.: -0.009 min
Response: 3722839
Conc: 244.49 ng/ml

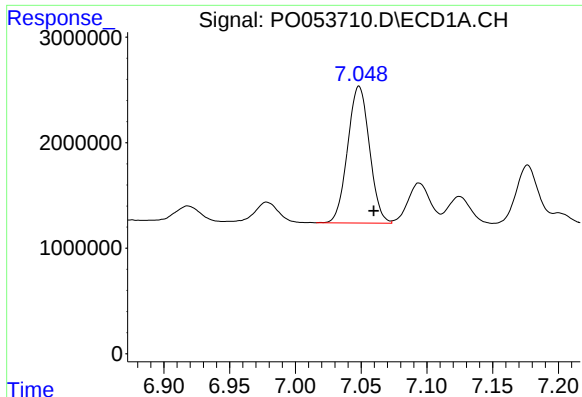

#32 AR-1260-2


R.T.: 7.048 min
Delta R.T.: -0.011 min
Response: 14974780
Conc: 240.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

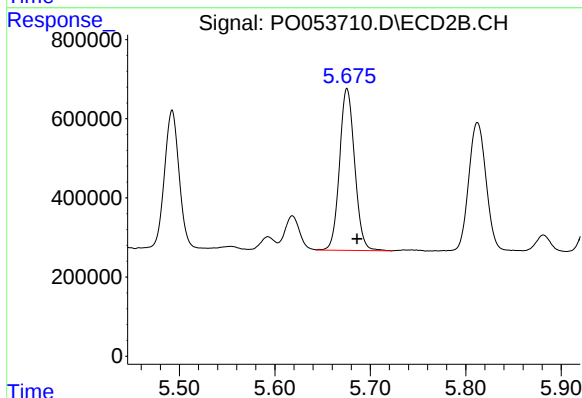


#32 AR-1260-2

R.T.: 5.676 min
Delta R.T.: -0.010 min
Response: 4499517
Conc: 242.67 ng/ml

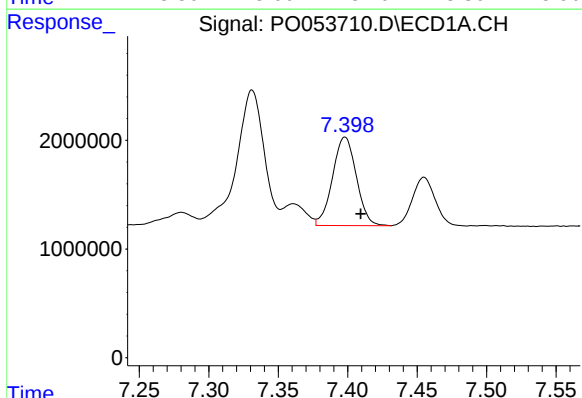


#33 AR-1260-3

R.T.: 7.398 min
Delta R.T.: -0.011 min
Response: 9715103
Conc: 248.36 ng/ml

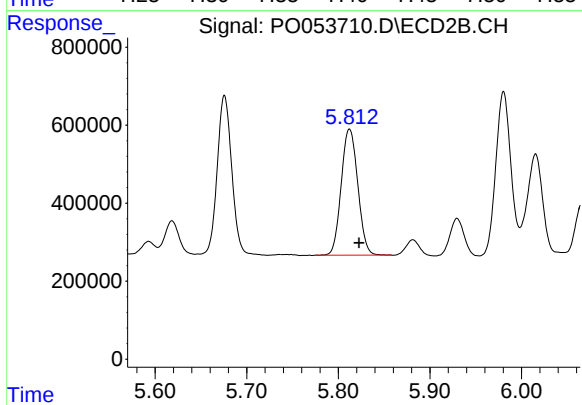

#33 AR-1260-3


R.T.: 5.812 min
Delta R.T.: -0.010 min
Response: 4067402
Conc: 237.93 ng/ml

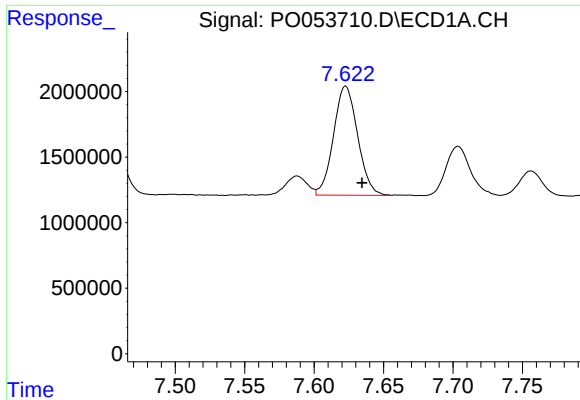

#34 AR-1260-4


R.T.: 7.623 min
Delta R.T.: -0.012 min
Response: 10072112
Conc: 233.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

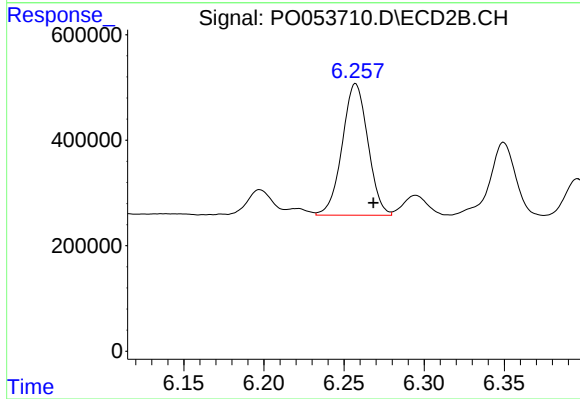


#34 AR-1260-4

R.T.: 6.257 min
Delta R.T.: -0.011 min
Response: 2785980
Conc: 252.99 ng/ml

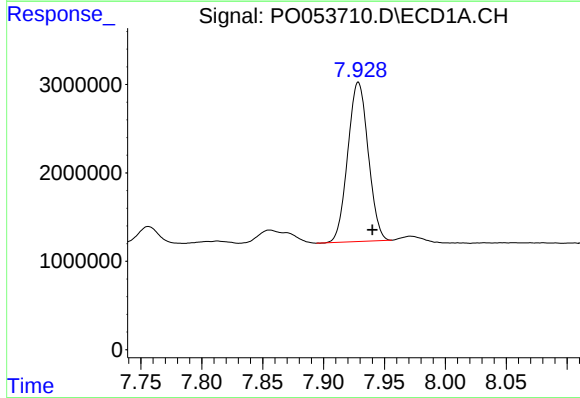


#35 AR-1260-5

R.T.: 7.929 min
Delta R.T.: -0.011 min
Response: 21068811
Conc: 231.45 ng/ml

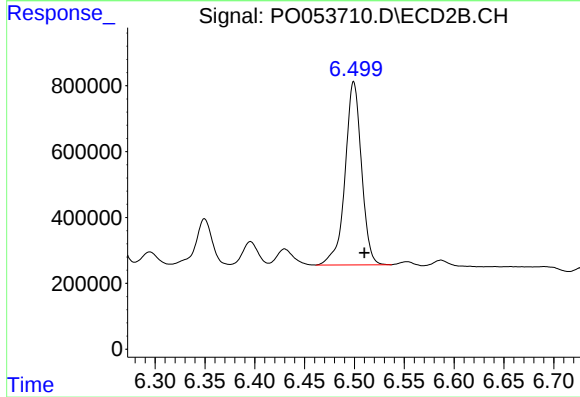

#35 AR-1260-5


R.T.: 6.499 min
Delta R.T.: -0.011 min
Response: 6380970
Conc: 234.33 ng/ml

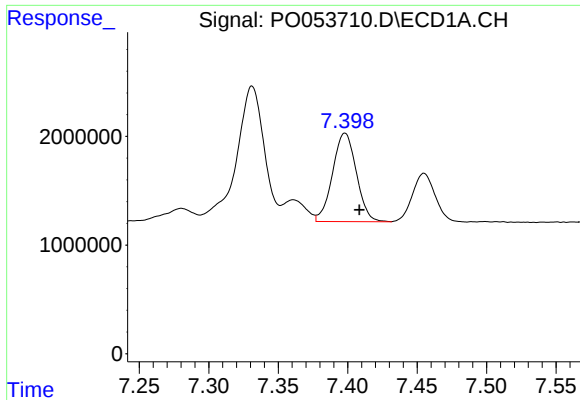

#36 AR-1262-1


R.T.: 7.398 min
Delta R.T.: -0.010 min
Response: 9715103
Conc: 141.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

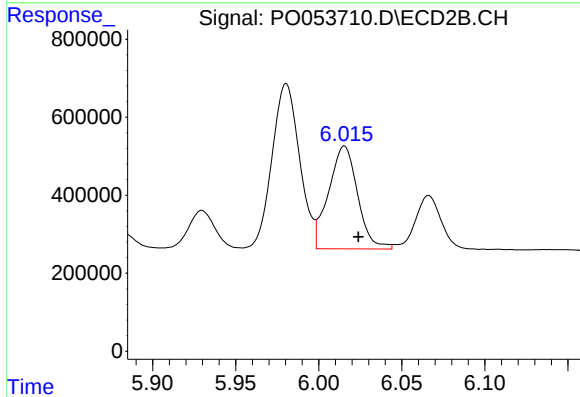


#36 AR-1262-1

R.T.: 6.015 min
Delta R.T.: -0.008 min
Response: 3205274
Conc: 161.85 ng/ml

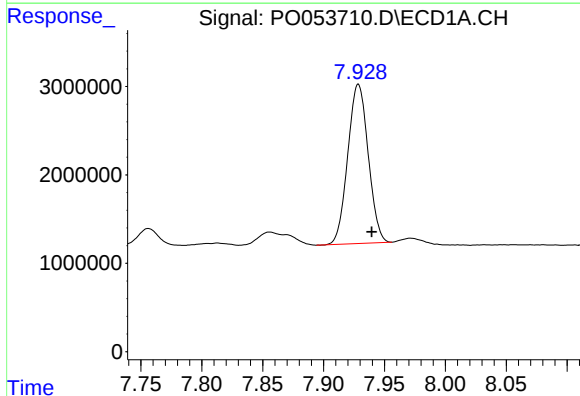


#37 AR-1262-2

R.T.: 7.929 min
Delta R.T.: -0.011 min
Response: 21068811
Conc: 174.86 ng/ml

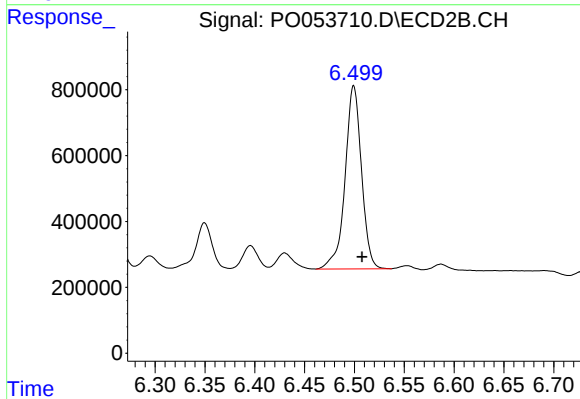

#37 AR-1262-2


R.T.: 6.499 min
Delta R.T.: -0.008 min
Response: 6380970
Conc: 187.89 ng/ml

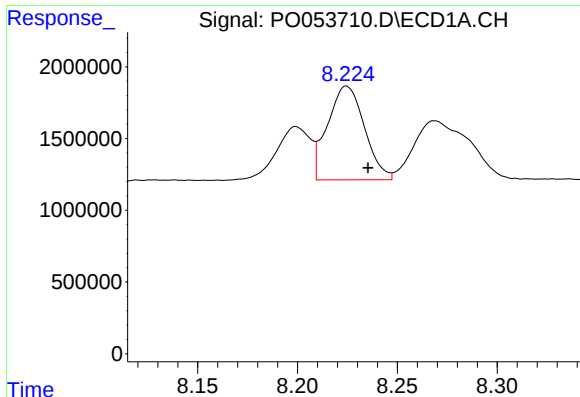

#38 AR-1262-3


R.T.: 8.225 min
Delta R.T.: -0.011 min
Response: 8401198
Conc: 340.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

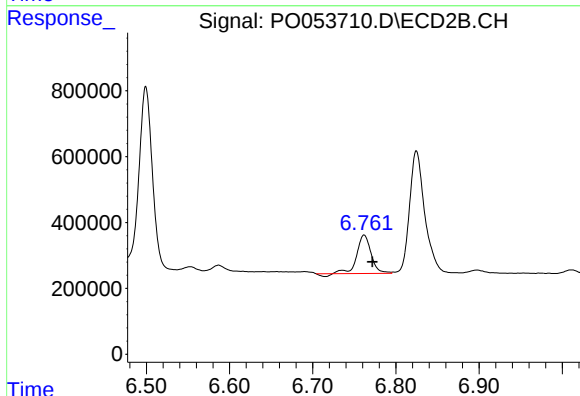


#38 AR-1262-3

R.T.: 6.762 min
Delta R.T.: -0.010 min
Response: 1377336
Conc: 105.95 ng/ml

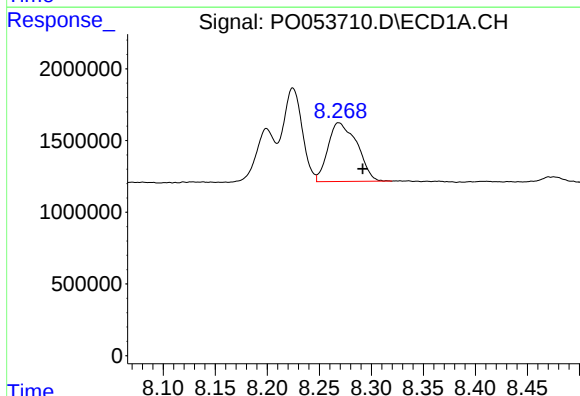


#39 AR-1262-4

R.T.: 8.269 min
Delta R.T.: -0.023 min
Response: 7948096
Conc: 128.22 ng/ml

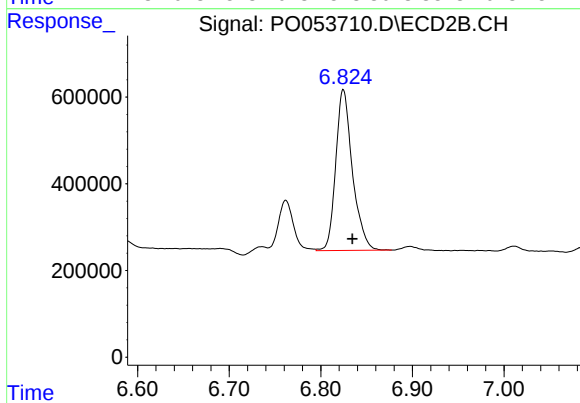

#39 AR-1262-4


R.T.: 6.825 min
Delta R.T.: -0.010 min
Response: 4704302
Conc: 192.20 ng/ml

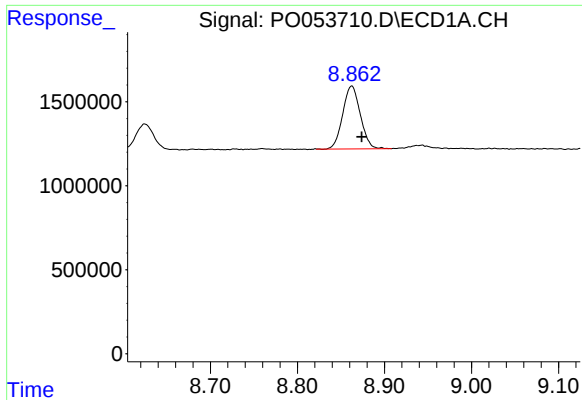

#40 AR-1262-5


R.T.: 8.862 min
Delta R.T.: -0.012 min
Response: 5261553
Conc: 124.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

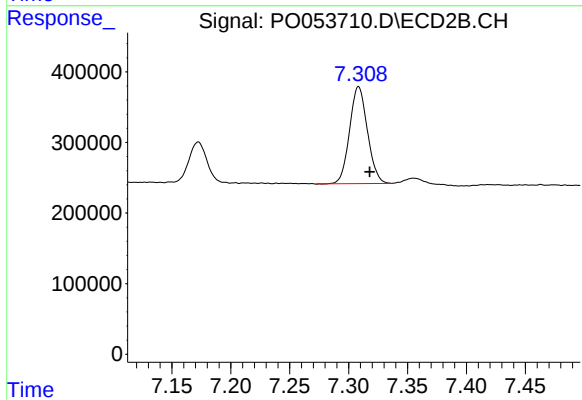


#40 AR-1262-5

R.T.: 7.309 min
Delta R.T.: -0.010 min
Response: 1449108
Conc: 129.63 ng/ml

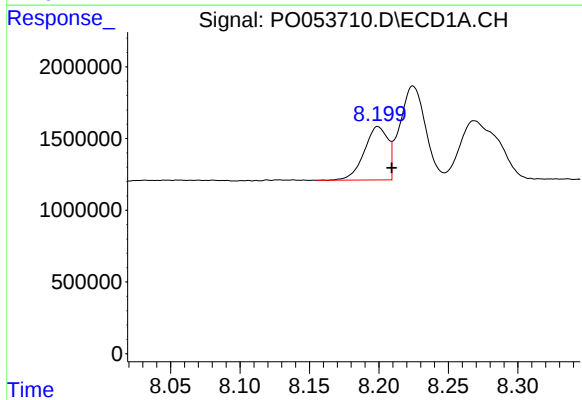


#41 AR-1268-1

R.T.: 8.199 min
Delta R.T.: -0.010 min
Response: 4413426
Conc: 29.79 ng/ml

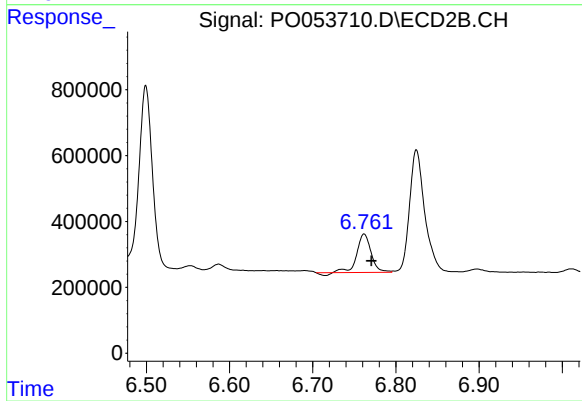

#41 AR-1268-1


R.T.: 6.762 min
Delta R.T.: -0.009 min
Response: 1377336
Conc: 35.67 ng/ml

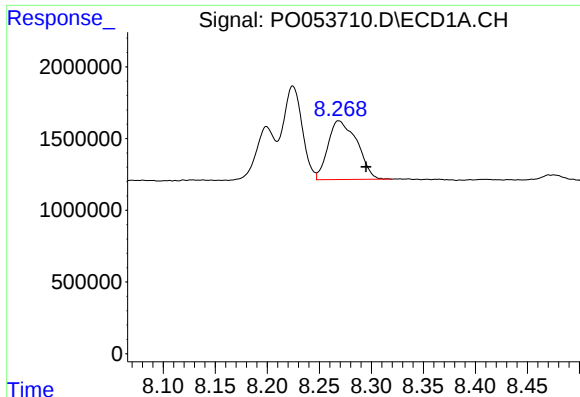

#42 AR-1268-2


R.T.: 8.269 min
Delta R.T.: -0.026 min
Response: 7948096
Conc: 56.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

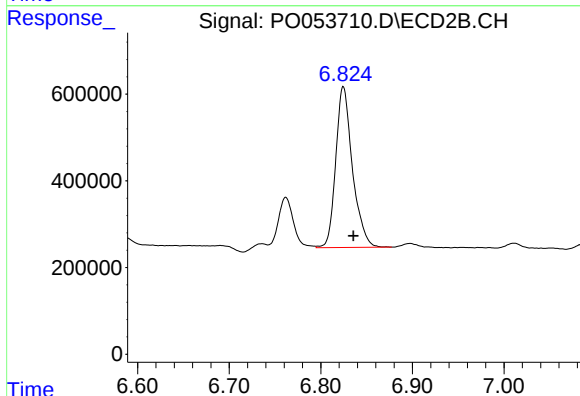


#42 AR-1268-2

R.T.: 6.825 min
Delta R.T.: -0.011 min
Response: 4704302
Conc: 128.65 ng/ml

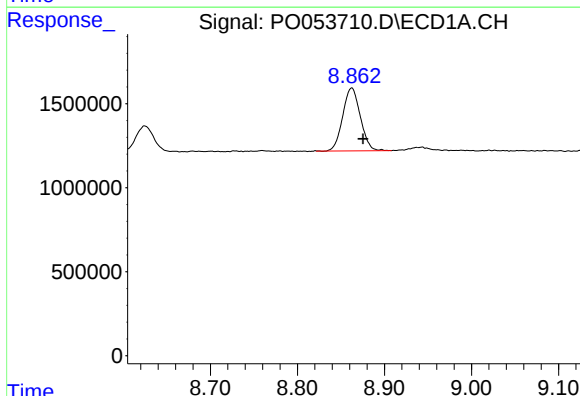


#44 AR-1268-4

R.T.: 8.862 min
Delta R.T.: -0.013 min
Response: 5261553
Conc: 110.68 ng/ml

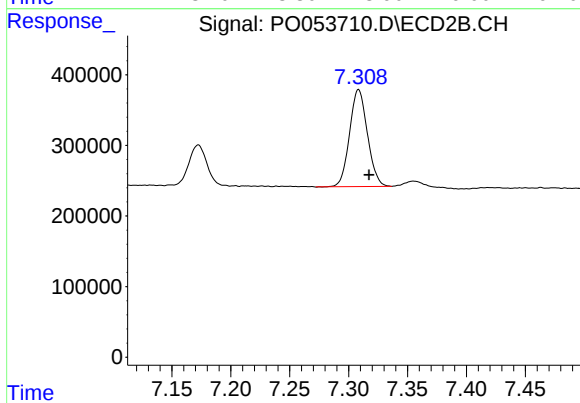

#44 AR-1268-4


R.T.: 7.309 min
Delta R.T.: -0.009 min
Response: 1449108
Conc: 116.36 ng/ml

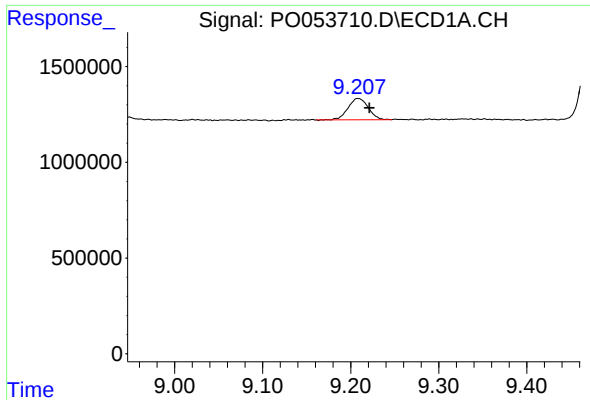

#45 AR-1268-5

R.T.: 9.208 min
Delta R.T.: -0.013 min
Response: 1779911
Conc: 4.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMS

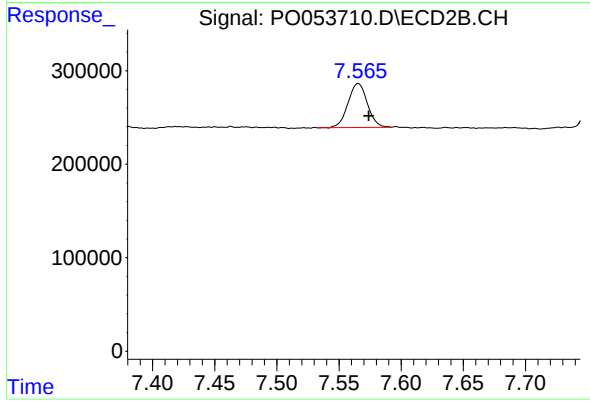

#45 AR-1268-5

R.T.: 7.566 min
Delta R.T.: -0.008 min
Response: 509577
Conc: 5.43 ng/ml