

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020419\
 Data File : P0053711.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2019 19:01
 Operator : SM/SJ
 Sample : K1362-01MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-005-ABCDMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 23:45:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.095	3.159	47431628	5146249	24.336	21.456
2)	SA Decachlor...	9.483	7.765	21024746	5499675	21.572	22.025
Target Compounds							
3)	L1 AR-1016-1	5.234	4.150	10830208	3723144	240.527	423.182 #
4)	L1 AR-1016-2	5.256	4.150	17656532	3723144	262.010	263.729
5)	L1 AR-1016-3	5.315	4.308	11454710	1980270	288.622	250.910
6)	L1 AR-1016-4	5.414	4.349	9341903	1492725	293.541	285.452
7)	L1 AR-1016-5	5.697	4.540	8351381	1950279	297.663	268.273
8)	L2 AR-1221-1	0.000	3.428	0	284658	N.D.	113.738 #
9)	L2 AR-1221-2	4.391	3.428	1938863	284658	162.001	159.555
10)	L2 AR-1221-3	4.465	3.496	7179796	1095083	182.289	173.900
11)	L3 AR-1232-1	4.465	3.496	7179796	1095083	223.562	204.503
12)	L3 AR-1232-2	4.974	4.150	9615078	3723144	631.997	586.251
13)	L3 AR-1232-3	5.256	4.308	17656532	1980270	602.640	561.174
14)	L3 AR-1232-4	5.414	4.385	9341903	1832315	659.946	715.967
15)	L3 AR-1232-5	5.497	4.540	7178949	1950279	895.933	620.287 #
16)	L4 AR-1242-1	5.234	4.136	10830208	2377326	299.570	320.197
17)	L4 AR-1242-2	5.256	4.150	17656532	3723144	334.220	324.907
18)	L4 AR-1242-3	5.315	4.308	11454710	1980270	358.640	321.286
19)	L4 AR-1242-4	5.414	4.385	9341903	1832315	361.145	343.746
20)	L4 AR-1242-5	0.000	4.861	0	1489432	N.D.	202.718 #
21)	L5 AR-1248-1	5.234	4.136	10830208	2377326	395.769	414.854
22)	L5 AR-1248-2	5.497	4.349	7178949	1492725	217.897	196.780
23)	L5 AR-1248-3	5.697	4.385	8351381	1832315	218.136	233.862
24)	L5 AR-1248-4	6.063	4.540	4718897	1950279	112.434	196.430 #
25)	L5 AR-1248-5	0.000	4.861	0	1489432	N.D.	143.843 #
26)	L6 AR-1254-1	6.063	4.861	4718897	1489432	112.234	91.452
27)	L6 AR-1254-2	6.275	5.001	5880412	1486499	90.092	107.777
28)	L6 AR-1254-3	6.639	5.385	2899730	2640448	42.354	120.797 #
29)	L6 AR-1254-4	6.918	5.592	1873318	313932	36.755	22.117 #
30)	L6 AR-1254-5	7.330	5.981	17172108	4932829	358.761	264.076 #
31)	L7 AR-1260-1	6.794	5.491	12277558	3771648	251.879	247.696
32)	L7 AR-1260-2	7.048	5.676	15078194	4536699	242.630	244.677
33)	L7 AR-1260-3	7.398	5.812	9708270	4118817	248.185	240.941
34)	L7 AR-1260-4	7.623	6.258	10105844	2804141	233.869	254.637
35)	L7 AR-1260-5	7.929	6.500	21245381	6453533	233.389	236.992
36)	L8 AR-1262-1	7.398	6.015	9708270	3243684	141.494	163.785
37)	L8 AR-1262-2	7.929	6.500	21245381	6453533	176.330	190.027
38)	L8 AR-1262-3	8.224	6.763	8348523	1377398	338.533	105.952 #
39)	L8 AR-1262-4	8.268	6.825	7930349	4738506	127.934	193.597 #
40)	L8 AR-1262-5	8.861	7.310	5352523	1448715	126.729	129.597
41)	L9 AR-1268-1	8.198	6.763	4396325	1377398	29.671	35.672

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020419\
 Data File : P0053711.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Feb 2019 19:01
 Operator : SM/SJ
 Sample : K1362-01MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-03-005-ABCDMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 23:45:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 01 08:56:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.268	6.825	7930349	4738506	56.505	129.580 #
44) L9	AR-1268-4	8.861	7.310	5352523	1448715	112.590	116.326
45) L9	AR-1268-5	9.207	7.565	1804713	528023	4.813	5.629



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020419\
Data File : P0053711.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2019 19:01
Operator : SM/SJ
Sample : K1362-01MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 23:45:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

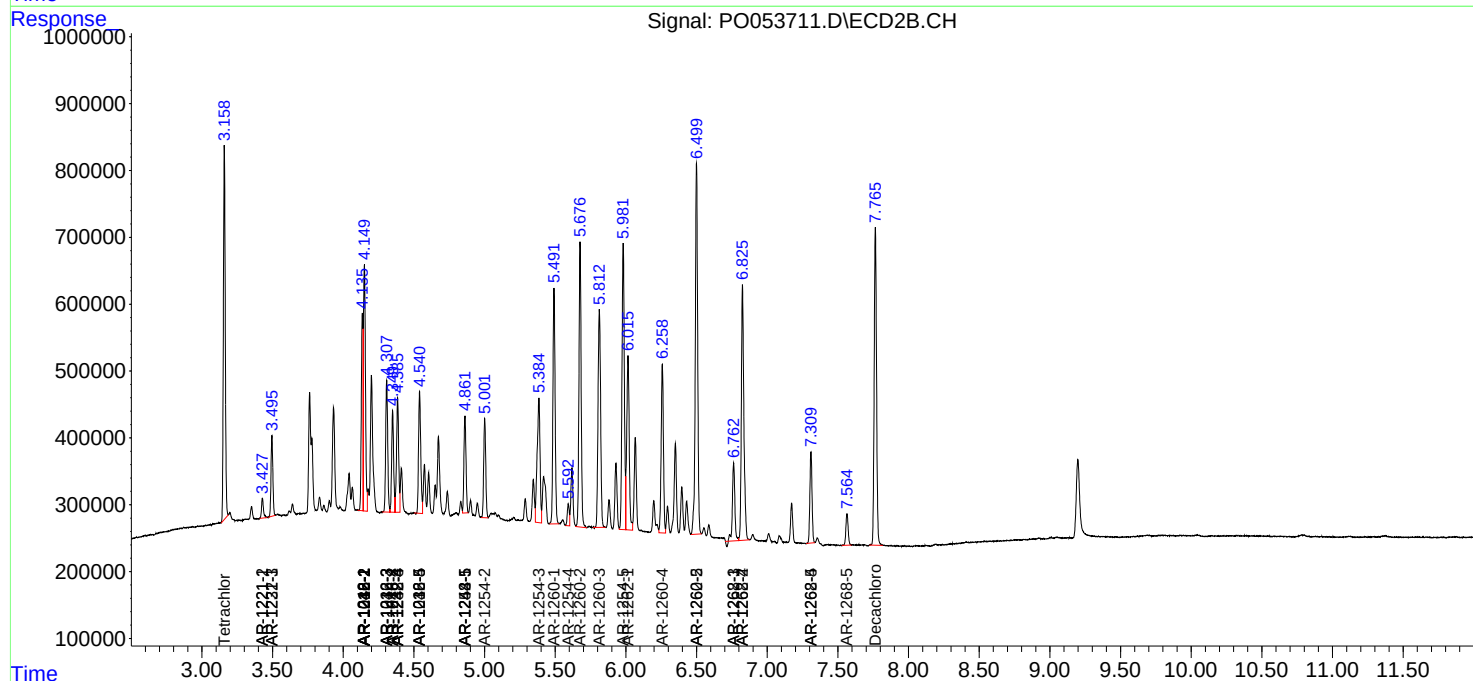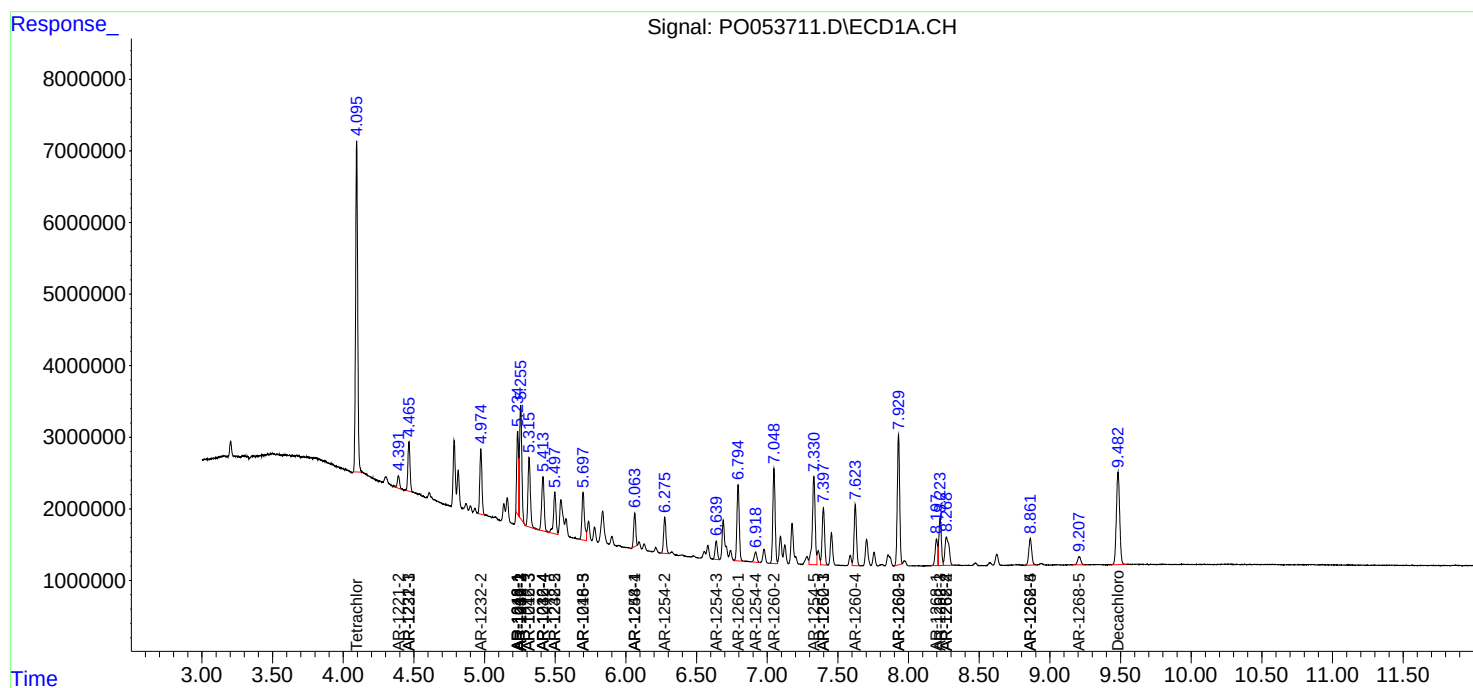


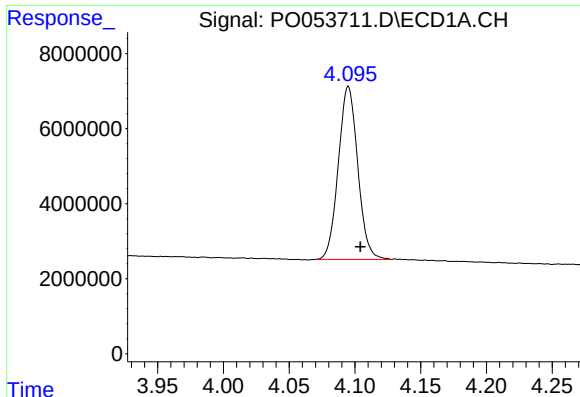

#1 Tetrachloro-m-xylene


R.T.: 4.095 min
Delta R.T.: -0.009 min
Response: 47431628
Conc: 24.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

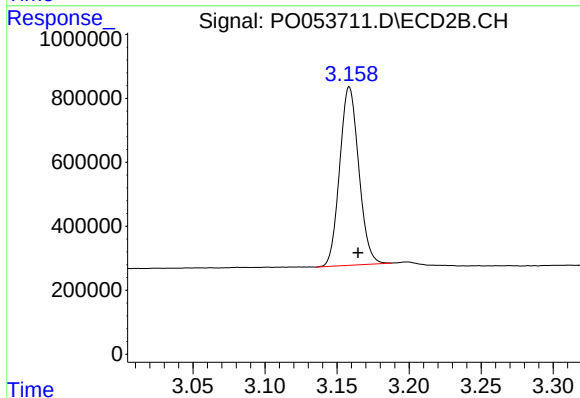


#1 Tetrachloro-m-xylene

R.T.: 3.159 min
Delta R.T.: -0.006 min
Response: 5146249
Conc: 21.46 ng/ml

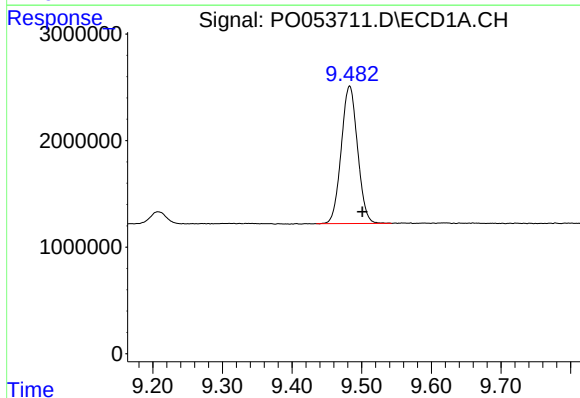


#2 Decachlorobiphenyl

R.T.: 9.483 min
Delta R.T.: -0.018 min
Response: 21024746
Conc: 21.57 ng/ml

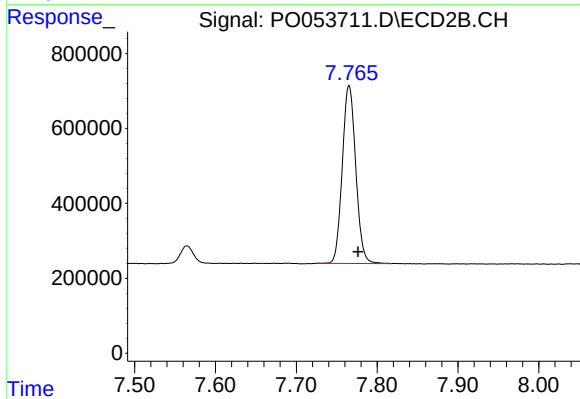

#2 Decachlorobiphenyl


R.T.: 7.765 min
Delta R.T.: -0.011 min
Response: 5499675
Conc: 22.03 ng/ml

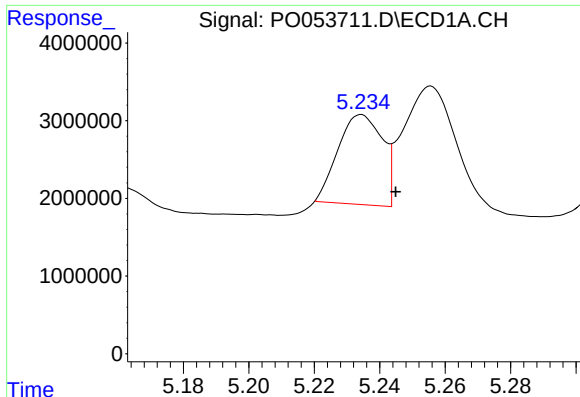

#3 AR-1016-1


R.T.: 5.234 min
Delta R.T.: -0.010 min
Response: 10830208
Conc: 240.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

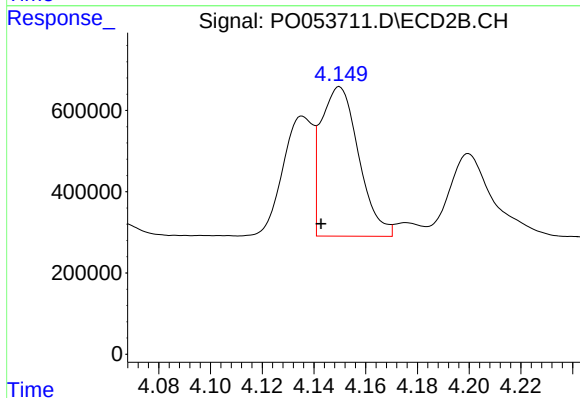


#3 AR-1016-1

R.T.: 4.150 min
Delta R.T.: 0.007 min
Response: 3723144
Conc: 423.18 ng/ml

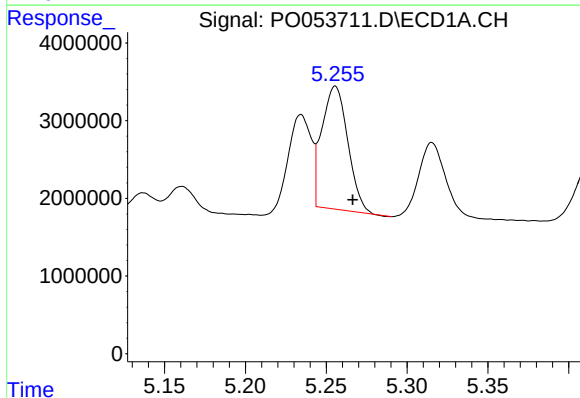


#4 AR-1016-2

R.T.: 5.256 min
Delta R.T.: -0.011 min
Response: 17656532
Conc: 262.01 ng/ml

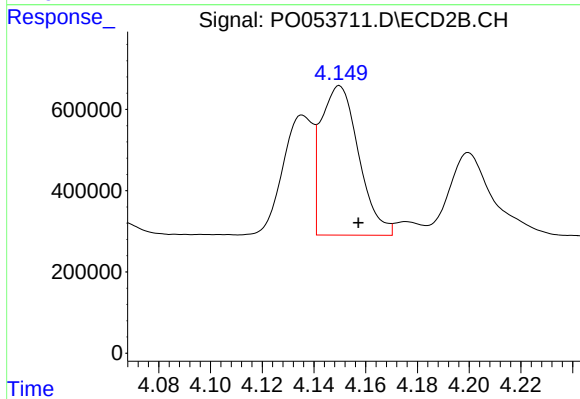

#4 AR-1016-2


R.T.: 4.150 min
Delta R.T.: -0.007 min
Response: 3723144
Conc: 263.73 ng/ml

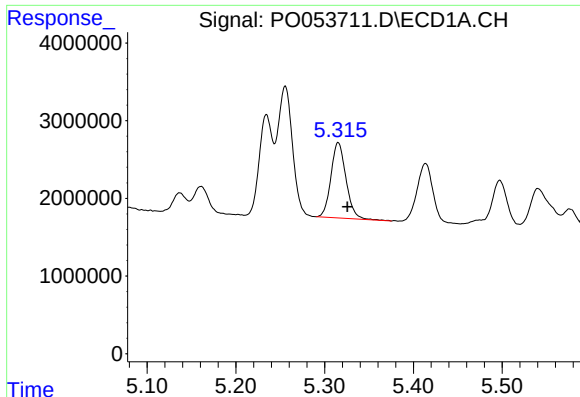

#5 AR-1016-3


R.T.: 5.315 min
Delta R.T.: -0.010 min
Response: 11454710
Conc: 288.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

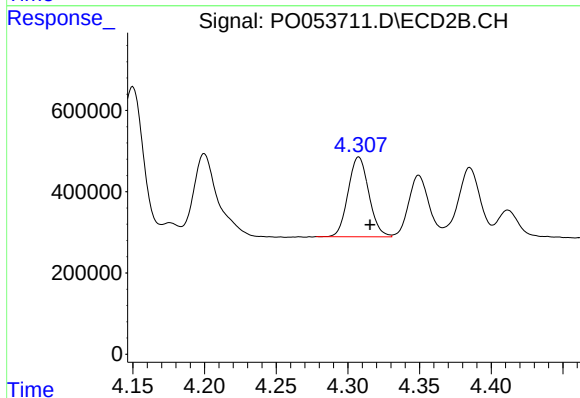


#5 AR-1016-3

R.T.: 4.308 min
Delta R.T.: -0.008 min
Response: 1980270
Conc: 250.91 ng/ml

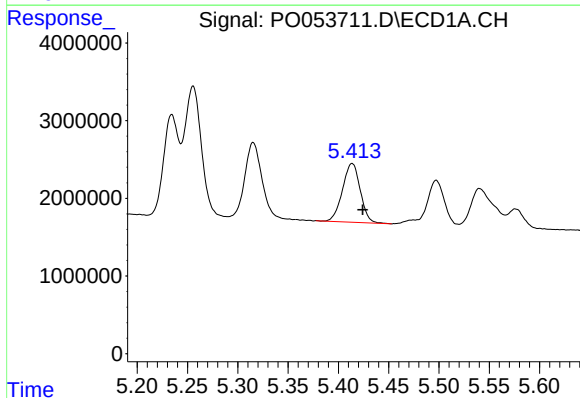


#6 AR-1016-4

R.T.: 5.414 min
Delta R.T.: -0.011 min
Response: 9341903
Conc: 293.54 ng/ml

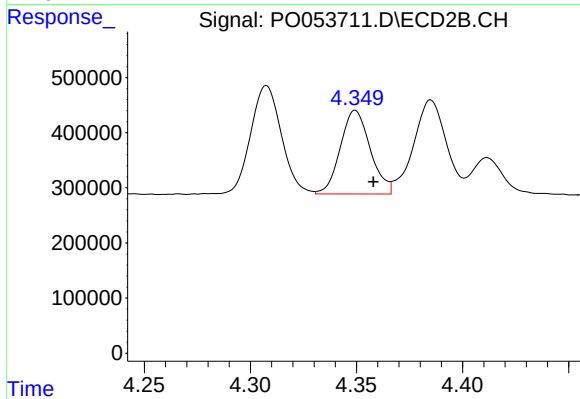

#6 AR-1016-4


R.T.: 4.349 min
Delta R.T.: -0.009 min
Response: 1492725
Conc: 285.45 ng/ml

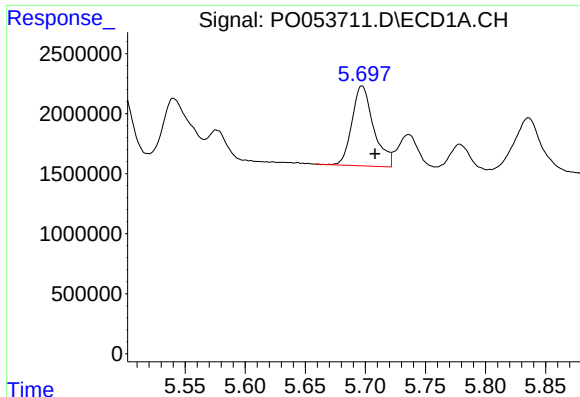

#7 AR-1016-5


R.T.: 5.697 min
Delta R.T.: -0.011 min
Response: 8351381
Conc: 297.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

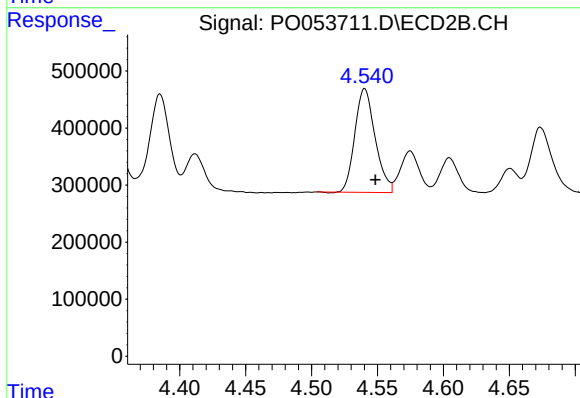


#7 AR-1016-5

R.T.: 4.540 min
Delta R.T.: -0.008 min
Response: 1950279
Conc: 268.27 ng/ml

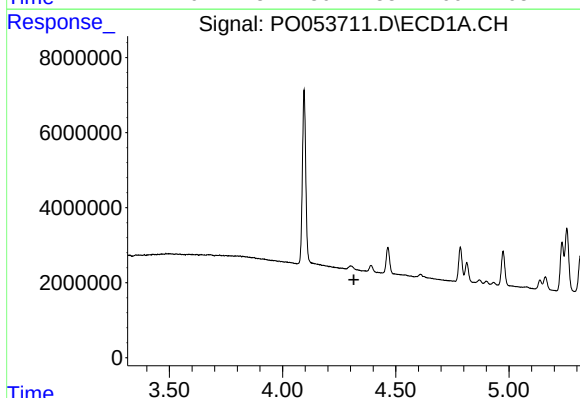


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.315 min
Response: 0
Conc: N.D.

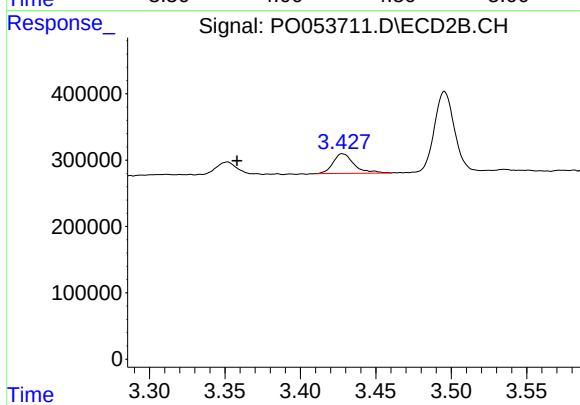

#8 AR-1221-1


R.T.: 3.428 min
Delta R.T.: 0.070 min
Response: 284658
Conc: 113.74 ng/ml

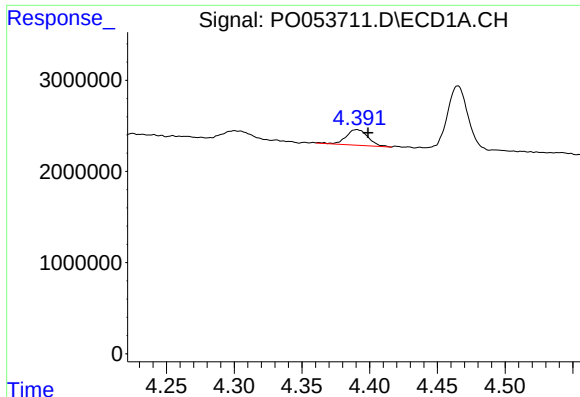

#9 AR-1221-2


R.T.: 4.391 min
Delta R.T.: -0.008 min
Response: 1938863
Conc: 162.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

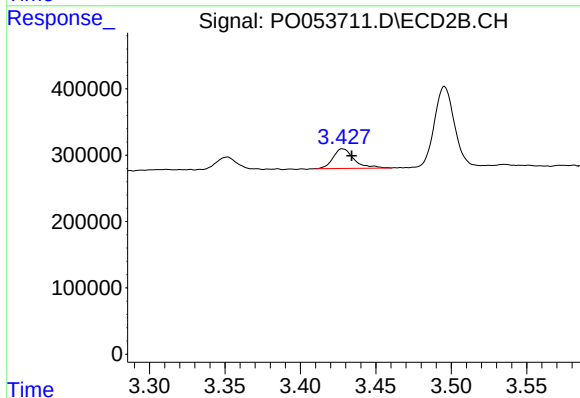


#9 AR-1221-2

R.T.: 3.428 min
Delta R.T.: -0.006 min
Response: 284658
Conc: 159.56 ng/ml

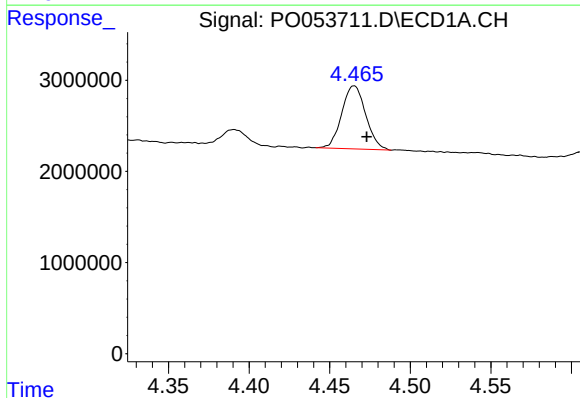


#10 AR-1221-3

R.T.: 4.465 min
Delta R.T.: -0.008 min
Response: 7179796
Conc: 182.29 ng/ml

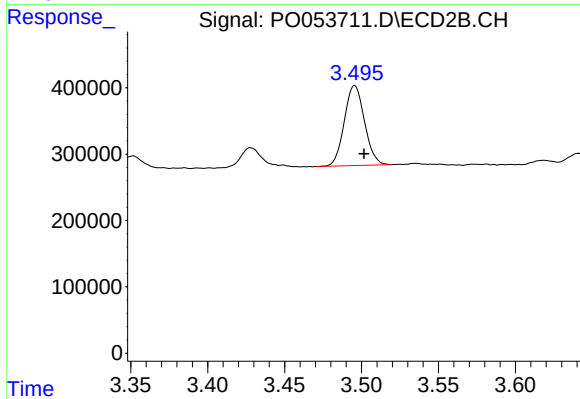

#10 AR-1221-3


R.T.: 3.496 min
Delta R.T.: -0.006 min
Response: 1095083
Conc: 173.90 ng/ml

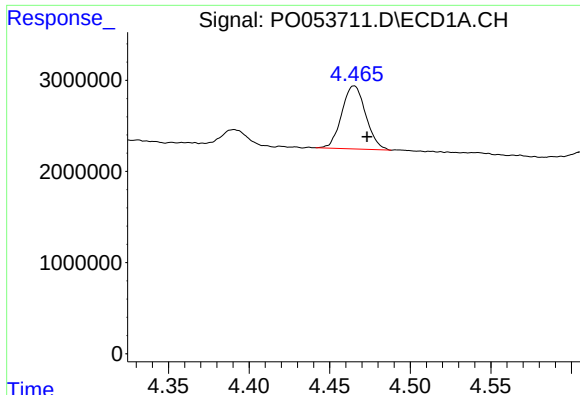

#11 AR-1232-1


R.T.: 4.465 min
Delta R.T.: -0.008 min
Response: 7179796
Conc: 223.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

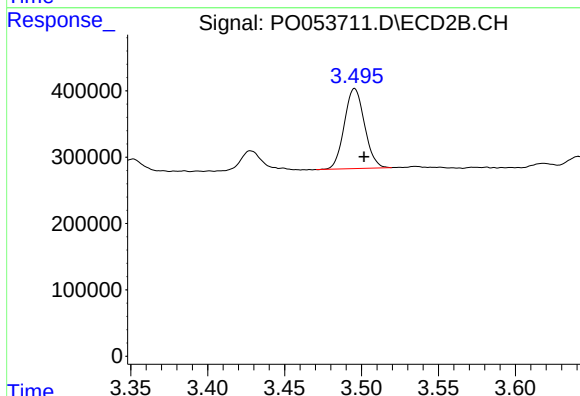


#11 AR-1232-1

R.T.: 3.496 min
Delta R.T.: -0.006 min
Response: 1095083
Conc: 204.50 ng/ml

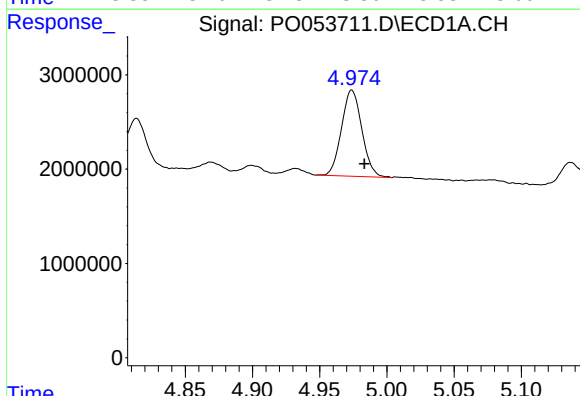


#12 AR-1232-2

R.T.: 4.974 min
Delta R.T.: -0.009 min
Response: 9615078
Conc: 632.00 ng/ml

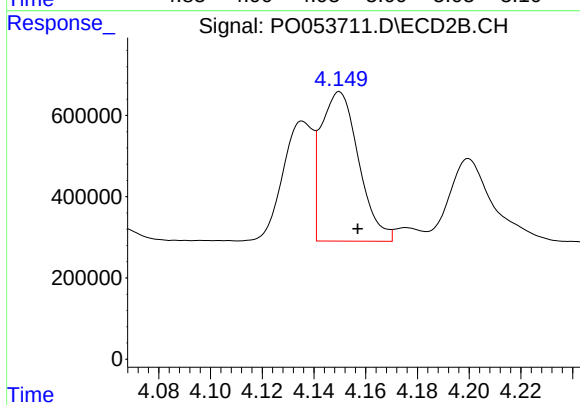

#12 AR-1232-2


R.T.: 4.150 min
Delta R.T.: -0.007 min
Response: 3723144
Conc: 586.25 ng/ml

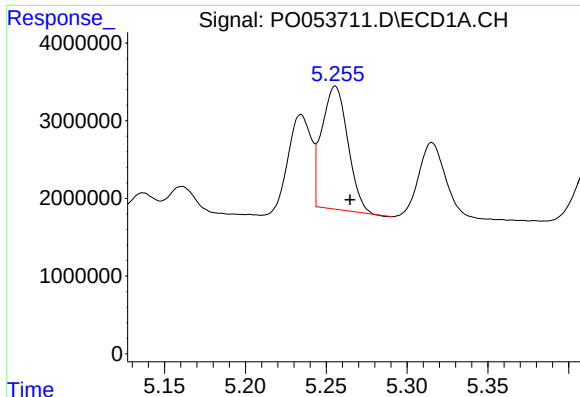

#13 AR-1232-3


R.T.: 5.256 min
Delta R.T.: -0.009 min
Response: 17656532
Conc: 602.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

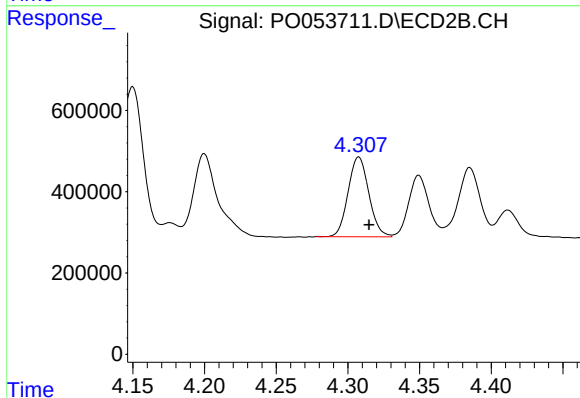


#13 AR-1232-3

R.T.: 4.308 min
Delta R.T.: -0.007 min
Response: 1980270
Conc: 561.17 ng/ml

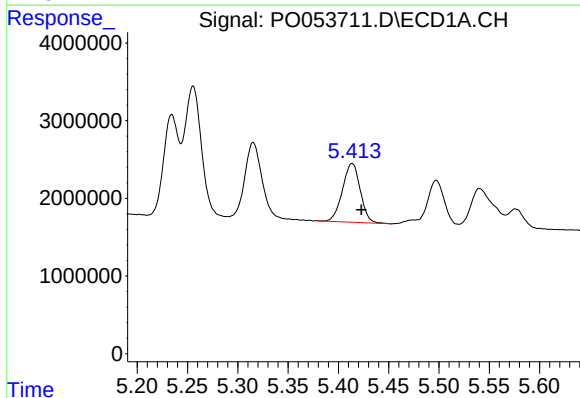


#14 AR-1232-4

R.T.: 5.414 min
Delta R.T.: -0.009 min
Response: 9341903
Conc: 659.95 ng/ml

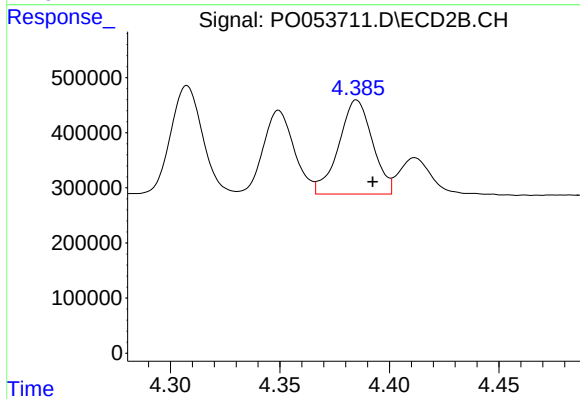

#14 AR-1232-4


R.T.: 4.385 min
Delta R.T.: -0.007 min
Response: 1832315
Conc: 715.97 ng/ml

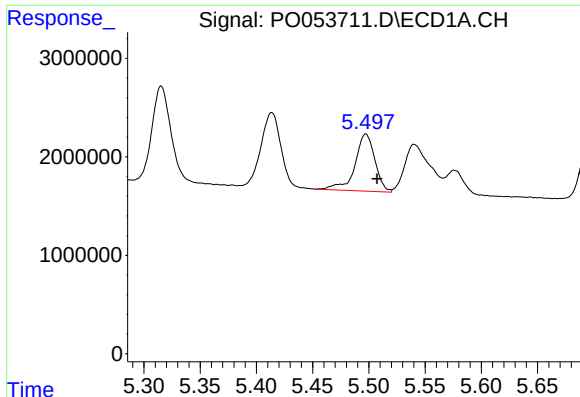

#15 AR-1232-5


R.T.: 5.497 min
Delta R.T.: -0.010 min
Response: 7178949
Conc: 895.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

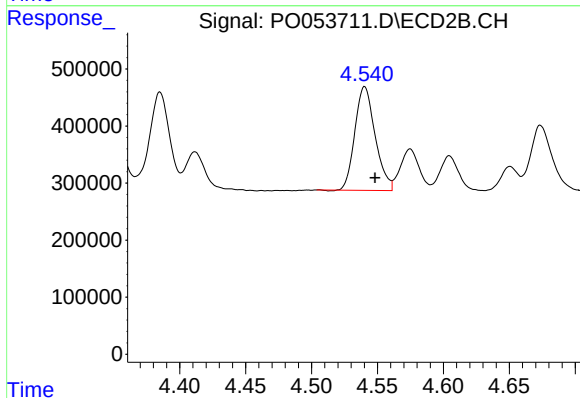


#15 AR-1232-5

R.T.: 4.540 min
Delta R.T.: -0.008 min
Response: 1950279
Conc: 620.29 ng/ml

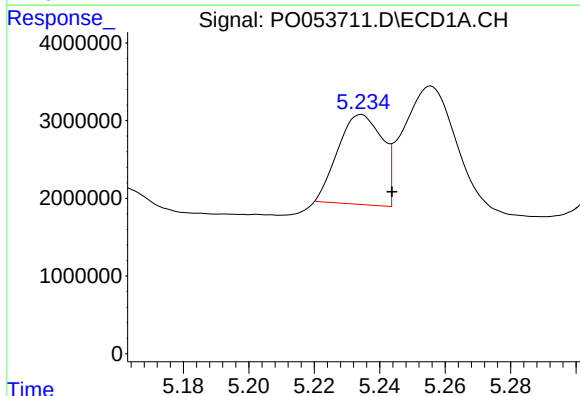


#16 AR-1242-1

R.T.: 5.234 min
Delta R.T.: -0.009 min
Response: 10830208
Conc: 299.57 ng/ml

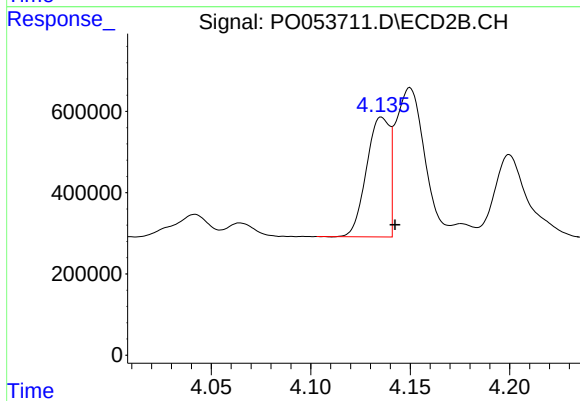

#16 AR-1242-1


R.T.: 4.136 min
Delta R.T.: -0.007 min
Response: 2377326
Conc: 320.20 ng/ml

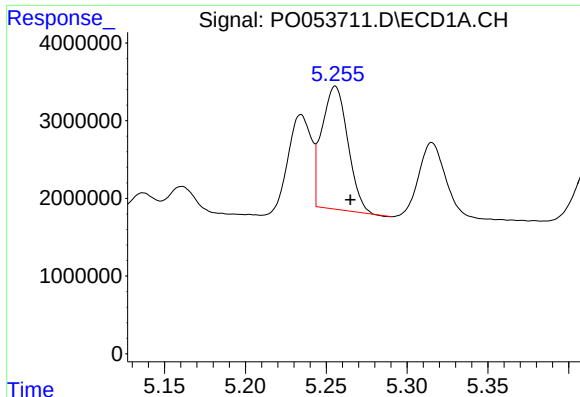

#17 AR-1242-2


R.T.: 5.256 min
Delta R.T.: -0.009 min
Response: 17656532
Conc: 334.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

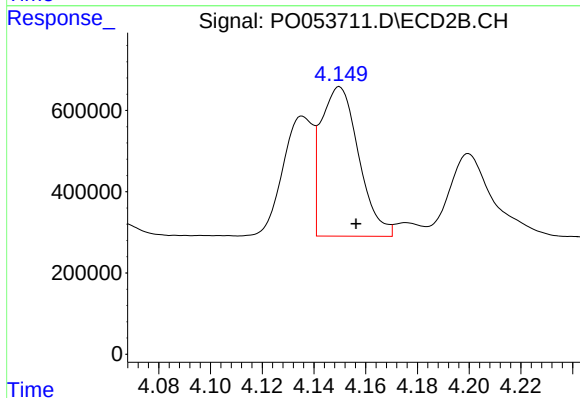


#17 AR-1242-2

R.T.: 4.150 min
Delta R.T.: -0.006 min
Response: 3723144
Conc: 324.91 ng/ml

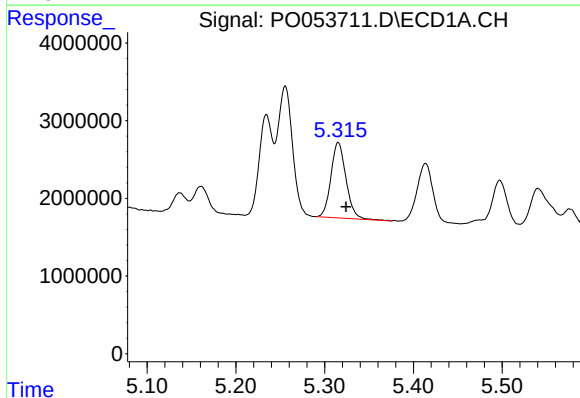


#18 AR-1242-3

R.T.: 5.315 min
Delta R.T.: -0.009 min
Response: 11454710
Conc: 358.64 ng/ml

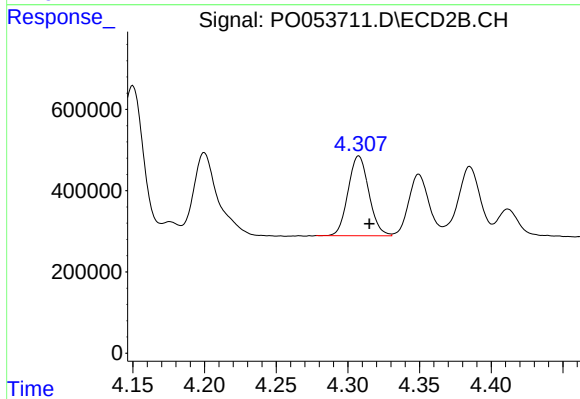

#18 AR-1242-3


R.T.: 4.308 min
Delta R.T.: -0.008 min
Response: 1980270
Conc: 321.29 ng/ml

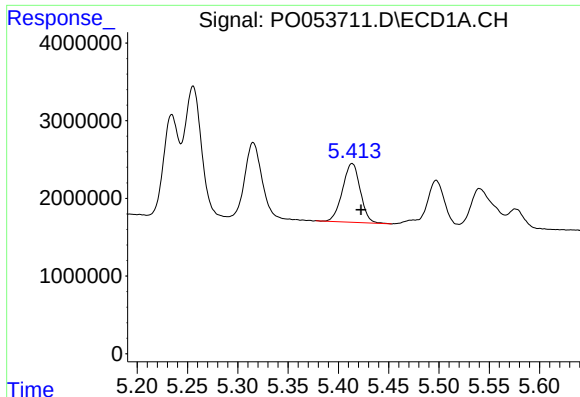

#19 AR-1242-4


R.T.: 5.414 min
Delta R.T.: -0.009 min
Response: 9341903
Conc: 361.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

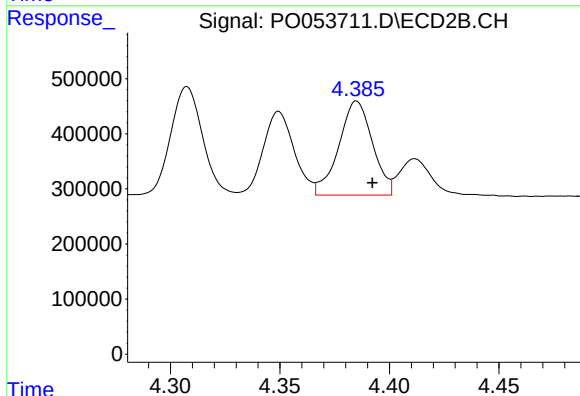


#19 AR-1242-4

R.T.: 4.385 min
Delta R.T.: -0.007 min
Response: 1832315
Conc: 343.75 ng/ml

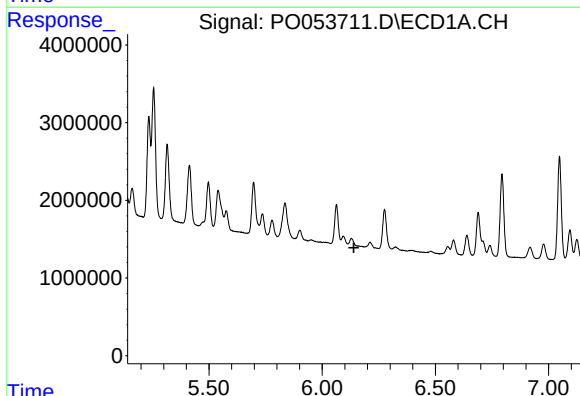


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 6.140 min
Response: 0
Conc: N.D.

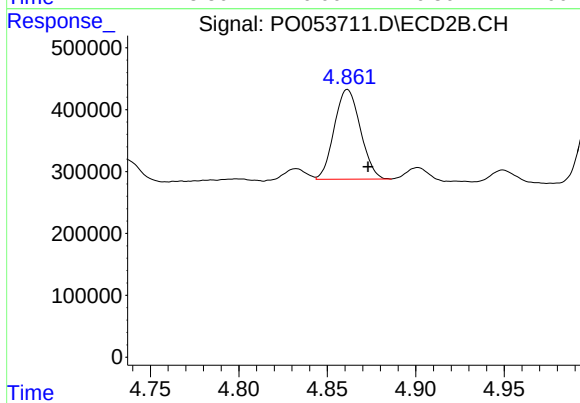

#20 AR-1242-5


R.T.: 4.861 min
Delta R.T.: -0.012 min
Response: 1489432
Conc: 202.72 ng/ml

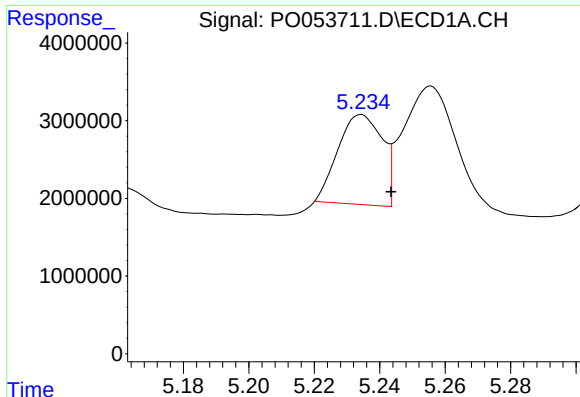

#21 AR-1248-1


R.T.: 5.234 min
Delta R.T.: -0.009 min
Response: 10830208
Conc: 395.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

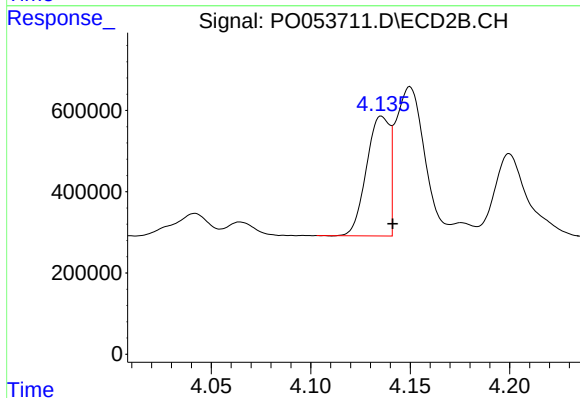


#21 AR-1248-1

R.T.: 4.136 min
Delta R.T.: -0.006 min
Response: 2377326
Conc: 414.85 ng/ml

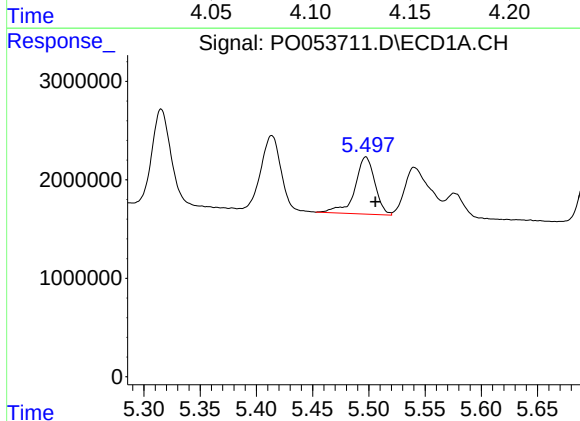


#22 AR-1248-2

R.T.: 5.497 min
Delta R.T.: -0.009 min
Response: 7178949
Conc: 217.90 ng/ml

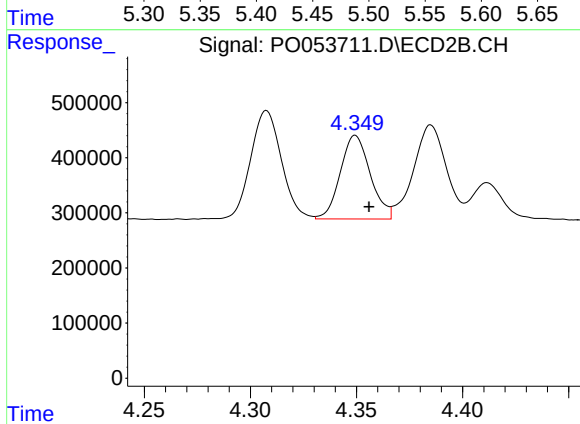

#22 AR-1248-2


R.T.: 4.349 min
Delta R.T.: -0.007 min
Response: 1492725
Conc: 196.78 ng/ml

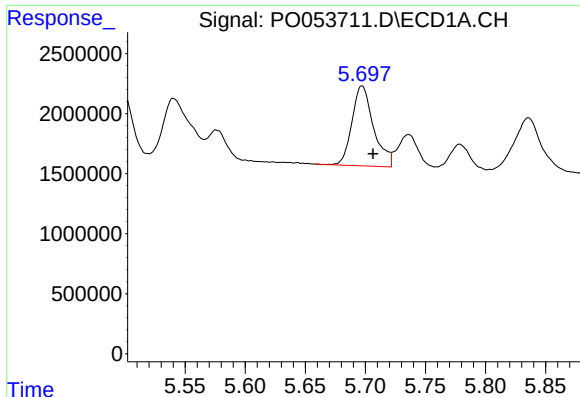

#23 AR-1248-3


R.T.: 5.697 min
Delta R.T.: -0.009 min
Response: 8351381
Conc: 218.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

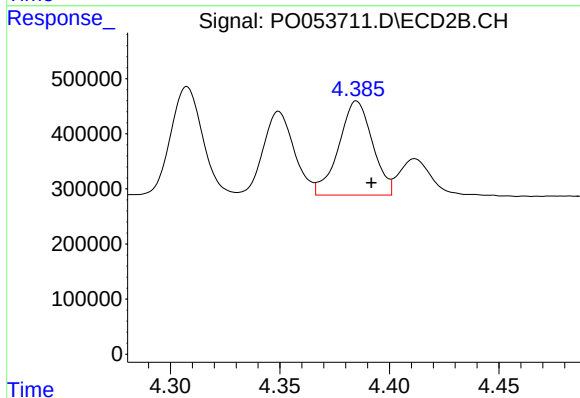


#23 AR-1248-3

R.T.: 4.385 min
Delta R.T.: -0.007 min
Response: 1832315
Conc: 233.86 ng/ml

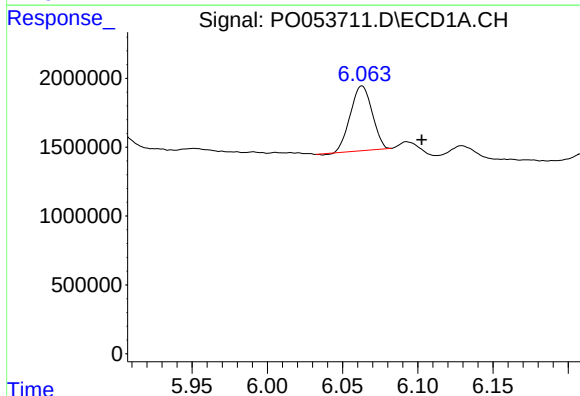


#24 AR-1248-4

R.T.: 6.063 min
Delta R.T.: -0.040 min
Response: 4718897
Conc: 112.43 ng/ml

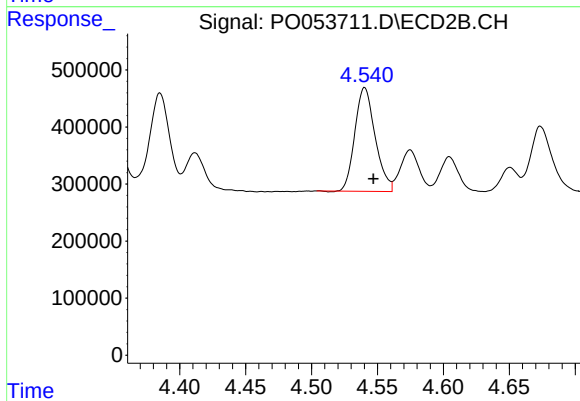

#24 AR-1248-4


R.T.: 4.540 min
Delta R.T.: -0.007 min
Response: 1950279
Conc: 196.43 ng/ml

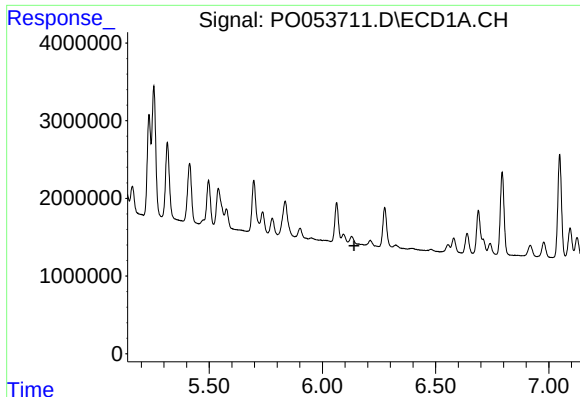

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.140 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

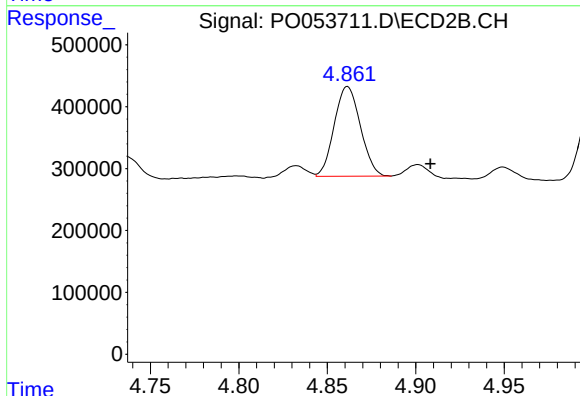


#25 AR-1248-5

R.T.: 4.861 min
Delta R.T.: -0.047 min
Response: 1489432
Conc: 143.84 ng/ml

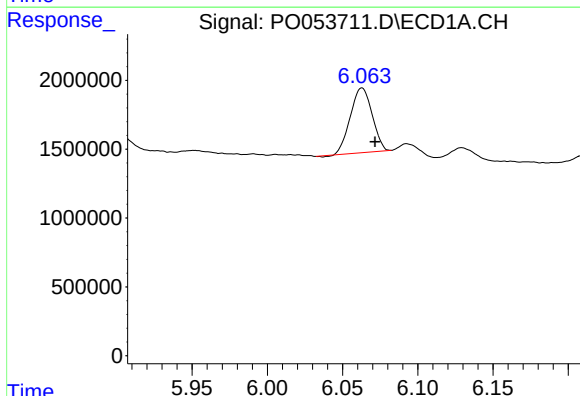


#26 AR-1254-1

R.T.: 6.063 min
Delta R.T.: -0.009 min
Response: 4718897
Conc: 112.23 ng/ml

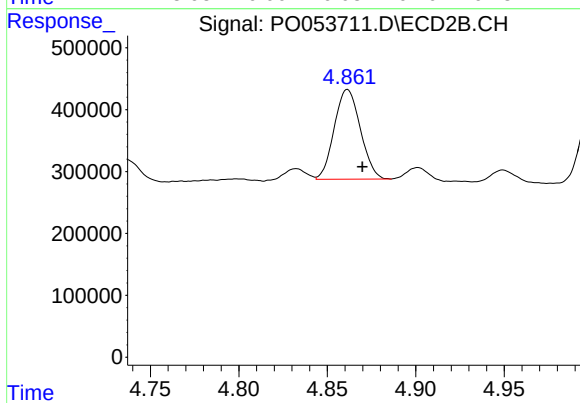

#26 AR-1254-1


R.T.: 4.861 min
Delta R.T.: -0.008 min
Response: 1489432
Conc: 91.45 ng/ml

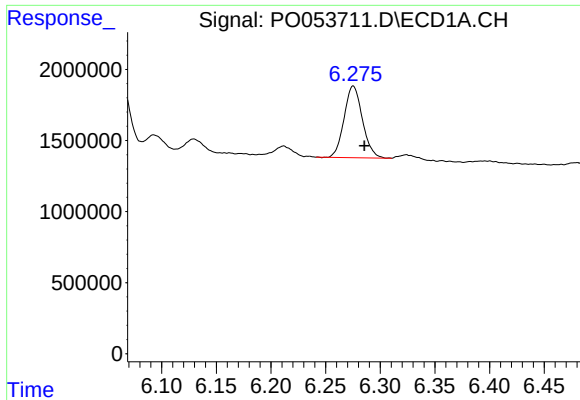

#27 AR-1254-2


R.T.: 6.275 min
Delta R.T.: -0.010 min
Response: 5880412
Conc: 90.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

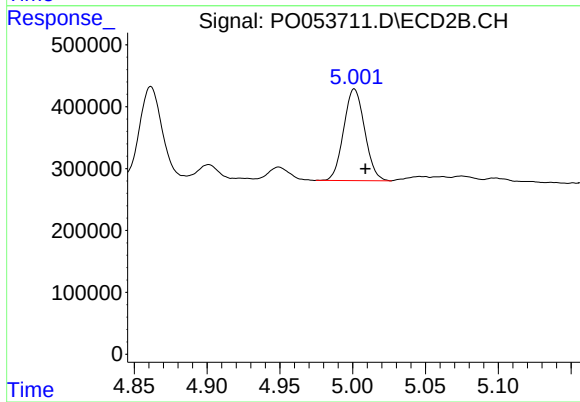


#27 AR-1254-2

R.T.: 5.001 min
Delta R.T.: -0.007 min
Response: 1486499
Conc: 107.78 ng/ml

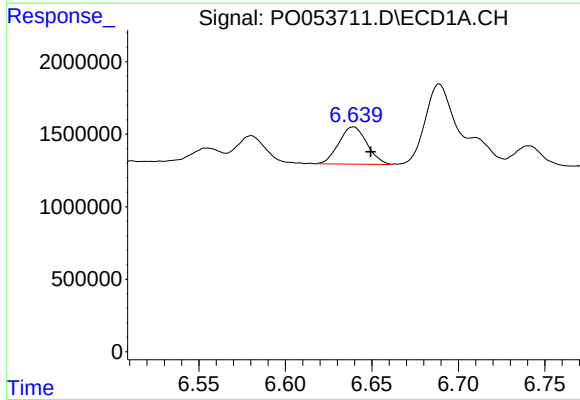


#28 AR-1254-3

R.T.: 6.639 min
Delta R.T.: -0.010 min
Response: 2899730
Conc: 42.35 ng/ml

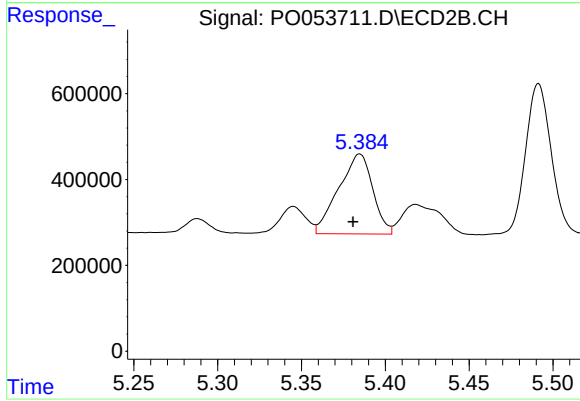

#28 AR-1254-3


R.T.: 5.385 min
Delta R.T.: 0.004 min
Response: 2640448
Conc: 120.80 ng/ml

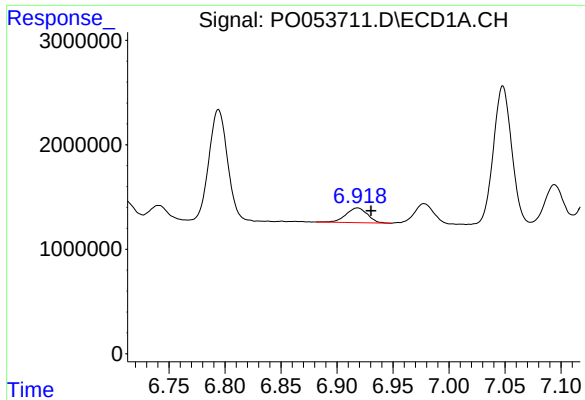

#29 AR-1254-4


R.T.: 6.918 min
Delta R.T.: -0.012 min
Response: 1873318
Conc: 36.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

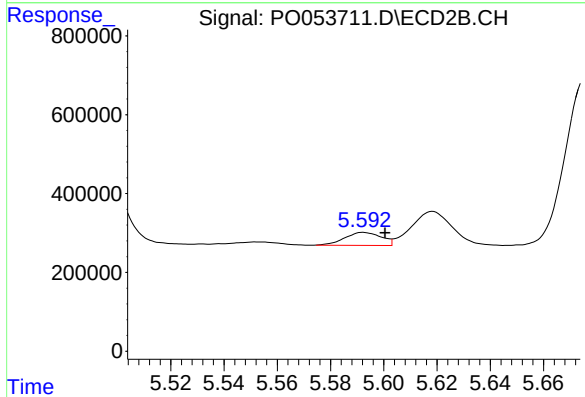


#29 AR-1254-4

R.T.: 5.592 min
Delta R.T.: -0.008 min
Response: 313932
Conc: 22.12 ng/ml

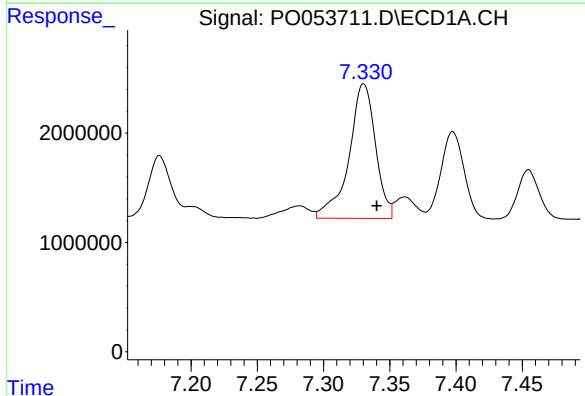


#30 AR-1254-5

R.T.: 7.330 min
Delta R.T.: -0.010 min
Response: 17172108
Conc: 358.76 ng/ml

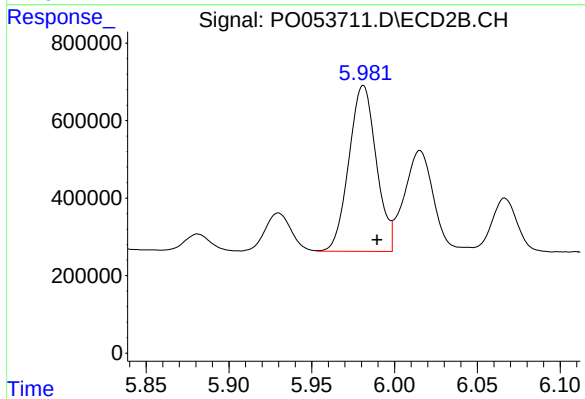

#30 AR-1254-5


R.T.: 5.981 min
Delta R.T.: -0.008 min
Response: 4932829
Conc: 264.08 ng/ml

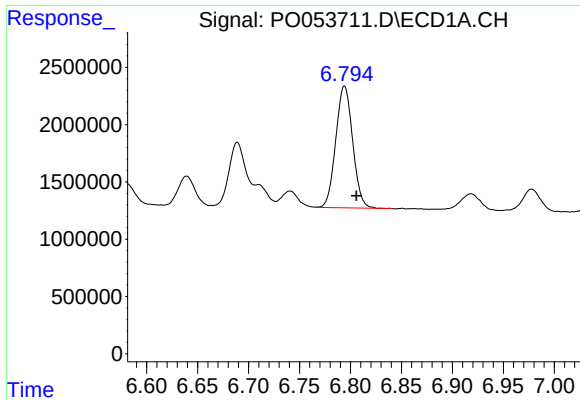

#31 AR-1260-1


R.T.: 6.794 min
Delta R.T.: -0.012 min
Response: 12277558
Conc: 251.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

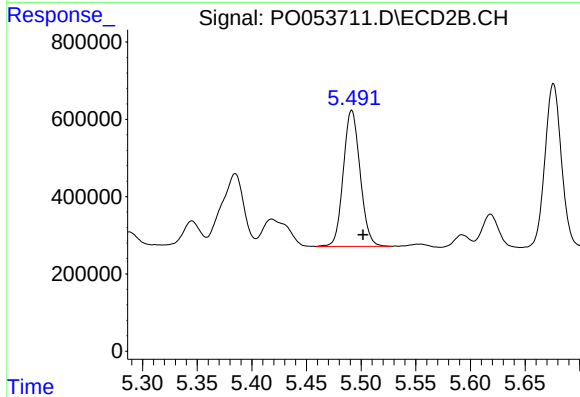


#31 AR-1260-1

R.T.: 5.491 min
Delta R.T.: -0.010 min
Response: 3771648
Conc: 247.70 ng/ml

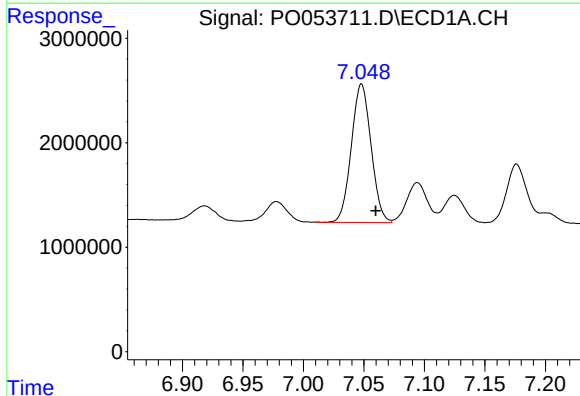


#32 AR-1260-2

R.T.: 7.048 min
Delta R.T.: -0.012 min
Response: 15078194
Conc: 242.63 ng/ml

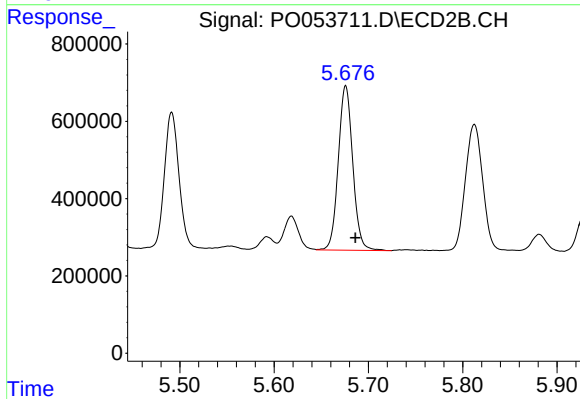

#32 AR-1260-2


R.T.: 5.676 min
Delta R.T.: -0.010 min
Response: 4536699
Conc: 244.68 ng/ml

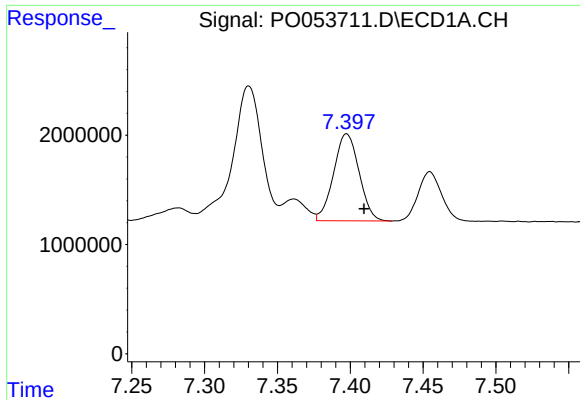

#33 AR-1260-3


R.T.: 7.398 min
Delta R.T.: -0.012 min
Response: 9708270
Conc: 248.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

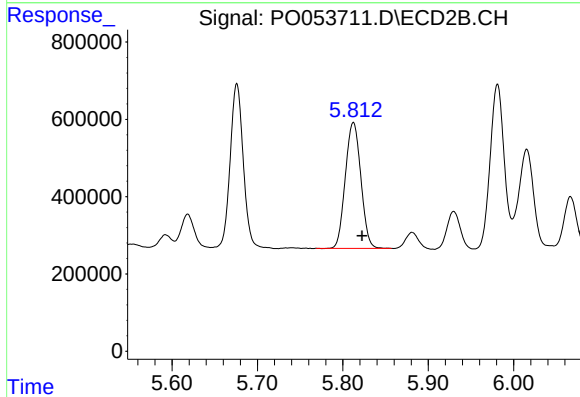


#33 AR-1260-3

R.T.: 5.812 min
Delta R.T.: -0.010 min
Response: 4118817
Conc: 240.94 ng/ml

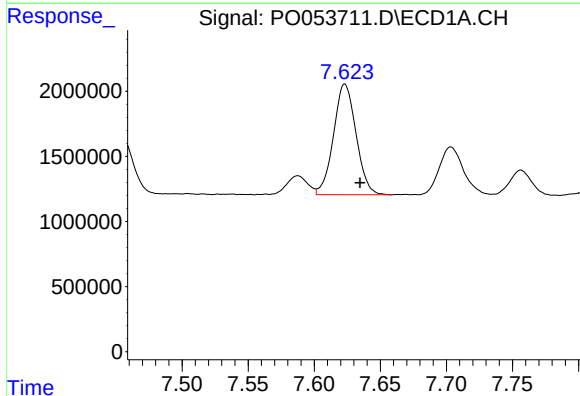


#34 AR-1260-4

R.T.: 7.623 min
Delta R.T.: -0.011 min
Response: 10105844
Conc: 233.87 ng/ml

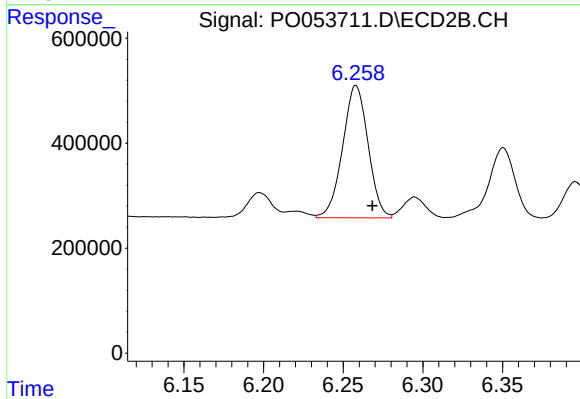

#34 AR-1260-4


R.T.: 6.258 min
Delta R.T.: -0.010 min
Response: 2804141
Conc: 254.64 ng/ml

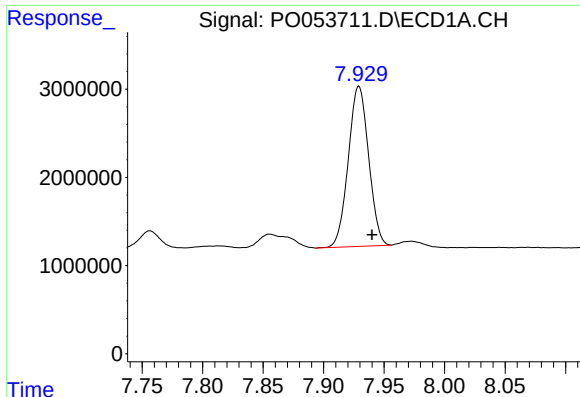

#35 AR-1260-5


R.T.: 7.929 min
Delta R.T.: -0.011 min
Response: 21245381
Conc: 233.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

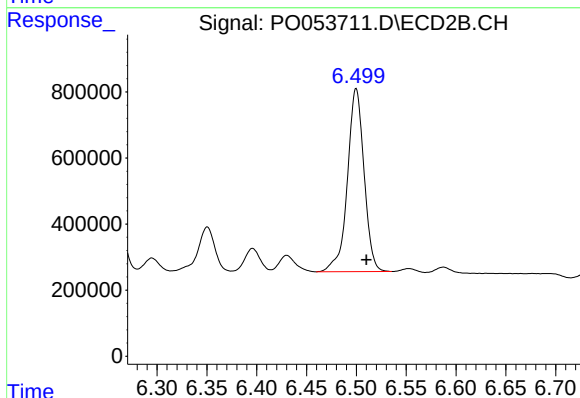


#35 AR-1260-5

R.T.: 6.500 min
Delta R.T.: -0.010 min
Response: 6453533
Conc: 236.99 ng/ml

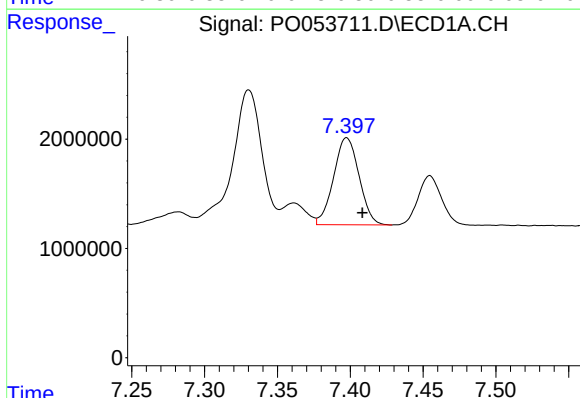


#36 AR-1262-1

R.T.: 7.398 min
Delta R.T.: -0.011 min
Response: 9708270
Conc: 141.49 ng/ml

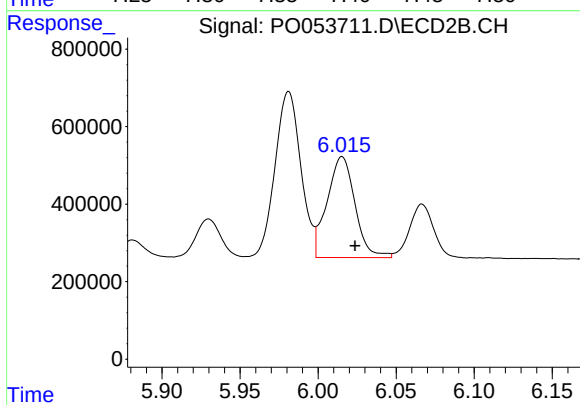

#36 AR-1262-1


R.T.: 6.015 min
Delta R.T.: -0.008 min
Response: 3243684
Conc: 163.78 ng/ml

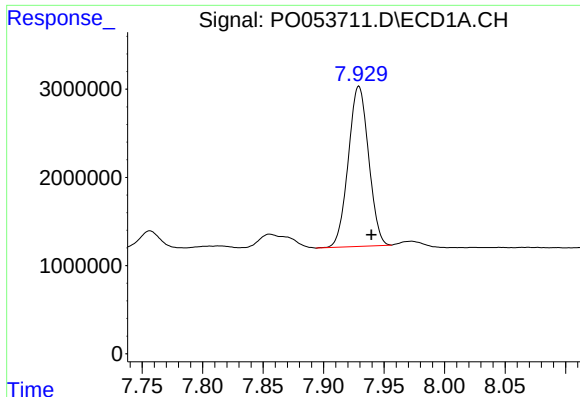

#37 AR-1262-2


R.T.: 7.929 min
Delta R.T.: -0.010 min
Response: 21245381
Conc: 176.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

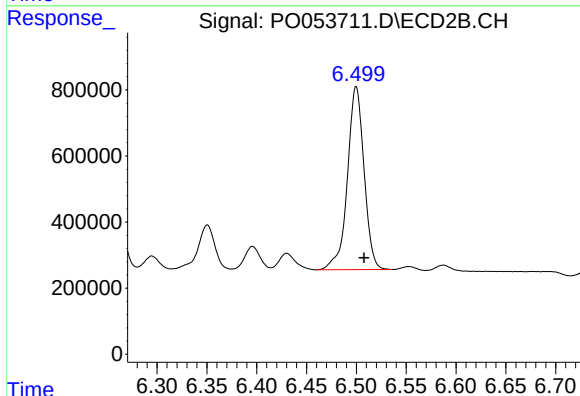


#37 AR-1262-2

R.T.: 6.500 min
Delta R.T.: -0.008 min
Response: 6453533
Conc: 190.03 ng/ml

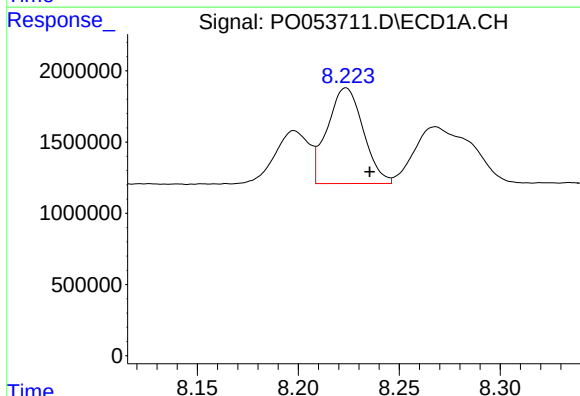


#38 AR-1262-3

R.T.: 8.224 min
Delta R.T.: -0.012 min
Response: 8348523
Conc: 338.53 ng/ml

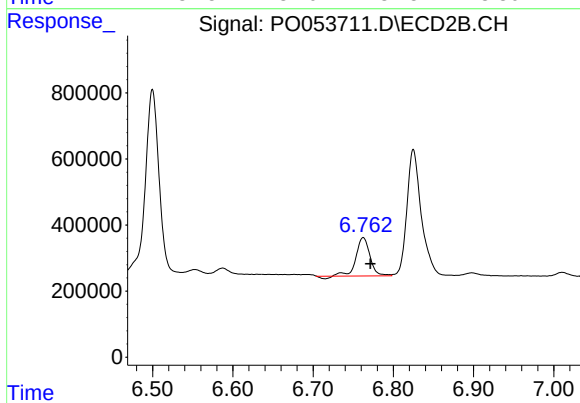

#38 AR-1262-3


R.T.: 6.763 min
Delta R.T.: -0.009 min
Response: 1377398
Conc: 105.95 ng/ml

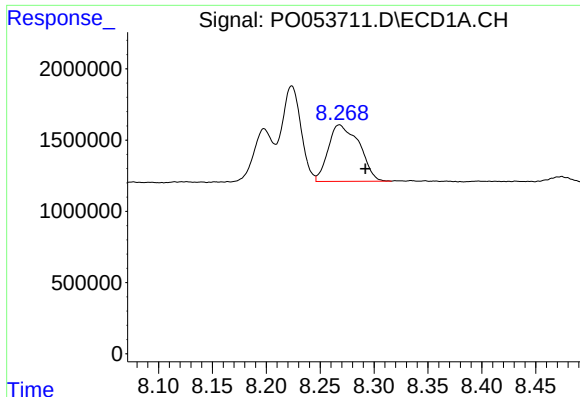

#39 AR-1262-4


R.T.: 8.268 min
Delta R.T.: -0.024 min
Response: 7930349
Conc: 127.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

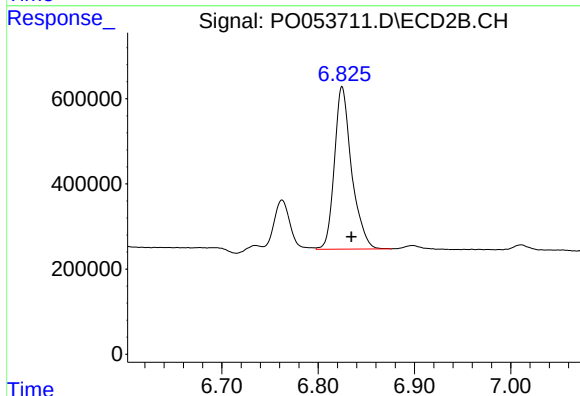


#39 AR-1262-4

R.T.: 6.825 min
Delta R.T.: -0.009 min
Response: 4738506
Conc: 193.60 ng/ml

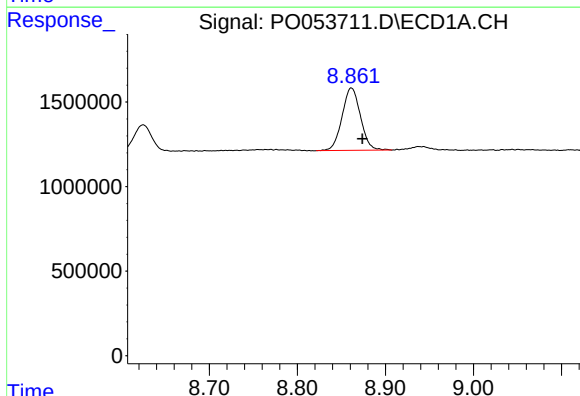


#40 AR-1262-5

R.T.: 8.861 min
Delta R.T.: -0.013 min
Response: 5352523
Conc: 126.73 ng/ml

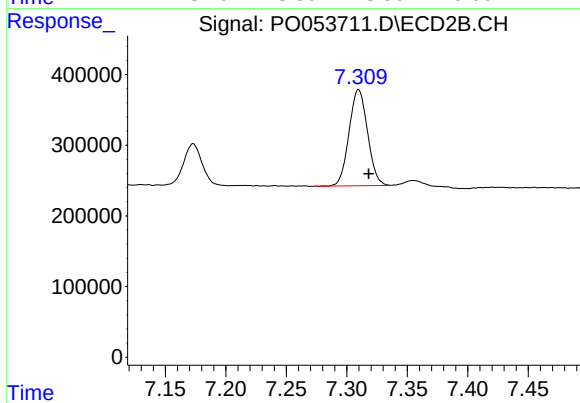

#40 AR-1262-5


R.T.: 7.310 min
Delta R.T.: -0.008 min
Response: 1448715
Conc: 129.60 ng/ml

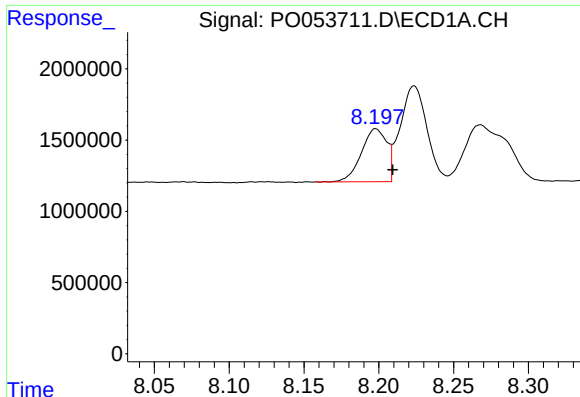

#41 AR-1268-1


R.T.: 8.198 min
Delta R.T.: -0.011 min
Response: 4396325
Conc: 29.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

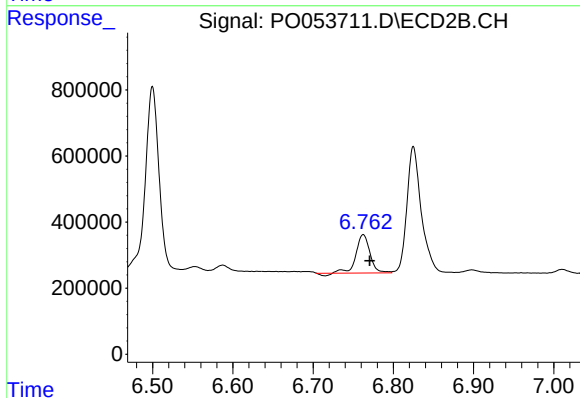


#41 AR-1268-1

R.T.: 6.763 min
Delta R.T.: -0.008 min
Response: 1377398
Conc: 35.67 ng/ml

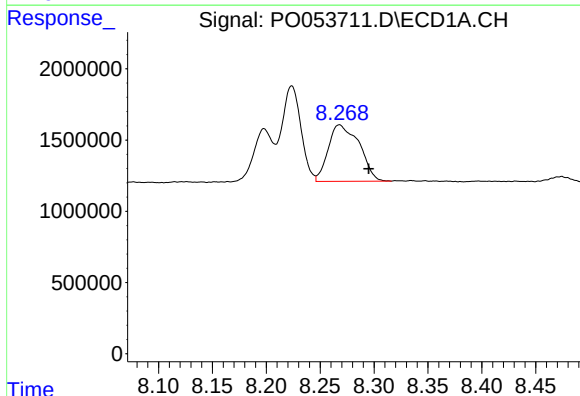


#42 AR-1268-2

R.T.: 8.268 min
Delta R.T.: -0.027 min
Response: 7930349
Conc: 56.50 ng/ml

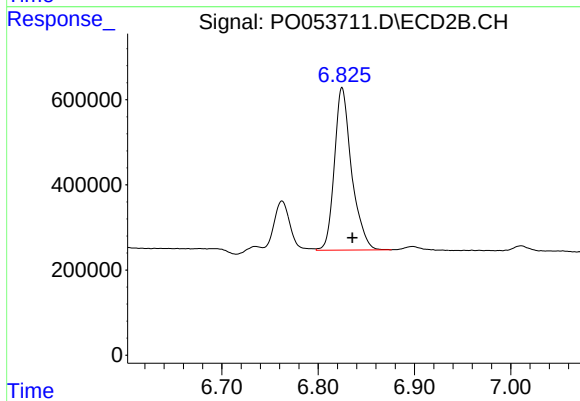

#42 AR-1268-2


R.T.: 6.825 min
Delta R.T.: -0.011 min
Response: 4738506
Conc: 129.58 ng/ml

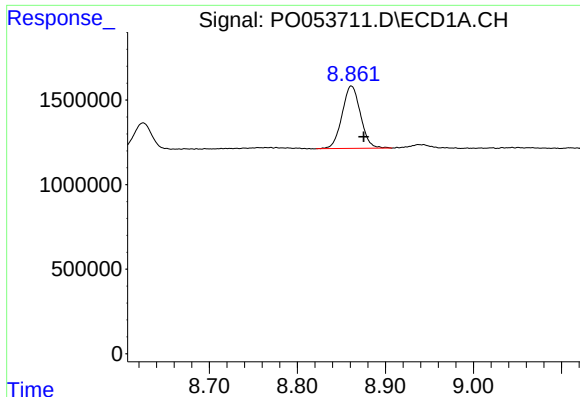

#44 AR-1268-4


R.T.: 8.861 min
Delta R.T.: -0.014 min
Response: 5352523
Conc: 112.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-005-ABCDMSD

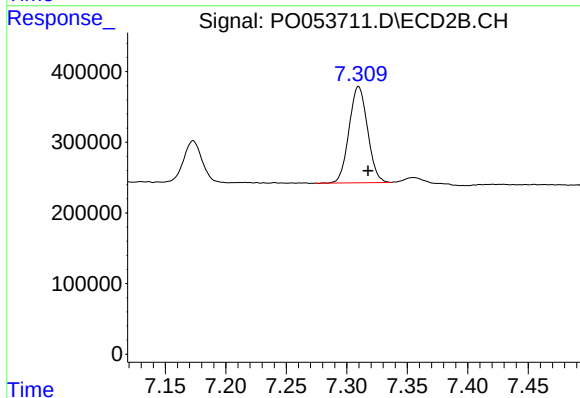


#44 AR-1268-4

R.T.: 7.310 min
Delta R.T.: -0.008 min
Response: 1448715
Conc: 116.33 ng/ml

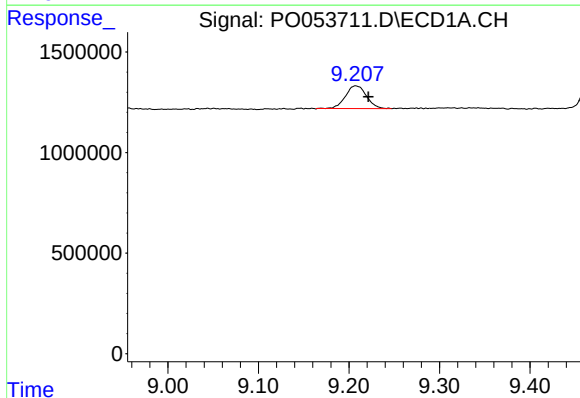

#45 AR-1268-5

R.T.: 9.207 min
Delta R.T.: -0.014 min
Response: 1804713
Conc: 4.81 ng/ml

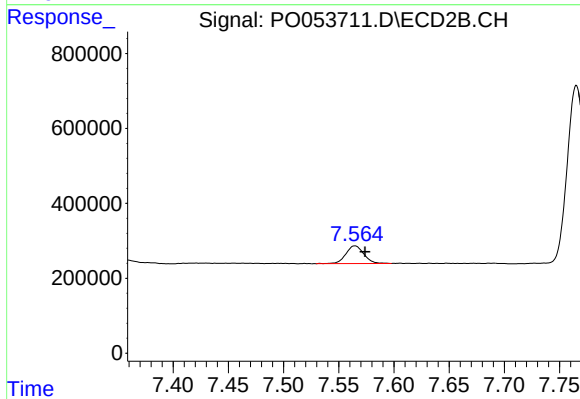

#45 AR-1268-5

R.T.: 7.565 min
Delta R.T.: -0.009 min
Response: 528023
Conc: 5.63 ng/ml