

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020419\
Data File : P0053700.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2019 15:55
Operator : SM/SJ
Sample : K1284-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-004-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 23:41:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.096	3.159	42299446	4892545	21.702	20.398
2) SA Decachlor...	9.484	7.765	18093061	4739025	18.564	18.979

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0020419\
Data File : P0053700.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Feb 2019 15:55
Operator : SM/SJ
Sample : K1284-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-004-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 23:41:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0013019.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 01 08:56:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

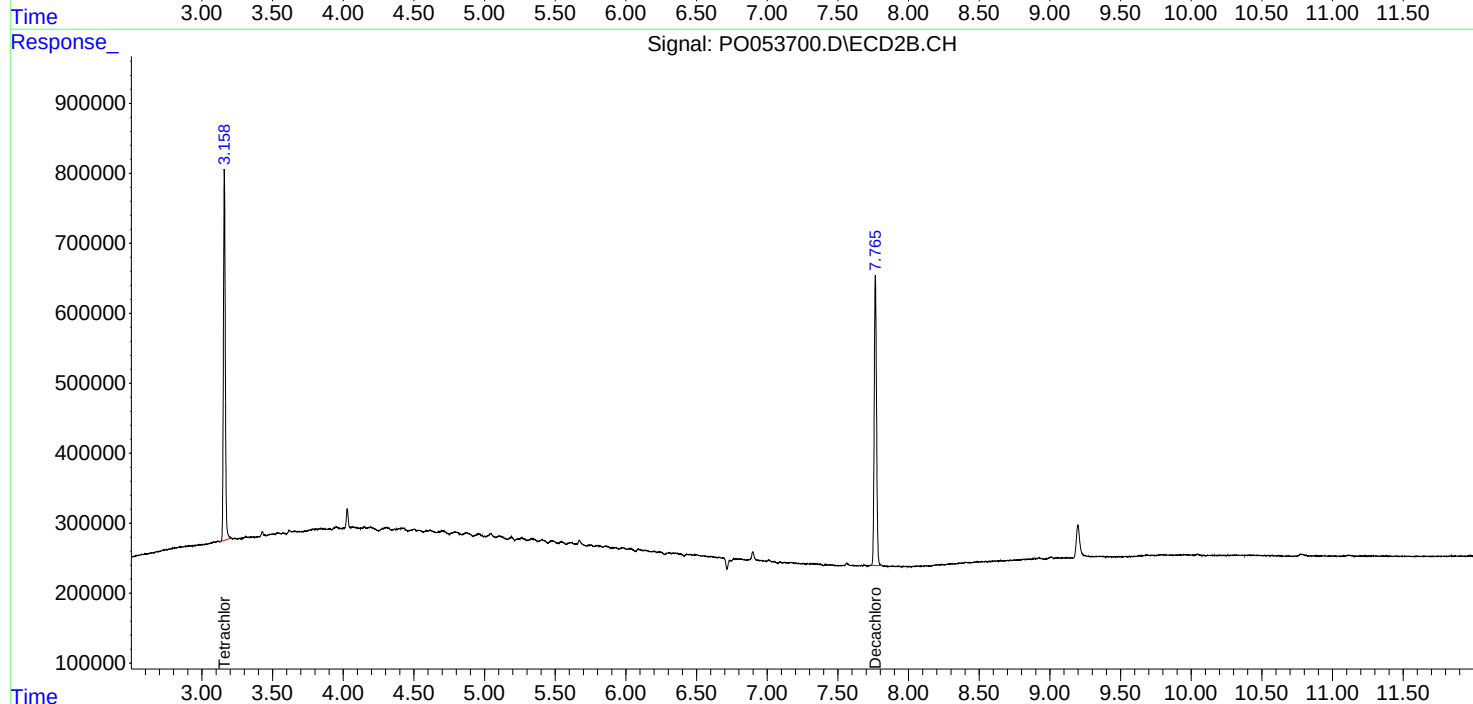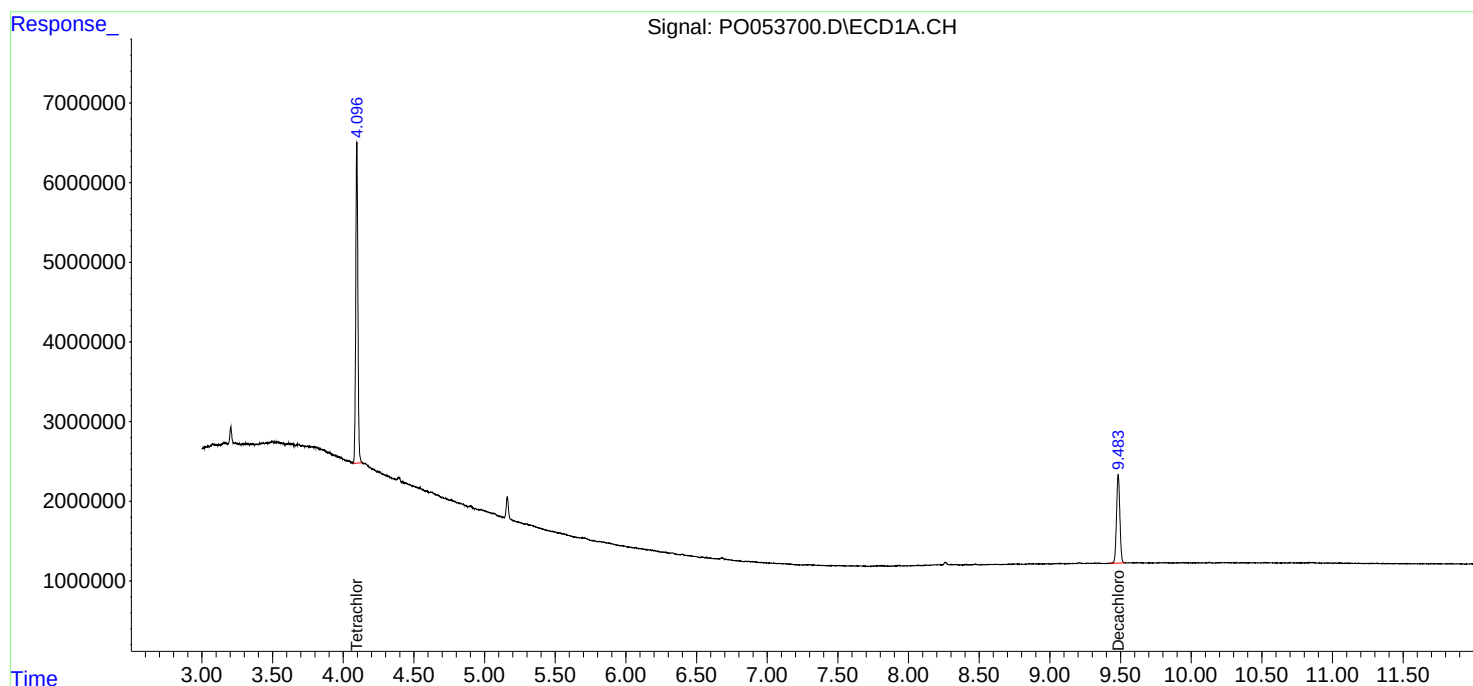


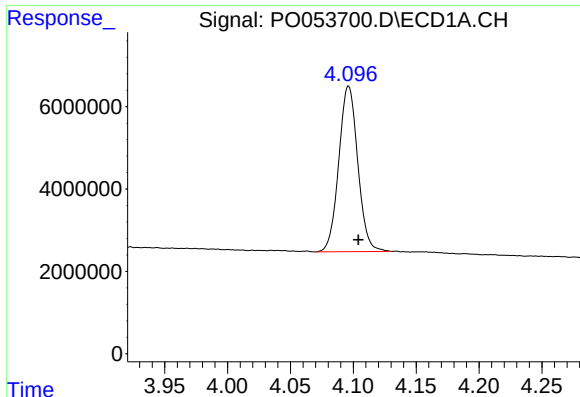

#1 Tetrachloro-m-xylene


R.T.: 4.096 min
Delta R.T.: -0.008 min
Response: 42299446
Conc: 21.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-03-004-ABCD

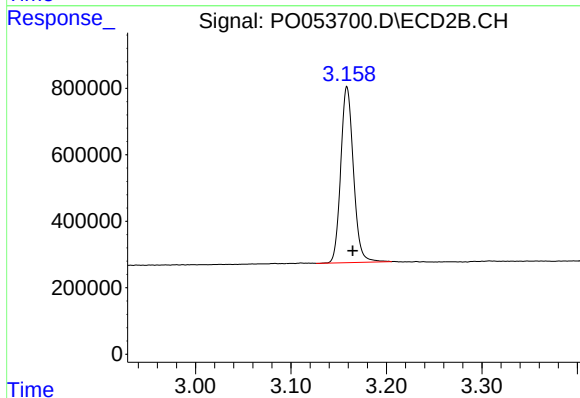


#1 Tetrachloro-m-xylene

R.T.: 3.159 min
Delta R.T.: -0.006 min
Response: 4892545
Conc: 20.40 ng/ml

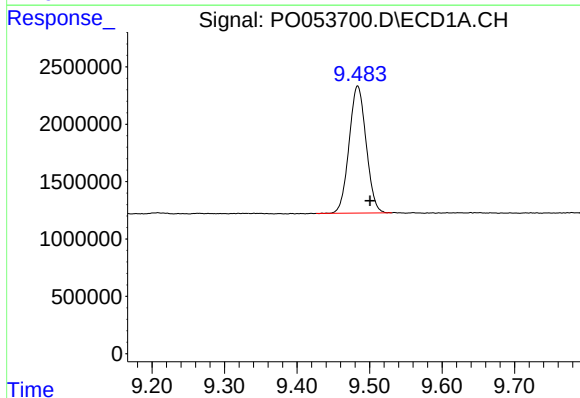

#2 Decachlorobiphenyl

R.T.: 9.484 min
Delta R.T.: -0.017 min
Response: 18093061
Conc: 18.56 ng/ml

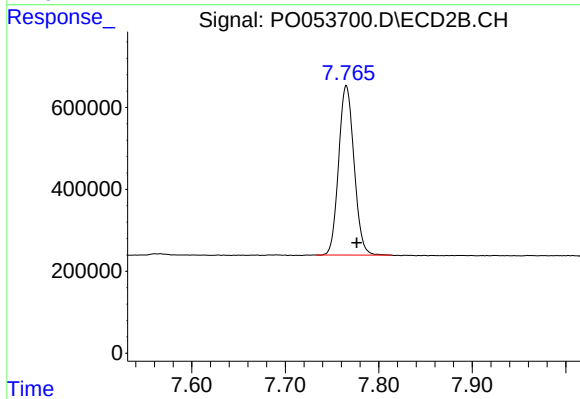

#2 Decachlorobiphenyl

R.T.: 7.765 min
Delta R.T.: -0.011 min
Response: 4739025
Conc: 18.98 ng/ml